

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072720\
Data File : FF007252.D
Signal(s) : FID2B.ch
Acq On : 27 Jul 2020 10:32
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jul 28 00:49:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.490	4121229	26.533 ug/ml
12)	N-OCTACOSANE	16.933	4033209	24.613 ug/ml
13)	N-TRIACONTANE	17.821	543250	3.286 ug/ml
14)	N-DOTRIACONTANE	18.657	512996	3.266 ug/ml
15)	N-TETRATRIACONTANE	19.444	335377	2.576 ug/ml
16)	N-HEXATRIACONTANE	20.187	218832	2.240 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072720\
Data File : FF07252.D
Signal(s) : FID2B.ch
Acq On : 27 Jul 2020 10:32
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jul 28 00:49:14 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

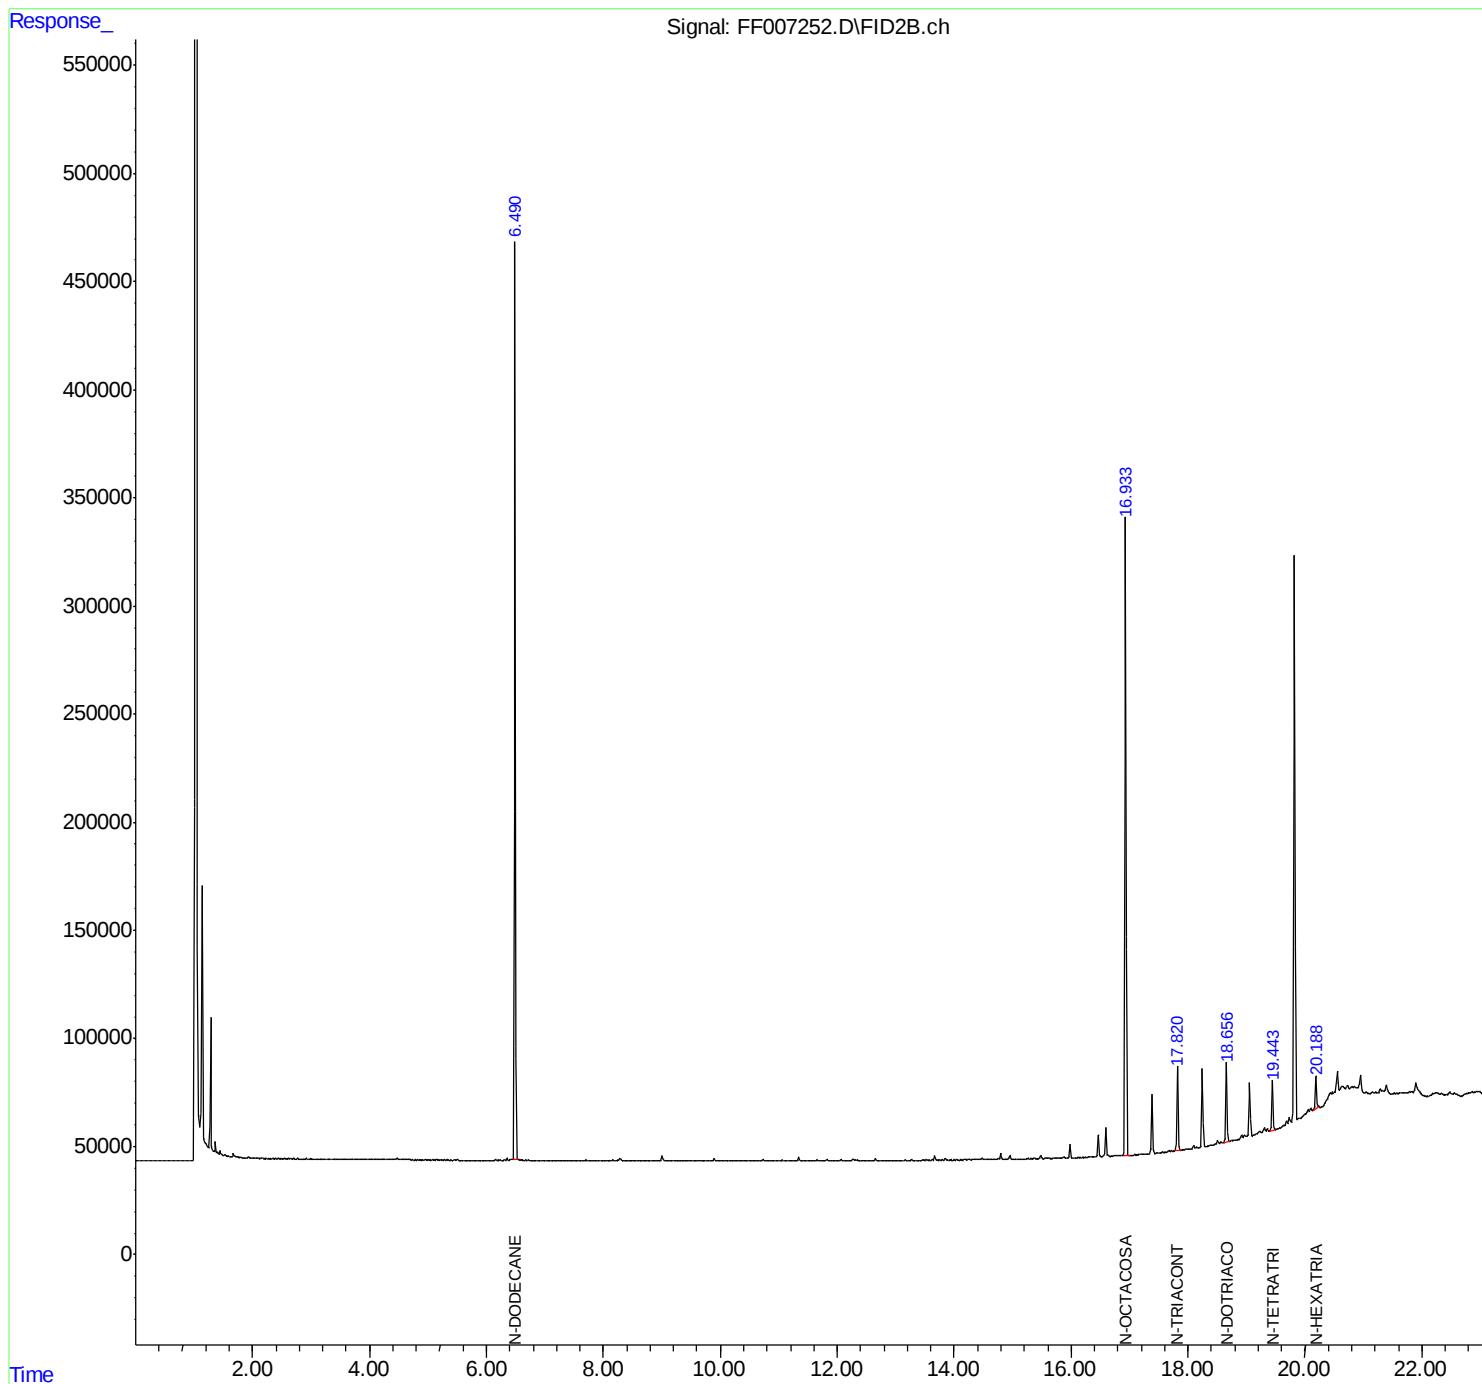


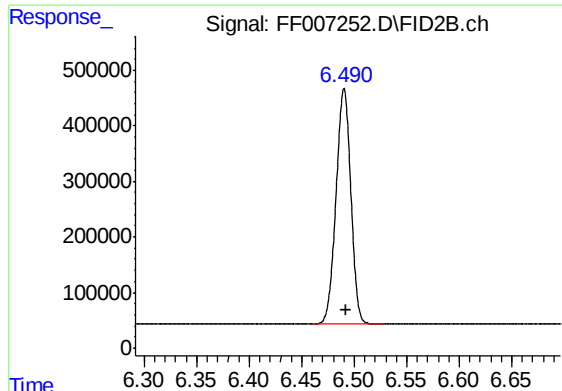

#3 N-DODECANE


R.T.: 6.490 min
Delta R.T.: -0.001 min
Response: 4121229
Conc: 26.53 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

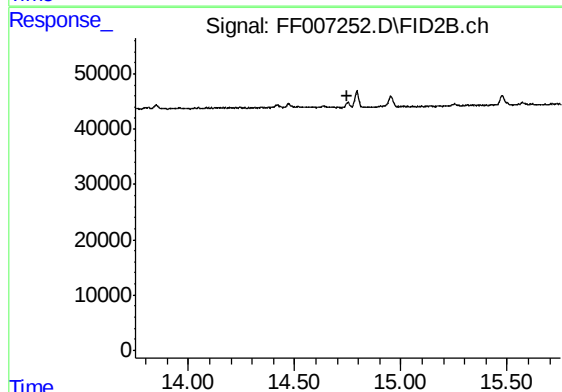


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.751 min
Response: 0
Conc: N.D.

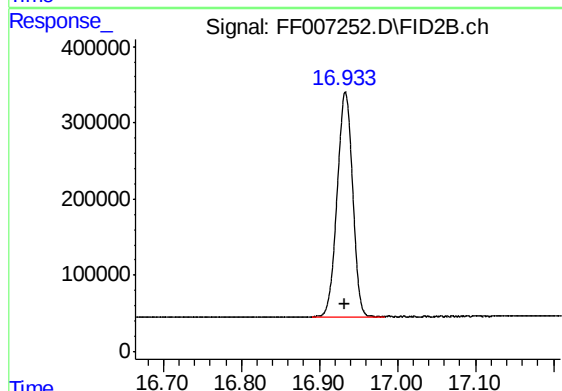


#12 N-OCTACOSANE

R.T.: 16.933 min
Delta R.T.: 0.000 min
Response: 4033209
Conc: 24.61 ug/ml

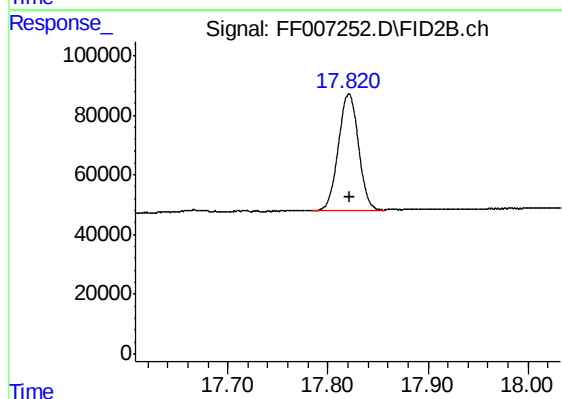

#13 N-TRIACONTANE


R.T.: 17.821 min
Delta R.T.: -0.001 min
Response: 543250
Conc: 3.29 ug/ml

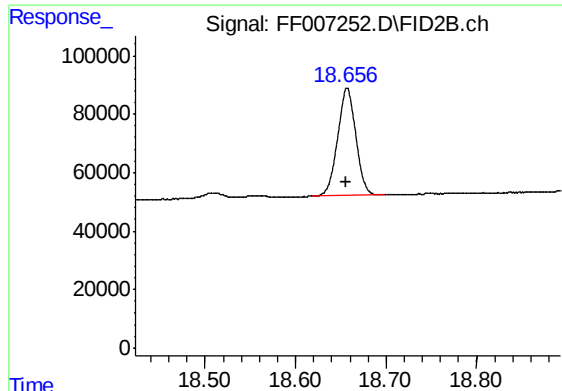

#14 N-DOTRIACONTANE


R.T.: 18.657 min
Delta R.T.: 0.000 min
Response: 512996
Conc: 3.27 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

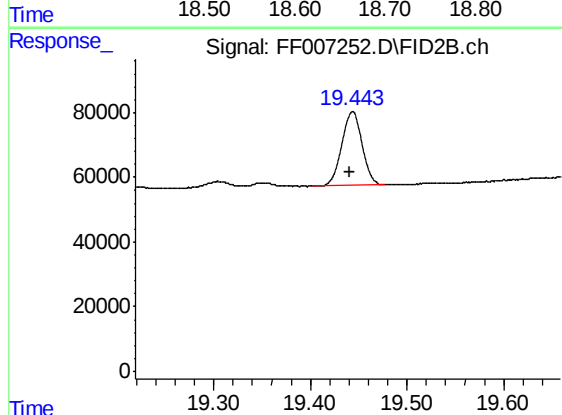

#15 N-TETRATRIACONTANE

R.T.: 19.444 min
Delta R.T.: 0.003 min
Response: 335377
Conc: 2.58 ug/ml

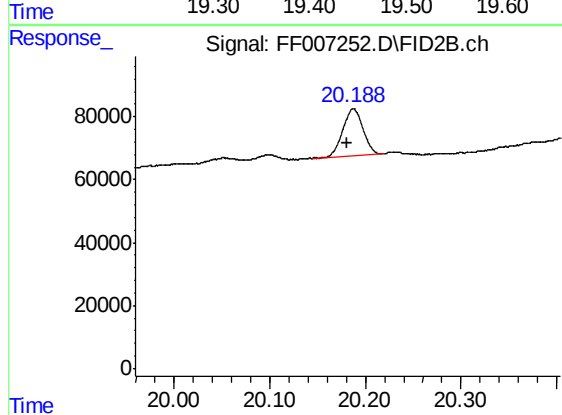

#16 N-HEXATRIACONTANE

R.T.: 20.187 min
Delta R.T.: 0.007 min
Response: 218832
Conc: 2.24 ug/ml