

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072720\
 Data File : FF007254.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jul 2020 11:41
 Operator : DD\AJ
 Sample : L3418-04 2X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 C0AF1

Integration File: autoint1.e
 Quant Time: Jul 28 00:49:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.752	1523997	10.810 ug/ml
Target Compounds			
3) N-DODECANE	6.444	148602	0.957 ug/ml
4) N-TETRADECANE	8.348f	358151	2.313 ug/ml
8) N-DOCOSANE	13.813	479576	2.957 ug/ml
10) N-TETRACOSANE	14.978	1499270	9.155 ug/ml
11) N-HEXACOSANE	16.042f	261434	1.608 ug/ml
14) N-DOTRIACONTANE	18.652	568847	3.622 ug/ml
15) N-TETRATRIACONTANE	19.446	560139	4.303 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072720\
Data File : FF07254.D
Signal(s) : FID2B.ch
Acq On : 27 Jul 2020 11:41
Operator : DD\AJ
Sample : L3418-04 2X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
C0AF1

Integration File: autoint1.e
Quant Time: Jul 28 00:49:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

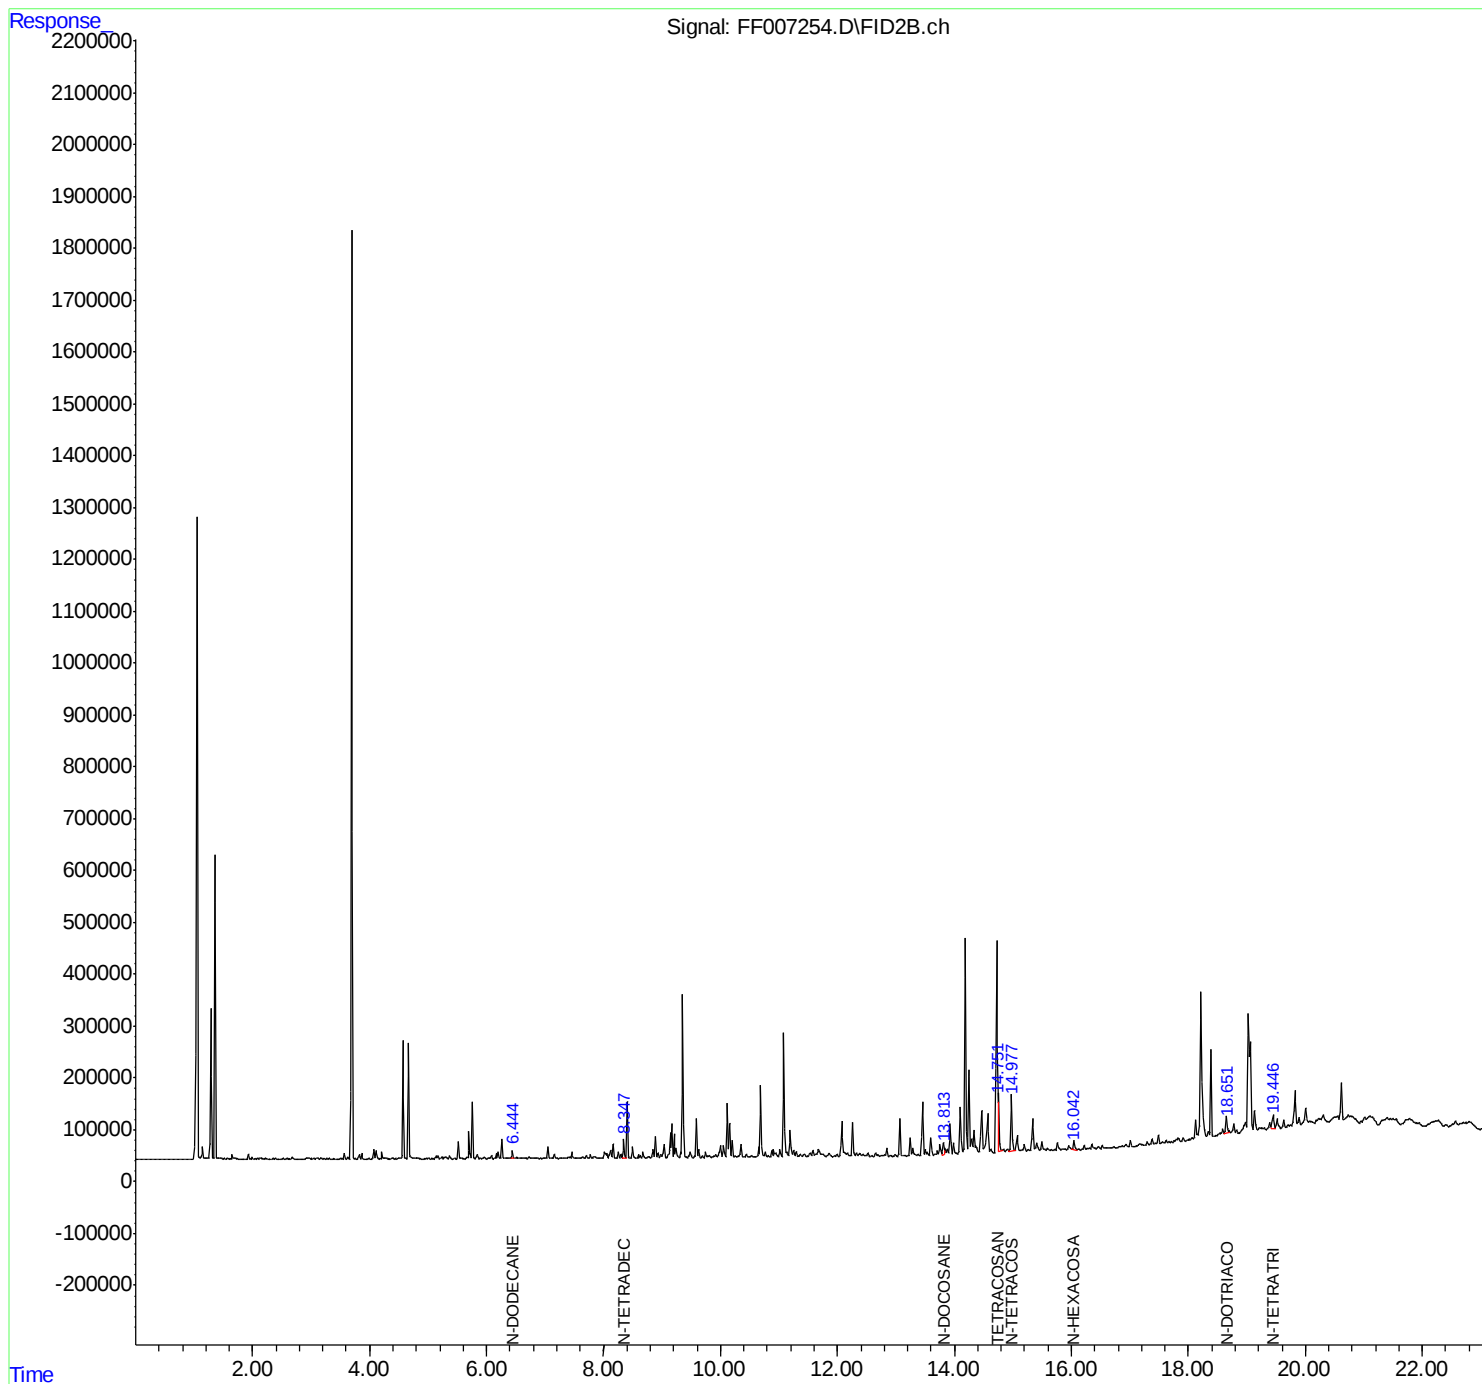


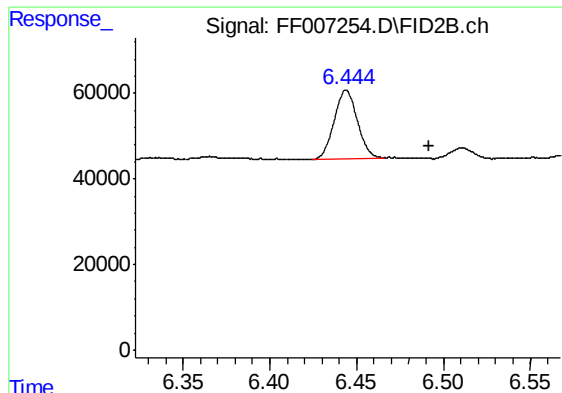

#3 N-DODECANE


R.T.: 6.444 min
Delta R.T.: -0.048 min
Response: 148602
Conc: 0.96 ug/ml

Instrument :
FID_F
ClientSampleId :
C0AF1

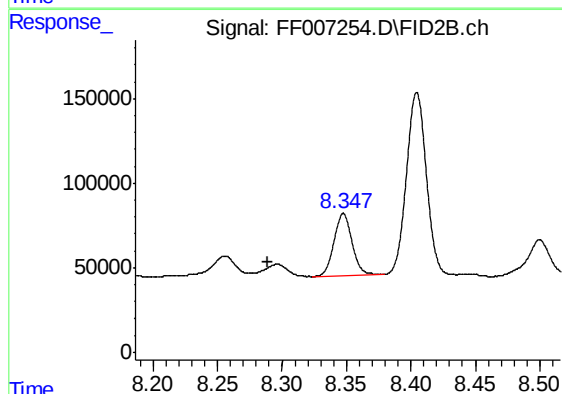


#4 N-TETRADECANE

R.T.: 8.348 min
Delta R.T.: 0.059 min
Response: 358151
Conc: 2.31 ug/ml

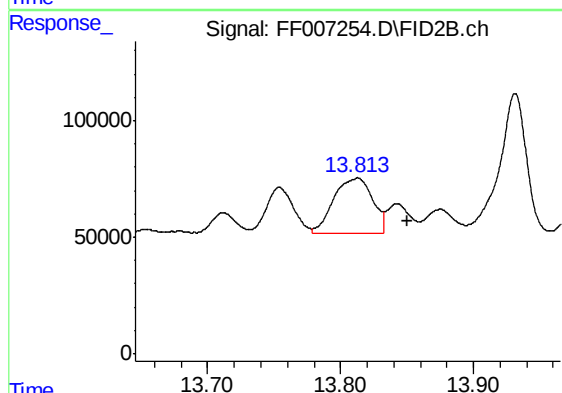


#8 N-DOCOSANE

R.T.: 13.813 min
Delta R.T.: -0.037 min
Response: 479576
Conc: 2.96 ug/ml

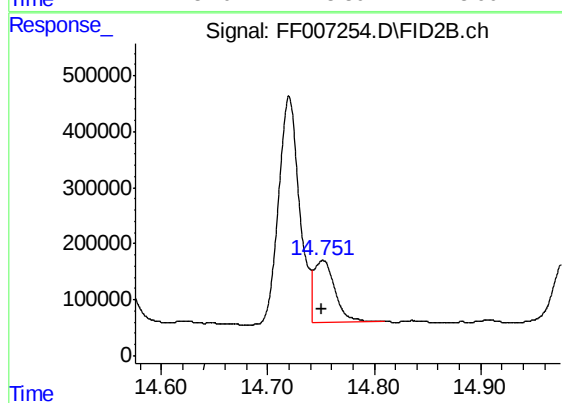

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.752 min
Delta R.T.: 0.001 min
Response: 1523997
Conc: 10.81 ug/ml

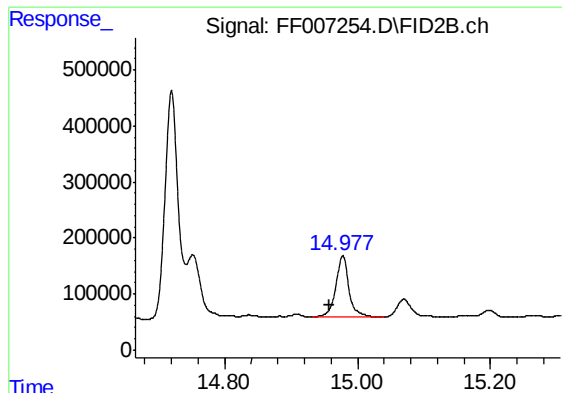

#10 N-TETRACOSANE


R.T.: 14.978 min
Delta R.T.: 0.021 min
Response: 1499270
Conc: 9.15 ug/ml

Instrument :
FID_F
ClientSampleId :
C0AF1

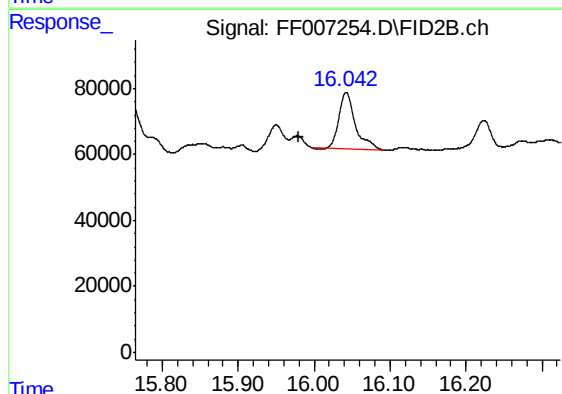


#11 N-HEXACOSANE

R.T.: 16.042 min
Delta R.T.: 0.063 min
Response: 261434
Conc: 1.61 ug/ml

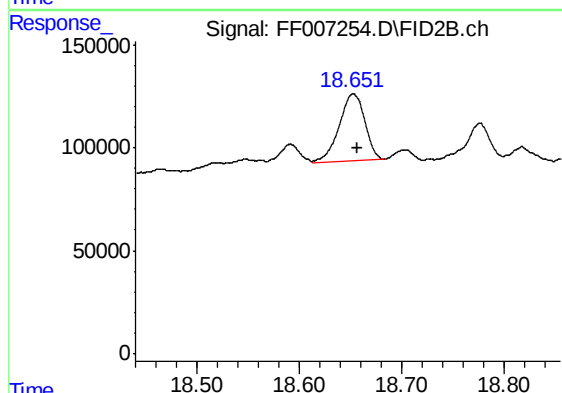

#14 N-DOTRIACONTANE

R.T.: 18.652 min
Delta R.T.: -0.004 min
Response: 568847
Conc: 3.62 ug/ml

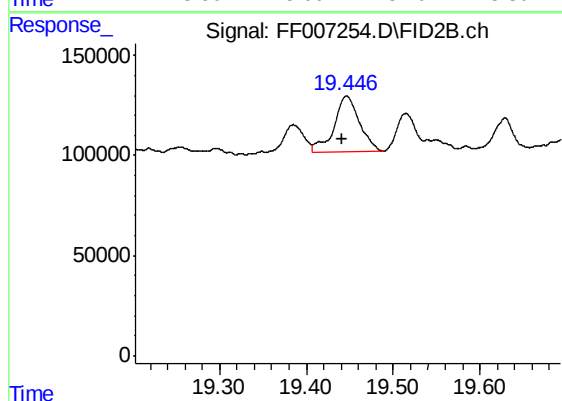

#15 N-TETRATRIACONTANE

R.T.: 19.446 min
Delta R.T.: 0.006 min
Response: 560139
Conc: 4.30 ug/ml