

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072720\
 Data File : FF07251.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jul 2020 10:01
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: Sample.e
 Quant Time: Jul 28 00:48:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
 Quant Title :
 QLast Update : Thu Jul 16 09:27:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.756	6948735	49.290 ug/ml
Target Compounds			
2) N-DECANE	4.465	8252447	53.650 ug/ml
3) N-DODECANE	6.493	8322888	53.583 ug/ml
4) N-TETRADECANE	8.290	8305263	53.639 ug/ml
5) N-HEXADECANE	9.894	8313681	52.733 ug/ml
6) N-OCTADECANE	11.339	8404891	52.143 ug/ml
7) N-EICOSANE	12.652	8280018	51.272 ug/ml
8) N-DOCOSANE	13.854	8123156	50.090 ug/ml
10) N-TETRACOSANE	14.960	7977459	48.711 ug/ml
11) N-HEXACOSANE	15.984	7663298	47.129 ug/ml
12) N-OCTACOSANE	16.937	7484610	45.676 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072720\
Data File : FF007251.D
Signal(s) : FID2B.ch
Acq On : 27 Jul 2020 10:01
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: Sample.e
Quant Time: Jul 28 00:48:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF071520.M
Quant Title :
QLast Update : Thu Jul 16 09:27:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

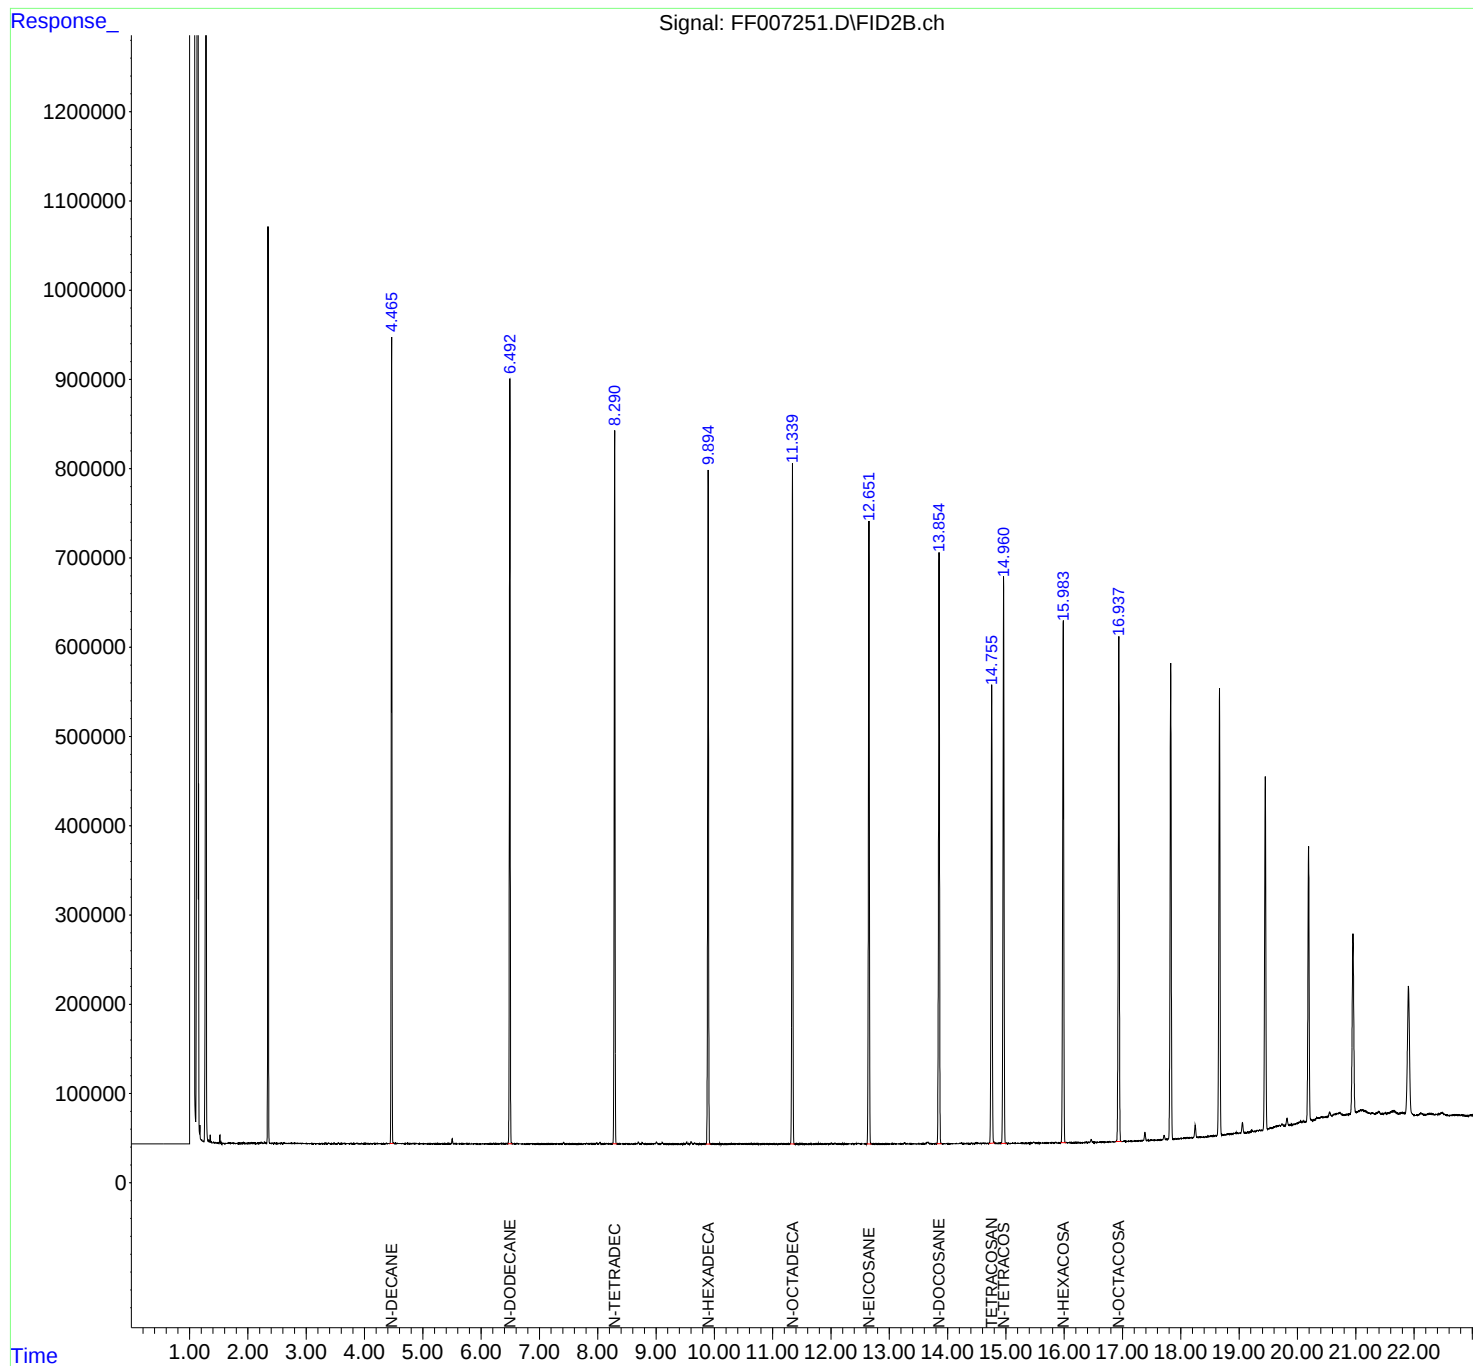


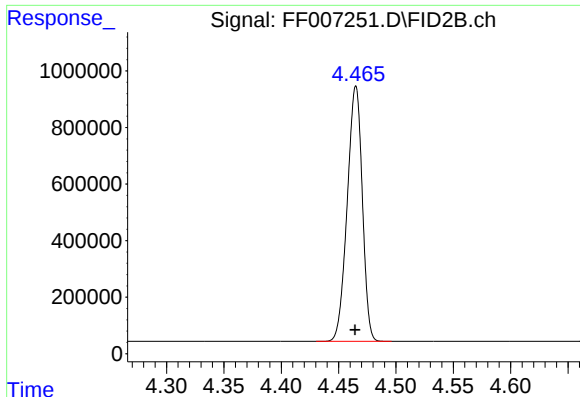

#2 N-DECANE


R.T.: 4.465 min
Delta R.T.: 0.000 min
Response: 8252447
Conc: 53.65 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

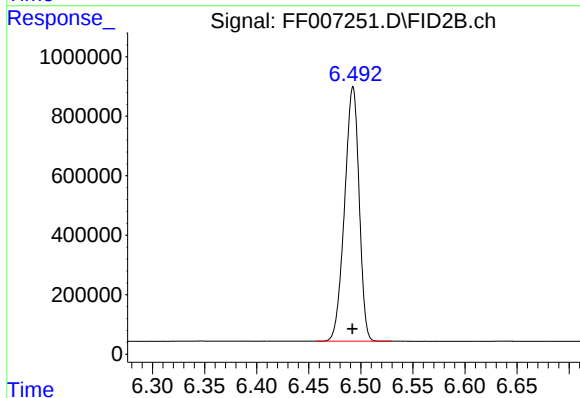


#3 N-DODECANE

R.T.: 6.493 min
Delta R.T.: 0.000 min
Response: 8322888
Conc: 53.58 ug/ml

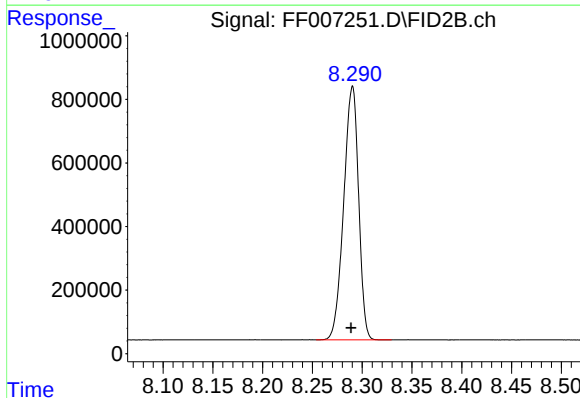


#4 N-TETRADECANE

R.T.: 8.290 min
Delta R.T.: 0.002 min
Response: 8305263
Conc: 53.64 ug/ml

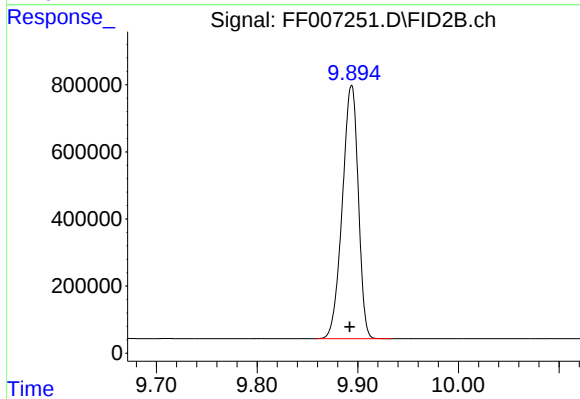

#5 N-HEXADECANE


R.T.: 9.894 min
Delta R.T.: 0.002 min
Response: 8313681
Conc: 52.73 ug/ml

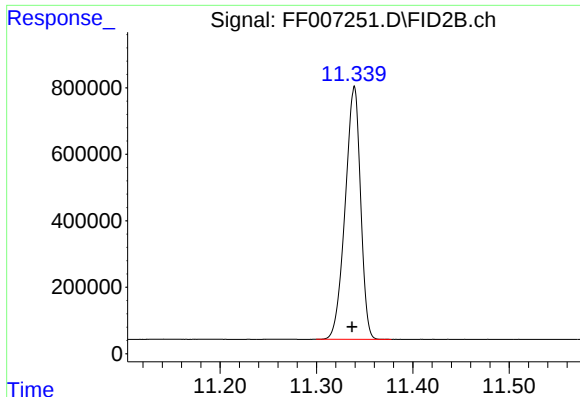

#6 N-OCTADECANE


R.T.: 11.339 min
Delta R.T.: 0.002 min
Response: 8404891
Conc: 52.14 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

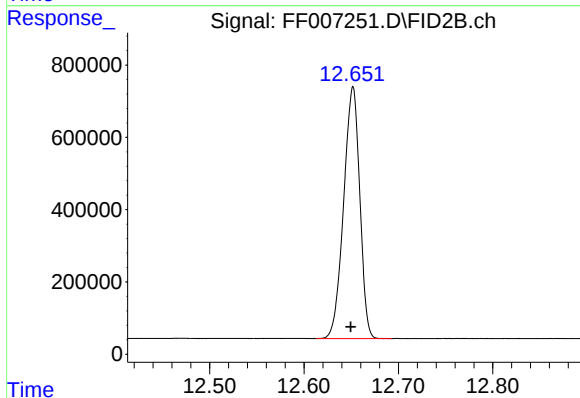


#7 N-EICOSANE

R.T.: 12.652 min
Delta R.T.: 0.002 min
Response: 8280018
Conc: 51.27 ug/ml

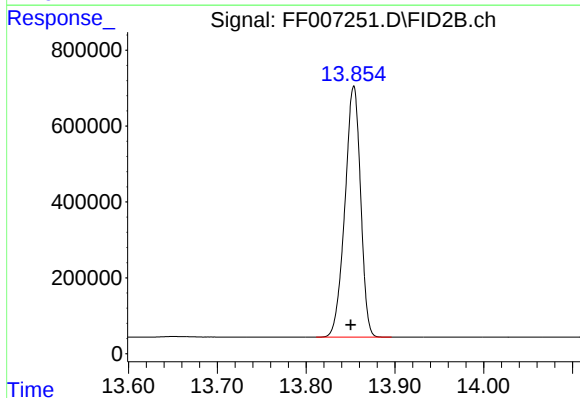


#8 N-DOCOSANE

R.T.: 13.854 min
Delta R.T.: 0.003 min
Response: 8123156
Conc: 50.09 ug/ml

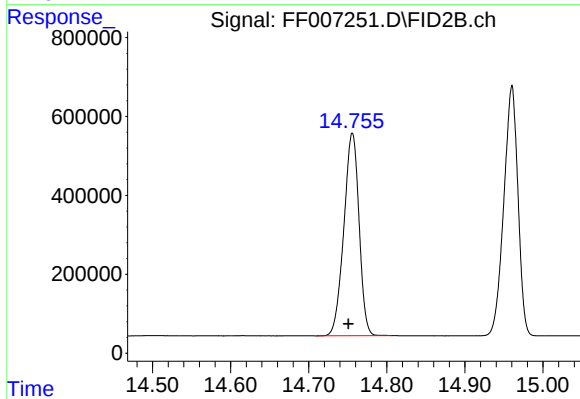

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.756 min
Delta R.T.: 0.005 min
Response: 6948735
Conc: 49.29 ug/ml

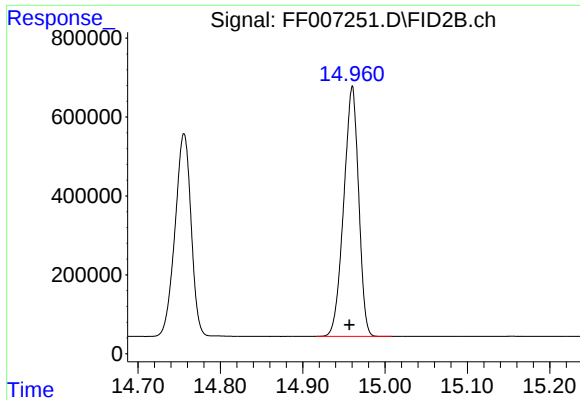

#10 N-TETRACOSANE


R.T.: 14.960 min
Delta R.T.: 0.003 min
Response: 7977459
Conc: 48.71 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

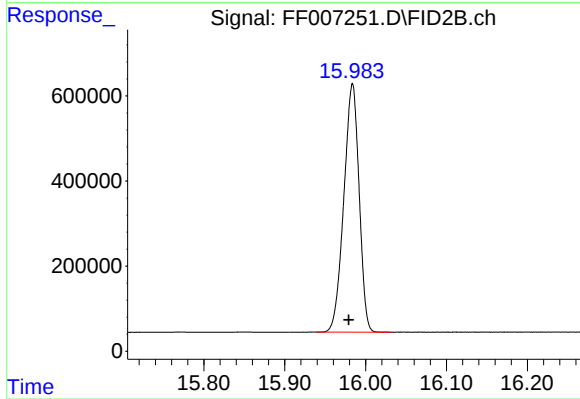

#11 N-HEXACOSANE

R.T.: 15.984 min
Delta R.T.: 0.005 min
Response: 7663298
Conc: 47.13 ug/ml

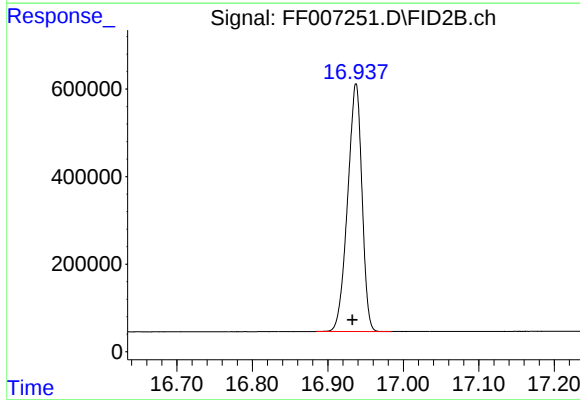

#12 N-OCTACOSANE

R.T.: 16.937 min
Delta R.T.: 0.005 min
Response: 7484610
Conc: 45.68 ug/ml