

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072822\
Data File : FF011118.D
Signal(s) : FID2B.ch
Acq On : 28 Jul 2022 11:48
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 28 15:12:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.801	2747668	25.280 ug/ml
Target Compounds			
18) N-TETRACONTANE	21.775	259320	2.366 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF072822\
Data File : FF011118.D
Signal(s) : FID2B.ch
Acq On : 28 Jul 2022 11:48
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 28 15:12:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

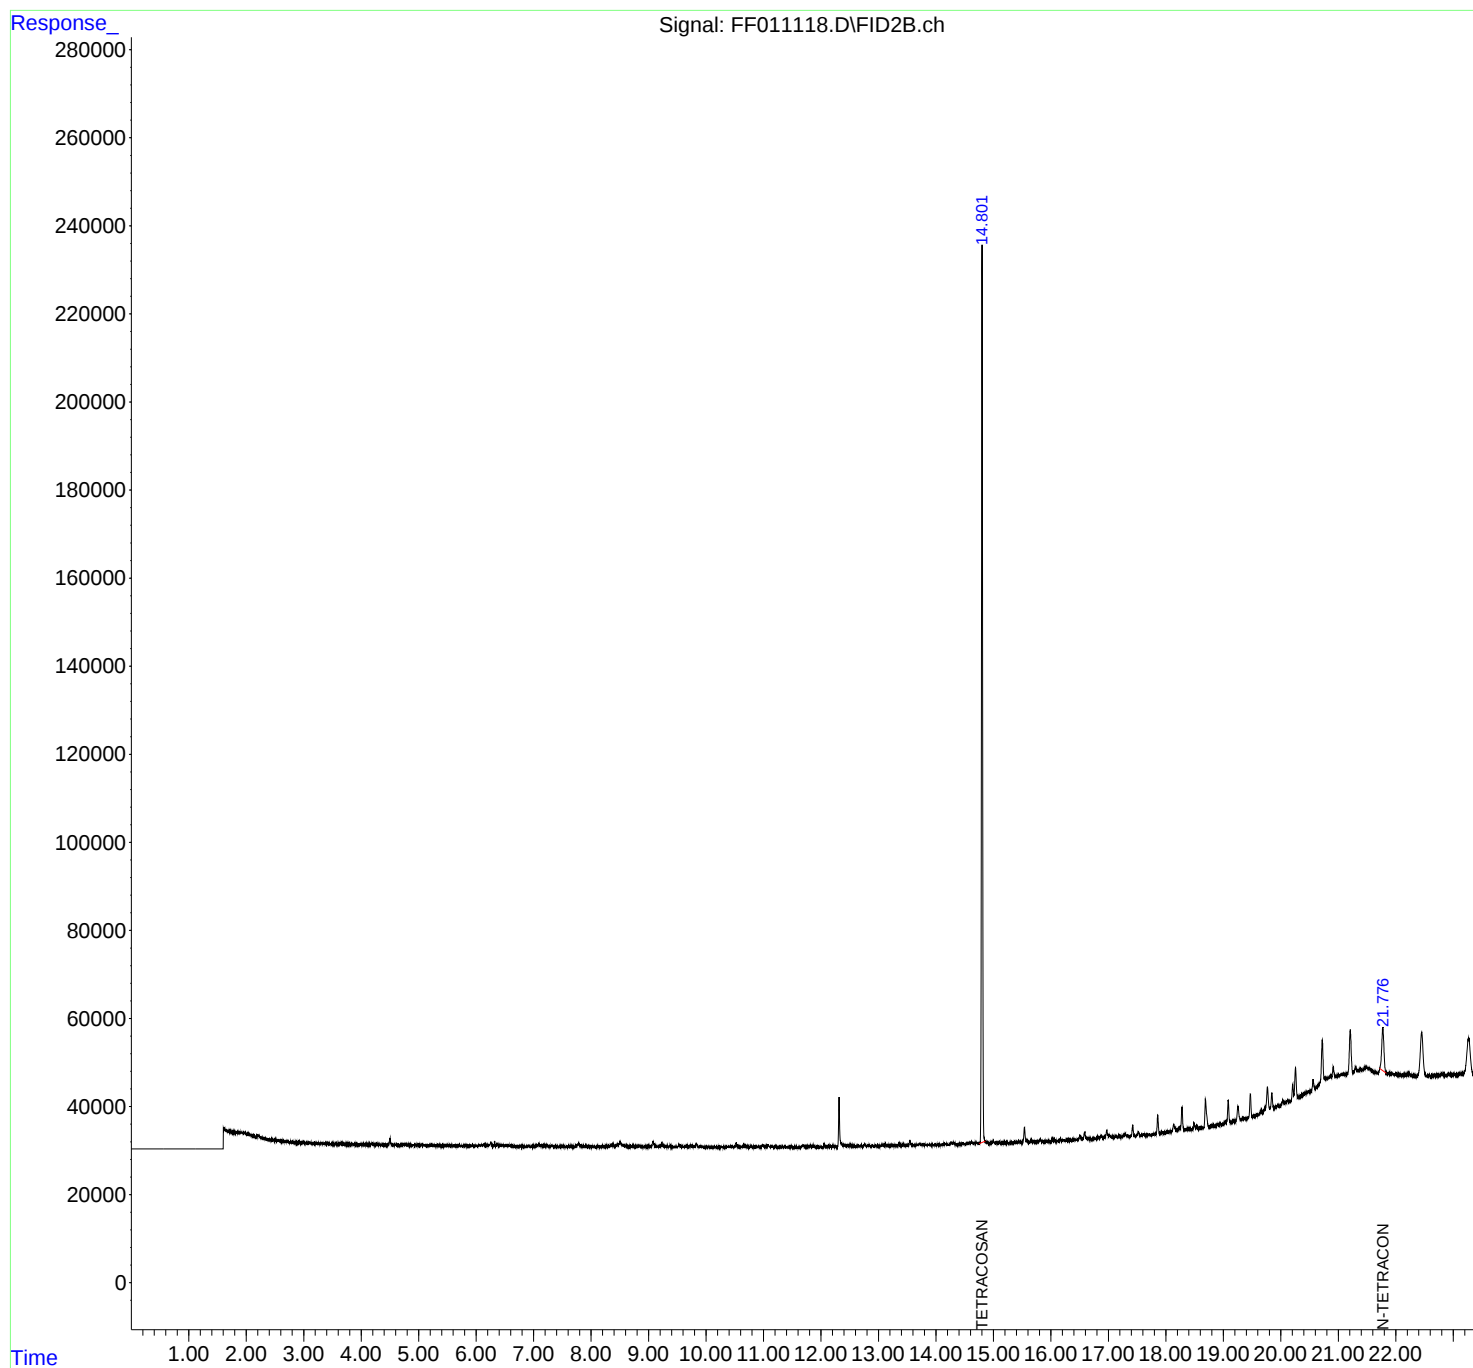


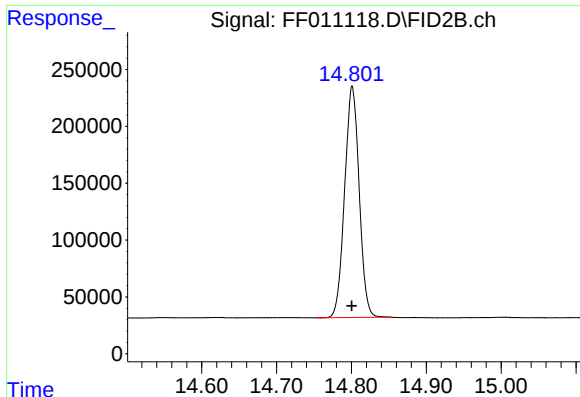

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.801 min
Delta R.T.: 0.000 min
Response: 2747668
Conc: 25.28 ug/ml

Instrument :
FID_F
ClientSampleId :

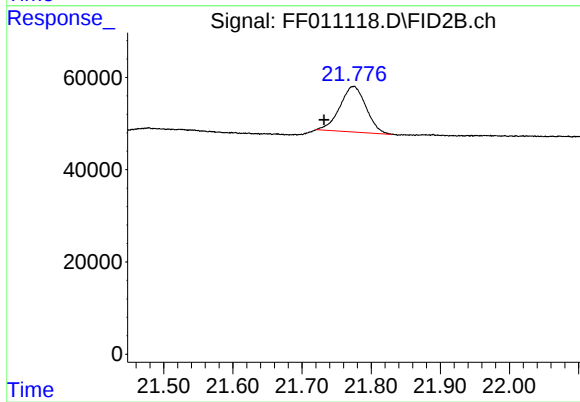

#18 N-TETRACONTANE

R.T.: 21.775 min
Delta R.T.: 0.043 min
Response: 259320
Conc: 2.37 ug/ml