

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF073118\
 Data File : FF001580.D
 Signal(s) : FID2B.ch
 Acq On : 31 Jul 2018 18:06
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 01 02:09:46 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Mon Jul 30 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.329	6541573	52.062 ug/ml
Target Compounds			
2) N-DECANE	4.121	7709356	52.279 ug/ml
3) N-DODECANE	6.125	7801612	52.087 ug/ml
4) N-TETRADECANE	7.909	7771342	51.656 ug/ml
5) N-HEXADECANE	9.501	7724604	51.726 ug/ml
6) N-OCTADECANE	10.936	7695679	51.487 ug/ml
7) N-EICOSANE	12.239	7596592	51.435 ug/ml
8) N-DOCOSANE	13.433	7507790	51.788 ug/ml
10) N-TETRACOSANE	14.531	7367751	51.971 ug/ml
11) N-HEXACOSANE	15.548	7266893	51.922 ug/ml
12) N-OCTACOSANE	16.494	7194772	51.852 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF073118\
Data File : FF001580.D
Signal(s) : FID2B.ch
Acq On : 31 Jul 2018 18:06
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 01 02:09:46 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Mon Jul 30 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

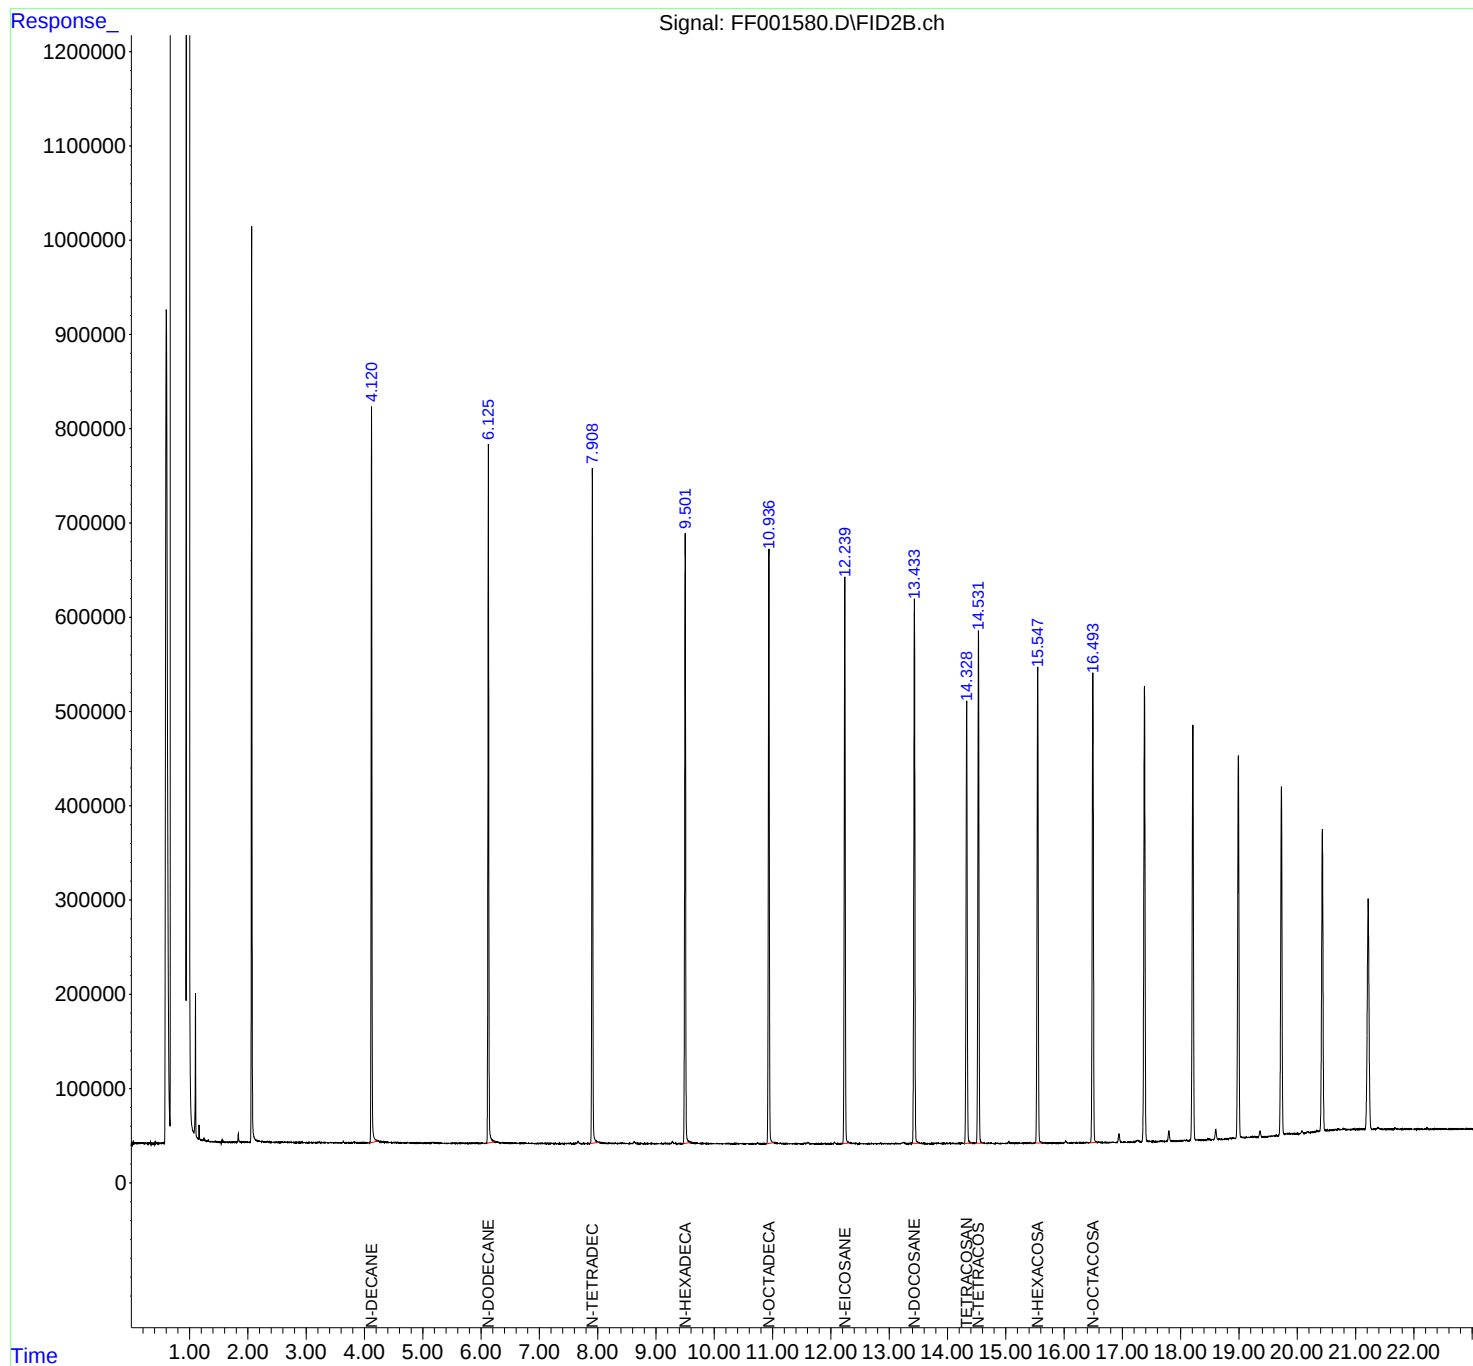

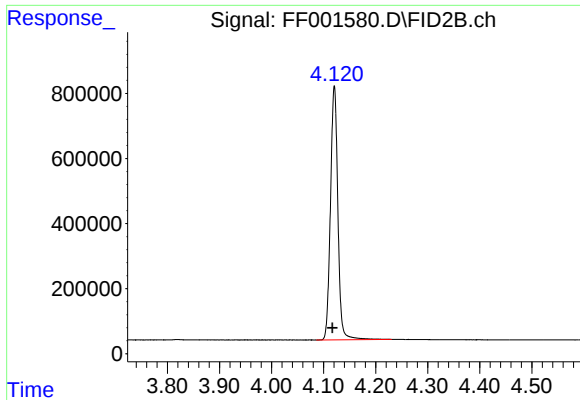


#2 N-DECANE

R.T.: 4.121 min
Delta R.T.: 0.004 min
Response: 7709356
Conc: 52.28 ug/ml

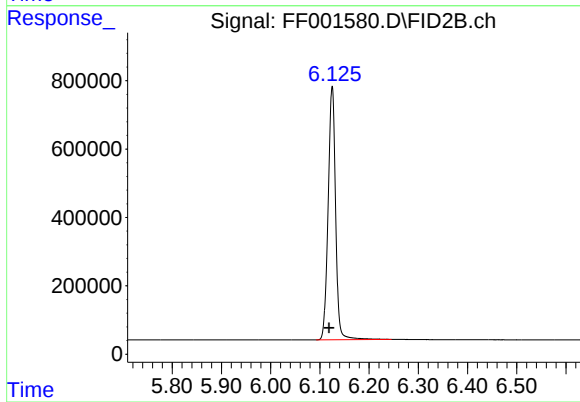


#3 N-DODECANE

R.T.: 6.125 min
Delta R.T.: 0.006 min
Response: 7801612
Conc: 52.09 ug/ml

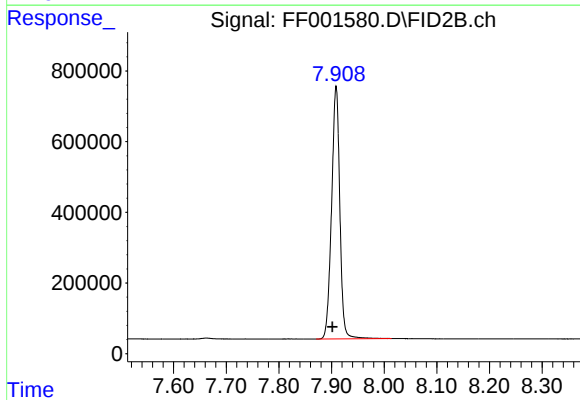


#4 N-TETRADECANE

R.T.: 7.909 min
Delta R.T.: 0.007 min
Response: 7771342
Conc: 51.66 ug/ml

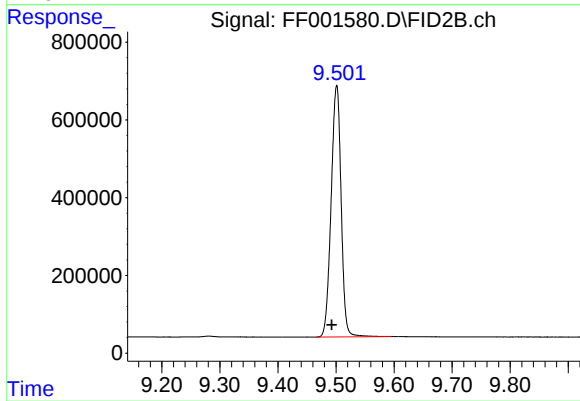


#5 N-HEXADECANE

R.T.: 9.501 min
Delta R.T.: 0.009 min
Response: 7724604
Conc: 51.73 ug/ml

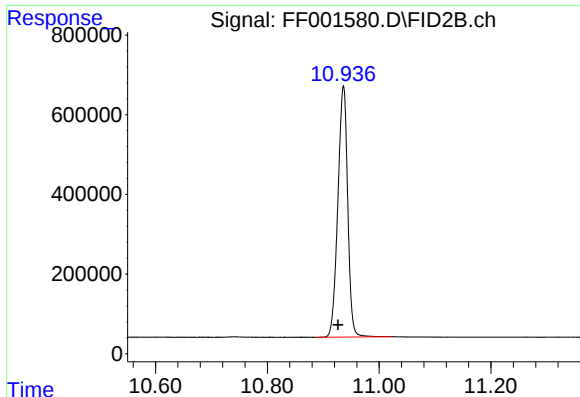


#6 N-OCTADECANE

R.T.: 10.936 min
Delta R.T.: 0.009 min
Response: 7695679
Conc: 51.49 ug/ml

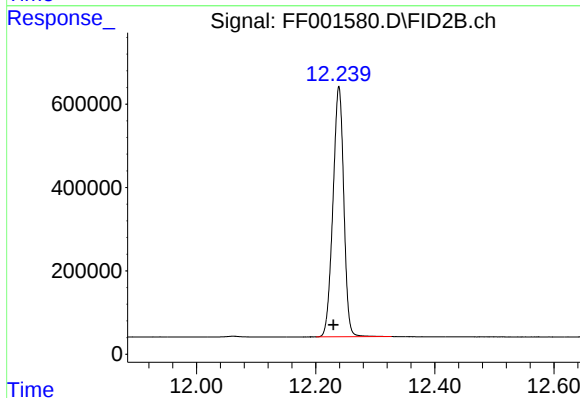


#7 N-EICOSANE

R.T.: 12.239 min
Delta R.T.: 0.010 min
Response: 7596592
Conc: 51.43 ug/ml

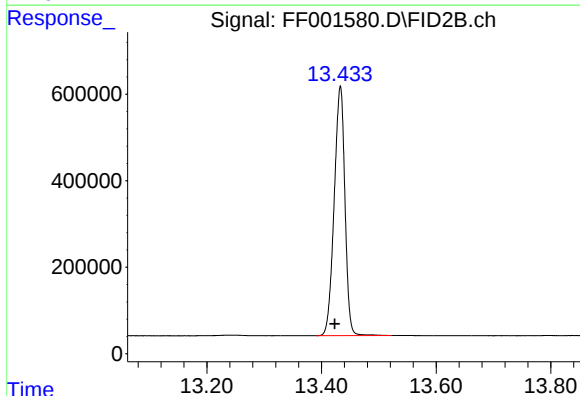


#8 N-DOCOSANE

R.T.: 13.433 min
Delta R.T.: 0.010 min
Response: 7507790
Conc: 51.79 ug/ml

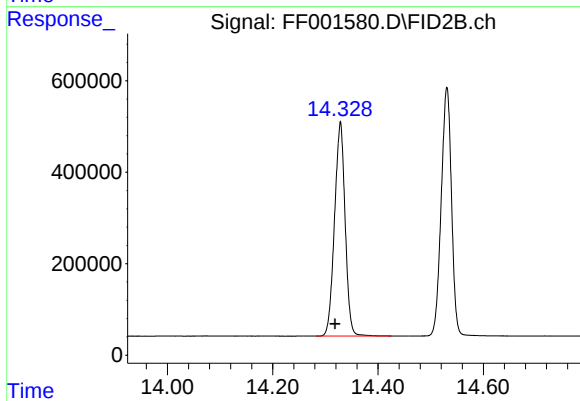


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.329 min
Delta R.T.: 0.010 min
Response: 6541573
Conc: 52.06 ug/ml

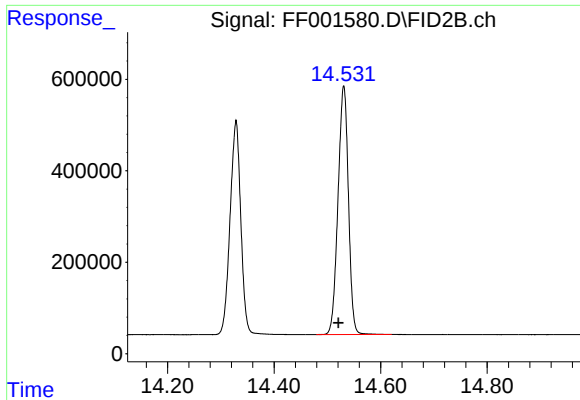


#10 N-TETRACOSANE

R.T.: 14.531 min
Delta R.T.: 0.010 min
Response: 7367751
Conc: 51.97 ug/ml

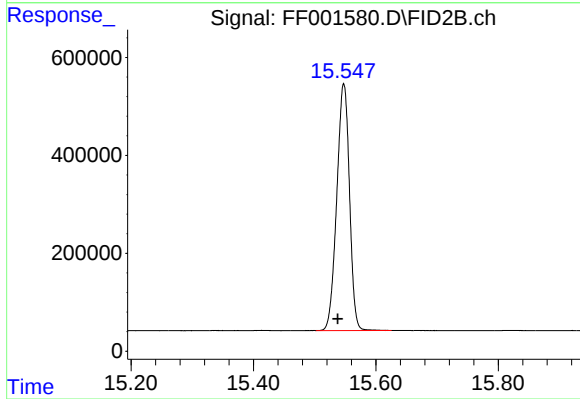

#11 N-HEXACOSANE

R.T.: 15.548 min
Delta R.T.: 0.010 min
Response: 7266893
Conc: 51.92 ug/ml

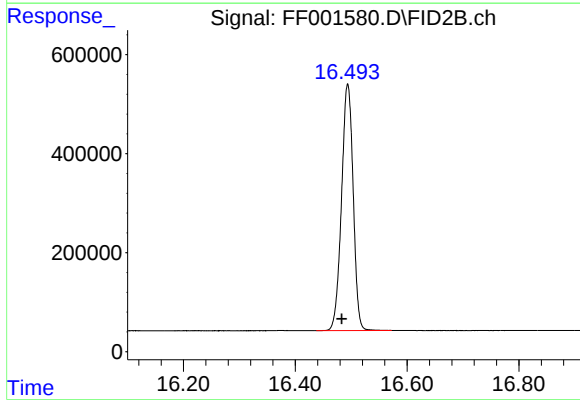

#12 N-OCTACOSANE

R.T.: 16.494 min
Delta R.T.: 0.011 min
Response: 7194772
Conc: 51.85 ug/ml