

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF073124\
Data File : FF014319.D
Signal(s) : FID2B.ch
Acq On : 31 Jul 2024 09:24
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 02:16:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:21 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.633	2229104	16.759 ug/ml
11)	N-HEXACOSANE	16.146	59740	0.465 ug/ml
12)	N-OCTACOSANE	17.094	1970465	15.691 ug/ml
13)	N-TRIACONTANE	17.984	180323	1.478 ug/ml
14)	N-DOTRIACONTANE	18.816	243801	2.078 ug/ml
15)	N-TETRATRIACONTANE	19.599	269743	2.833 ug/ml
16)	N-HEXATRIACONTANE	20.342	233501	3.138 ug/ml
17)	N-OCTATRIACONTANE	21.068	187907	2.785 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF073124\
Data File : FF014319.D
Signal(s) : FID2B.ch
Acq On : 31 Jul 2024 09:24
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 02:16:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:21 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

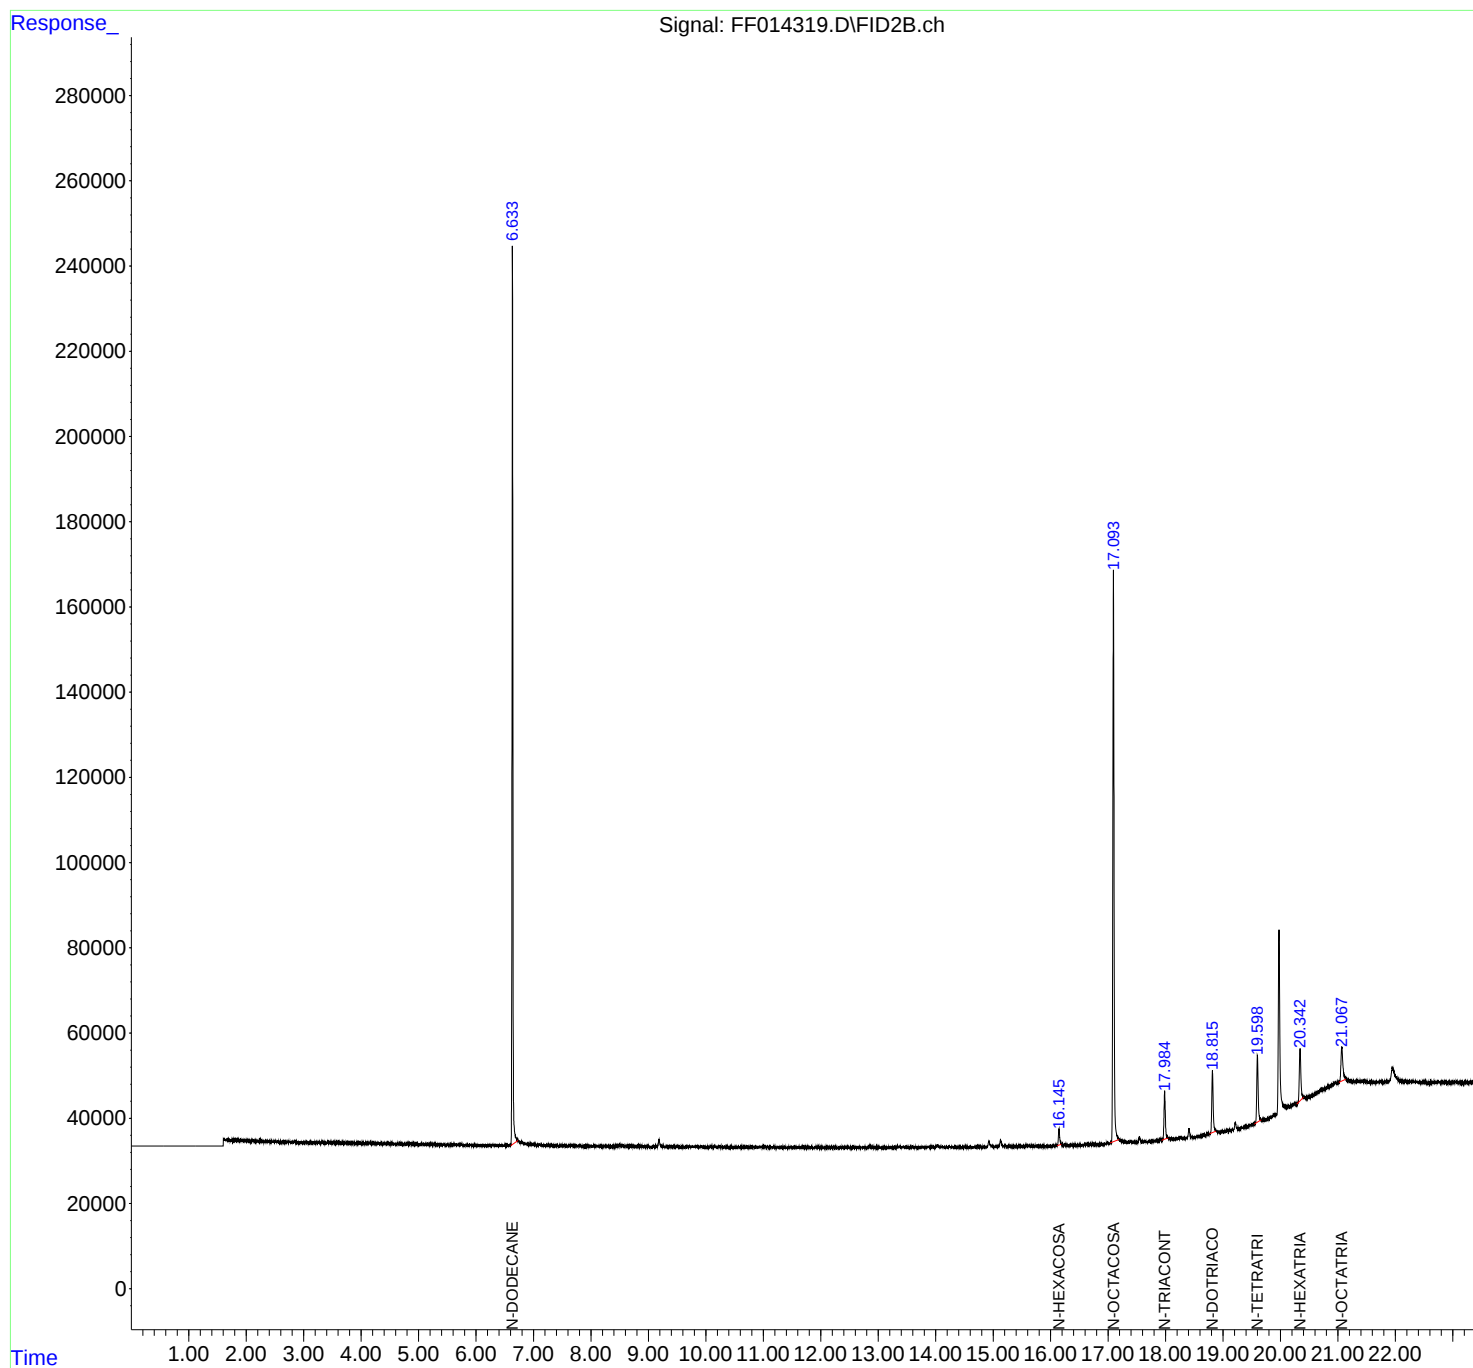


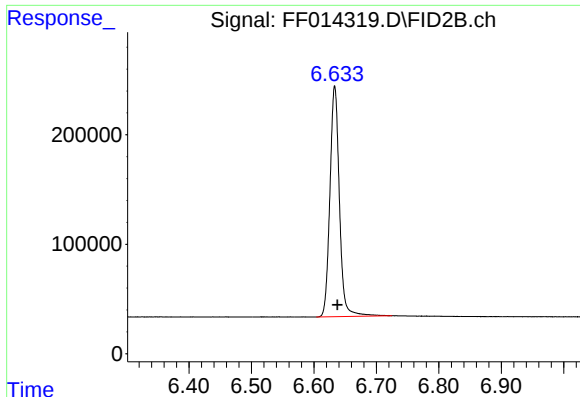

#3 N-DODECANE


R.T.: 6.633 min
Delta R.T.: -0.004 min
Response: 2229104
Conc: 16.76 ug/ml

Instrument :
FID_F
ClientSampleId :

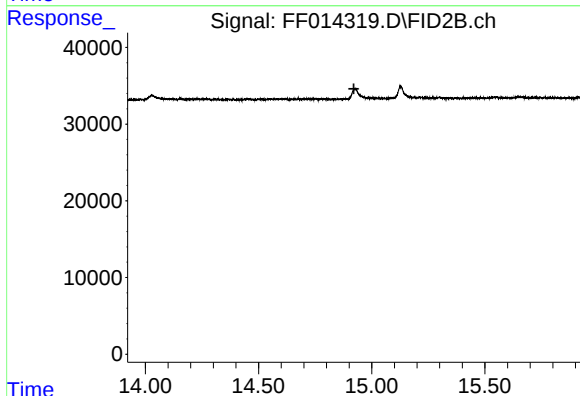


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.921 min
Response: 0
Conc: N.D.

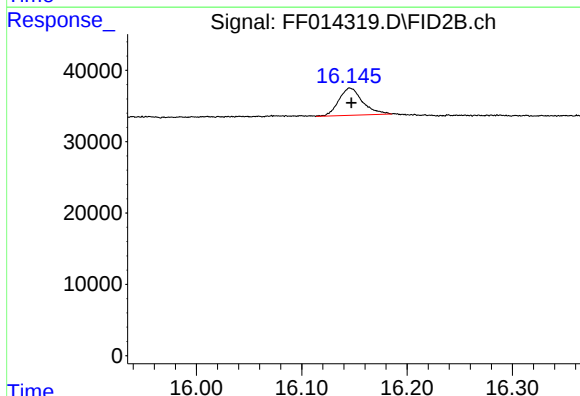


#11 N-HEXACOSANE

R.T.: 16.146 min
Delta R.T.: -0.001 min
Response: 59740
Conc: 0.46 ug/ml

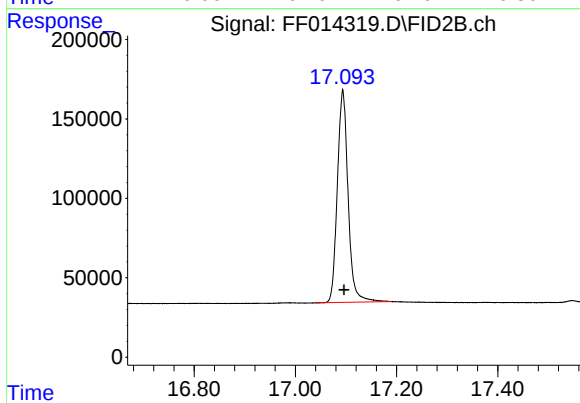

#12 N-OCTACOSANE


R.T.: 17.094 min
Delta R.T.: -0.002 min
Response: 1970465
Conc: 15.69 ug/ml

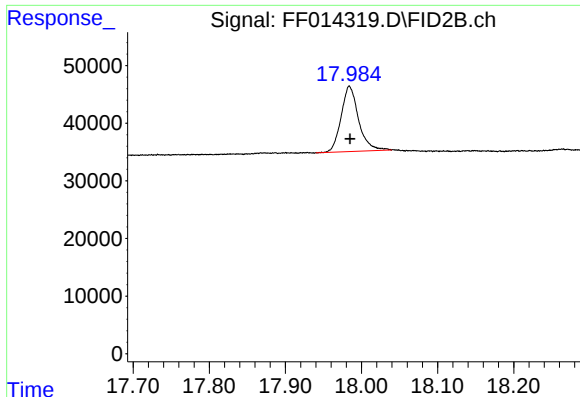

#13 N-TRIACONTANE


R.T.: 17.984 min
Delta R.T.: 0.000 min
Response: 180323
Conc: 1.48 ug/ml

Instrument :
FID_F
ClientSampleId :

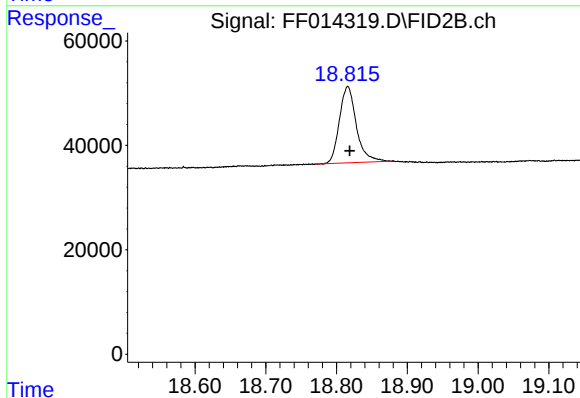


#14 N-DOTRIACONTANE

R.T.: 18.816 min
Delta R.T.: -0.003 min
Response: 243801
Conc: 2.08 ug/ml

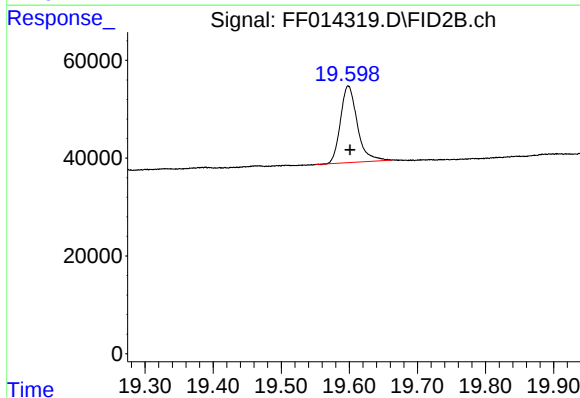


#15 N-TETRATRIACONTANE

R.T.: 19.599 min
Delta R.T.: -0.002 min
Response: 269743
Conc: 2.83 ug/ml

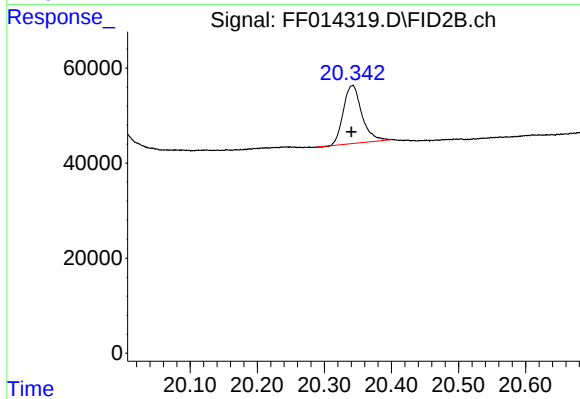

#16 N-HEXATRIACONTANE

R.T.: 20.342 min
Delta R.T.: 0.002 min
Response: 233501
Conc: 3.14 ug/ml

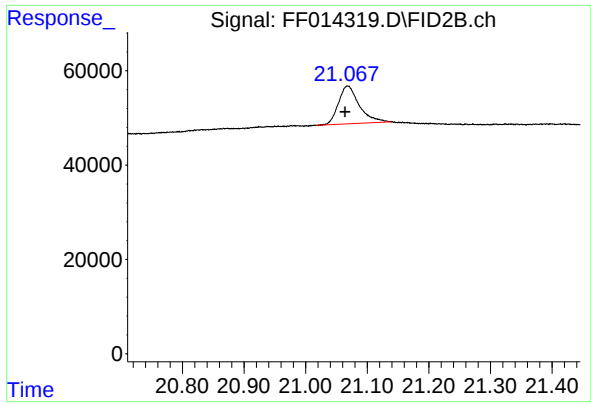

#17 N-OCTATRIACONTANE

R.T.: 21.068 min
Delta R.T.: 0.004 min
Response: 187907
Conc: 2.78 ug/ml

Instrument :
FID_F
ClientSampleId :