

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF073124\
 Data File : FF014332.D
 Signal(s) : FID2B.ch
 Acq On : 31 Jul 2024 16:18
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 01 02:20:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072324.M
 Quant Title :
 QLast Update : Tue Jul 23 14:43:21 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.633	2107630	15.846 ug/ml
12) N-OCTACOSANE	17.093	1990653	15.851 ug/ml
13) N-TRIACONTANE	17.981	217072	1.779 ug/ml
14) N-DOTRIACONTANE	18.814	374533	3.192 ug/ml
15) N-TETRATRIACONTANE	19.596	501578	5.268 ug/ml
16) N-HEXATRIACONTANE	20.338	555774	7.468 ug/ml
17) N-OCTATRIACONTANE	21.063	476506	7.062 ug/ml
18) N-TETRACONTANE	21.943	355218	5.648 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF073124\
Data File : FF014332.D
Signal(s) : FID2B.ch
Acq On : 31 Jul 2024 16:18
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 02:20:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:21 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

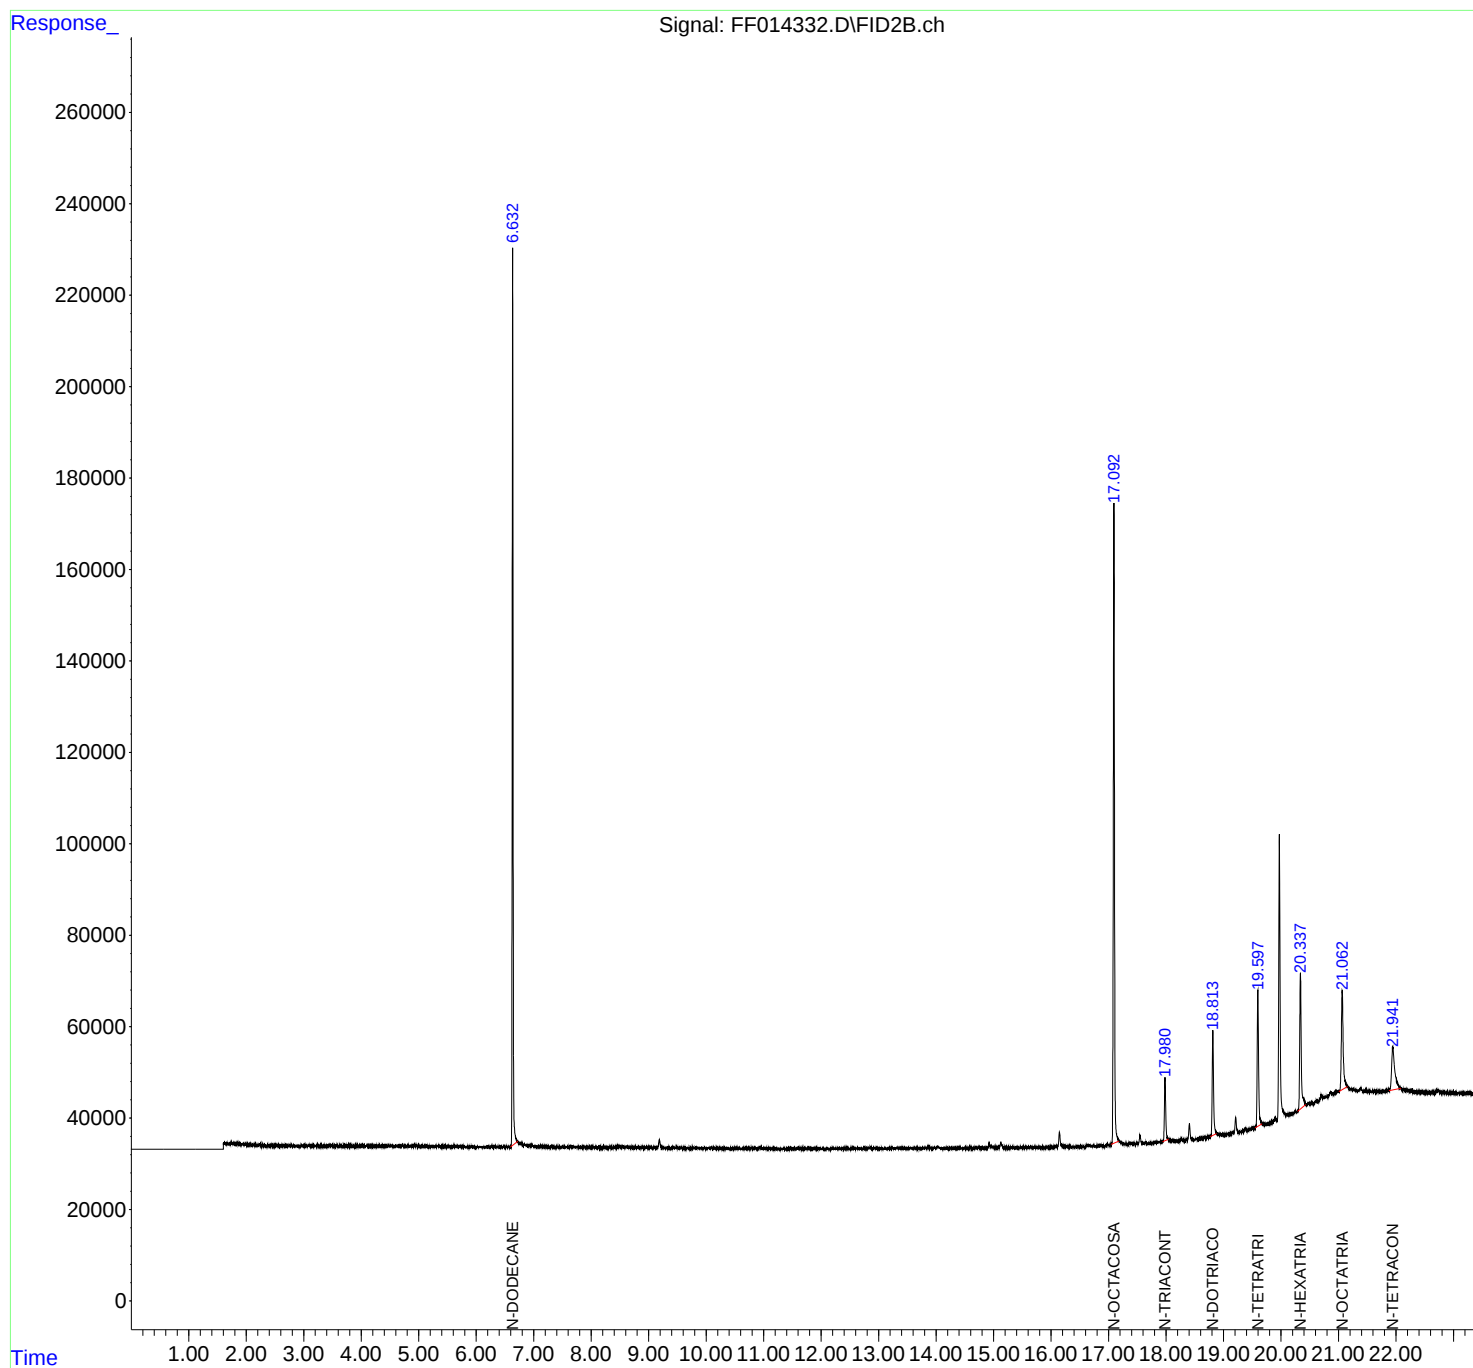


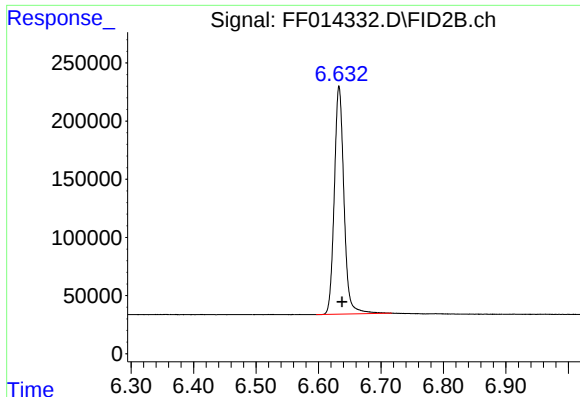

#3 N-DODECANE


R.T.: 6.633 min
Delta R.T.: -0.005 min
Response: 2107630
Conc: 15.85 ug/ml

Instrument :
FID_F
ClientSampleId :

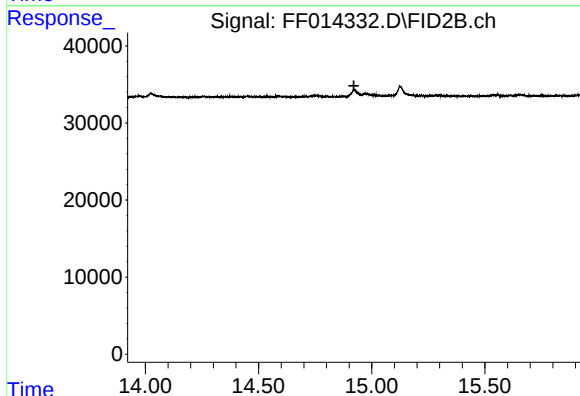


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.921 min
Response: 0
Conc: N.D.

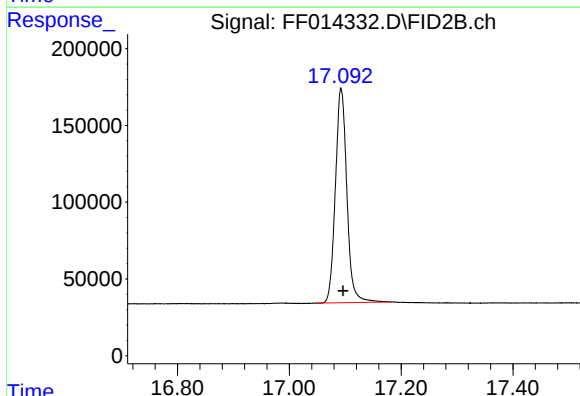


#12 N-OCTACOSANE

R.T.: 17.093 min
Delta R.T.: -0.004 min
Response: 1990653
Conc: 15.85 ug/ml

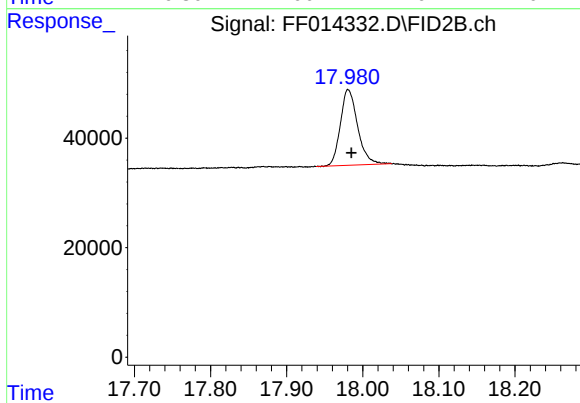

#13 N-TRIACONTANE


R.T.: 17.981 min
Delta R.T.: -0.004 min
Response: 217072
Conc: 1.78 ug/ml

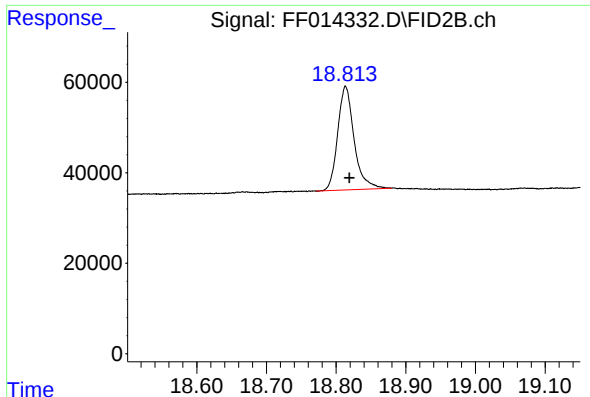

#14 N-DOTRIACONTANE


R.T.: 18.814 min
Delta R.T.: -0.005 min
Response: 374533
Conc: 3.19 ug/ml

Instrument :
FID_F
ClientSampleId :

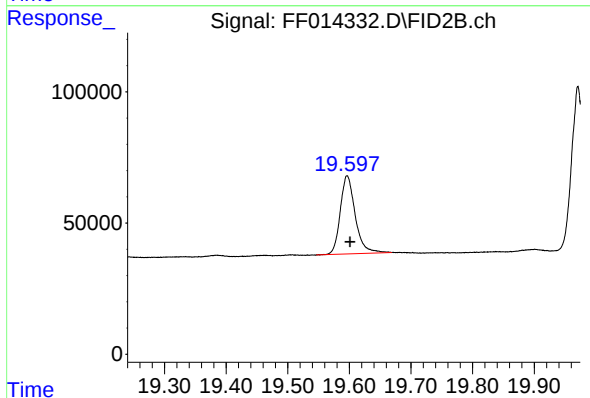


#15 N-TETRATRIACONTANE

R.T.: 19.596 min
Delta R.T.: -0.005 min
Response: 501578
Conc: 5.27 ug/ml

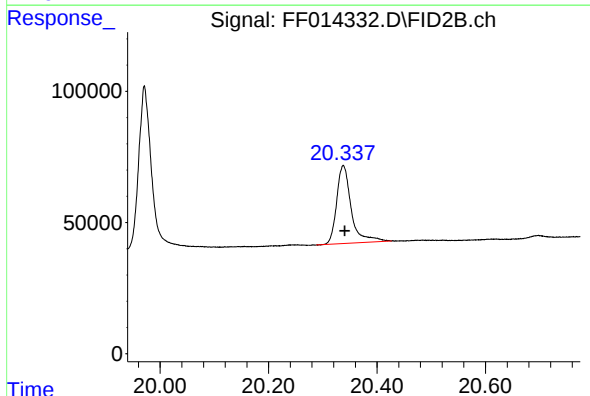


#16 N-HEXATRIACONTANE

R.T.: 20.338 min
Delta R.T.: -0.003 min
Response: 555774
Conc: 7.47 ug/ml

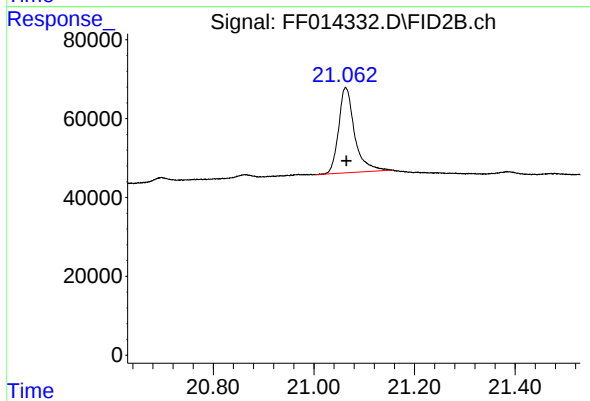

#17 N-OCTATRIACONTANE

R.T.: 21.063 min
Delta R.T.: -0.001 min
Response: 476506
Conc: 7.06 ug/ml

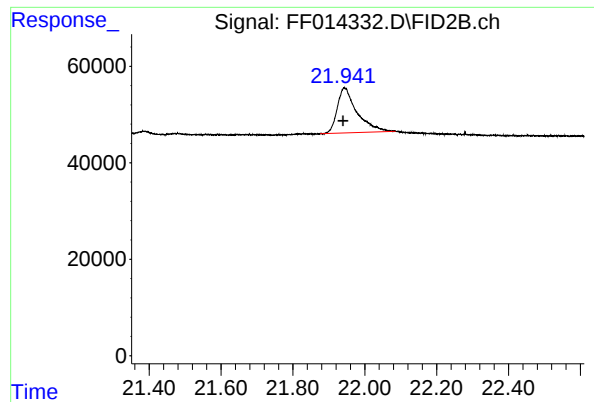

#18 N-TETRACONTANE

R.T.: 21.943 min
Delta R.T.: 0.003 min
Response: 355218
Conc: 5.65 ug/ml

Instrument :

FID_F

ClientSampleId :