

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
Data File : FF001610.D
Signal(s) : FID2B.ch
Acq On : 01 Aug 2018 09:25
Operator : AJ\SJ
Sample : J4231-11 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 13:06:51 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Mon Jul 30 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.336	278763	2.219 ug/ml
Target Compounds			
4) N-TETRADECANE	7.853	87581	0.582 ug/ml
7) N-EICOSANE	12.206	259986	1.760 ug/ml
8) N-DOCOSANE	13.443	250186	1.726 ug/ml
10) N-TETRACOSANE	14.496	1028562	7.255 ug/ml
12) N-OCTACOSANE	16.500	143312	1.033 ug/ml
14) N-DOTRIACONTANE	18.162	259742	2.023 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
Data File : FF001610.D
Signal(s) : FID2B.ch
Acq On : 01 Aug 2018 09:25
Operator : AJ\SJ
Sample : J4231-11 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 13:06:51 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Mon Jul 30 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

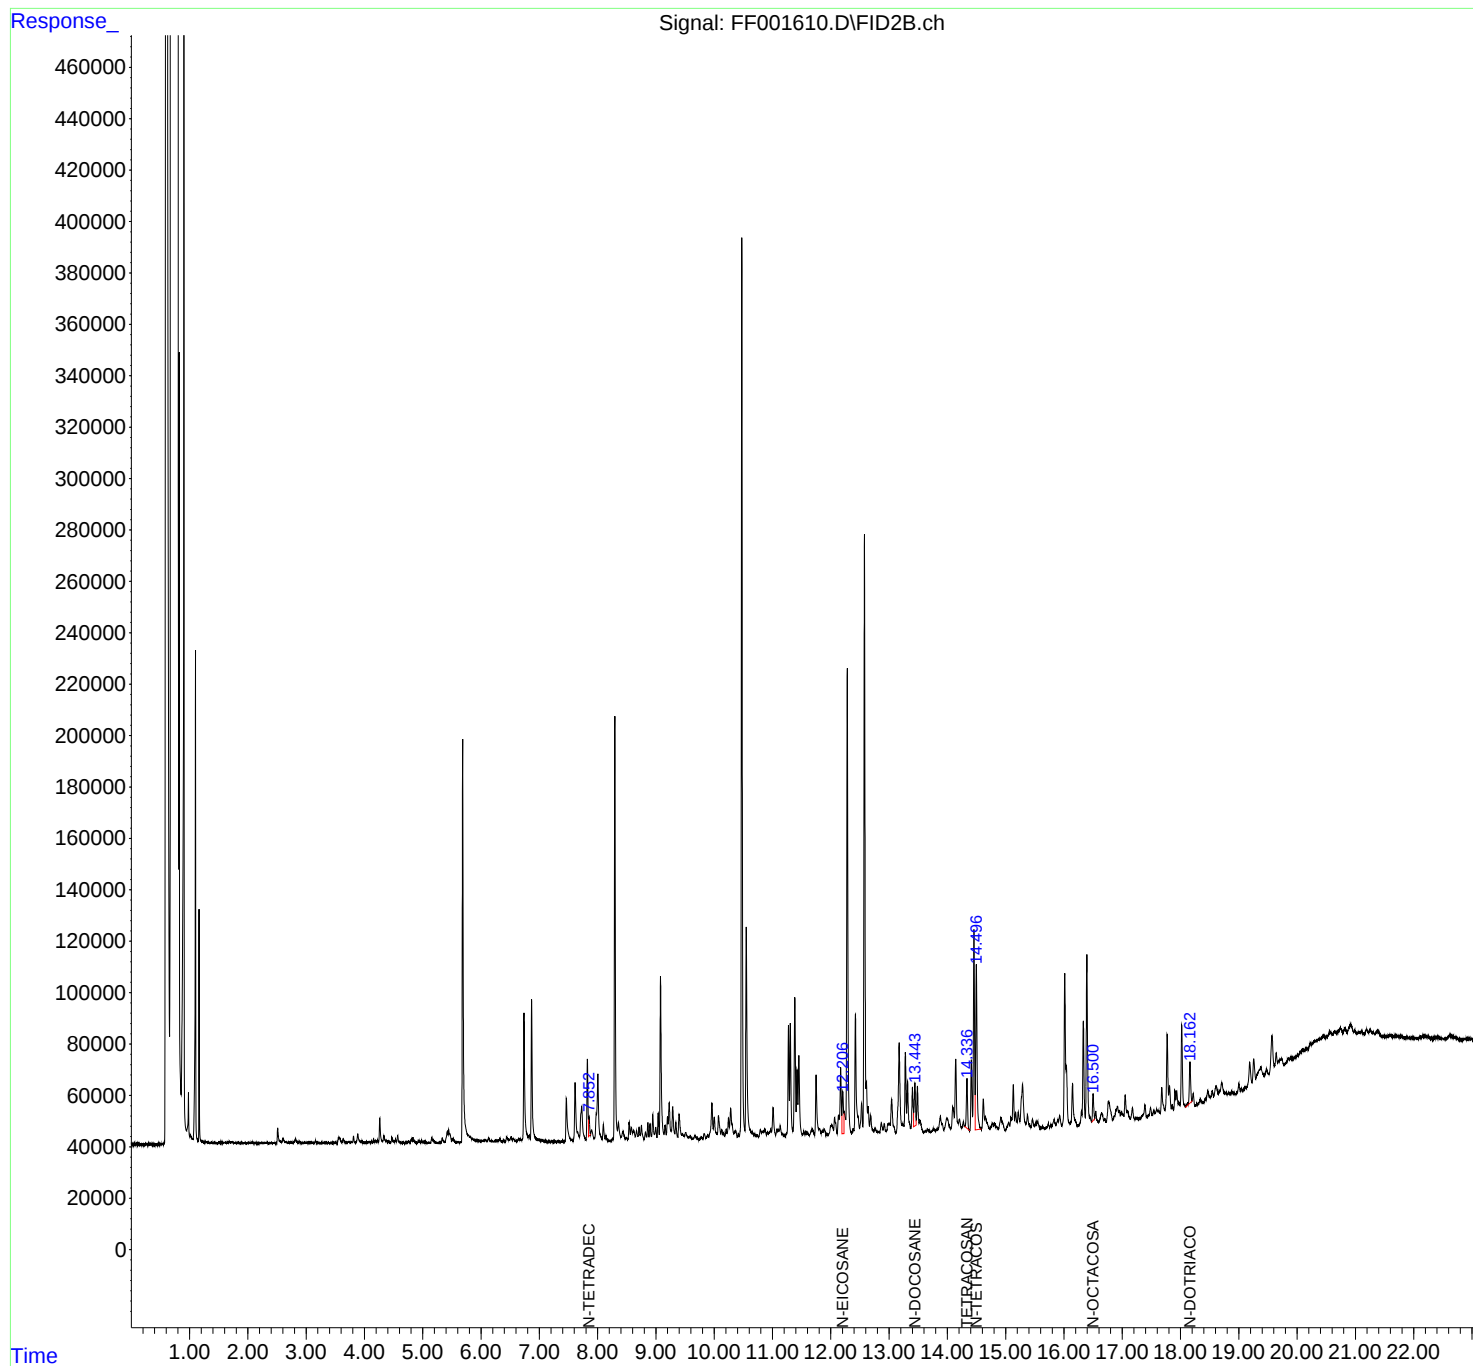


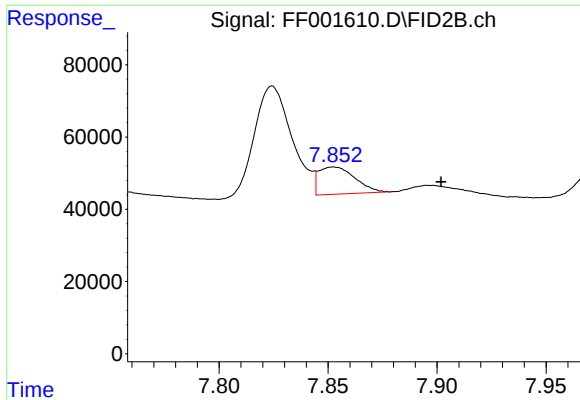

#4 N-TETRADECANE


R.T.: 7.853 min
Delta R.T.: -0.049 min
Response: 87581
Conc: 0.58 ug/ml

Instrument :
FID_F
ClientSampleId :

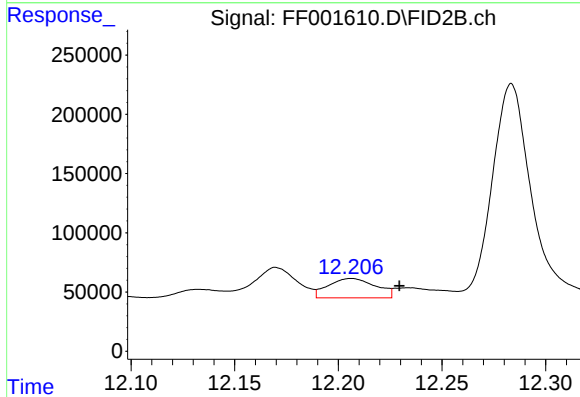


#7 N-EICOSANE

R.T.: 12.206 min
Delta R.T.: -0.023 min
Response: 259986
Conc: 1.76 ug/ml

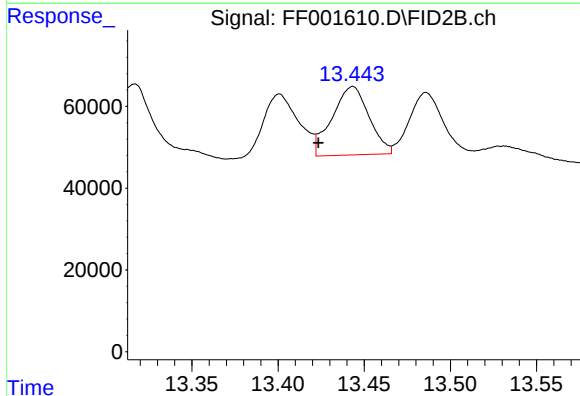


#8 N-DOCOSANE

R.T.: 13.443 min
Delta R.T.: 0.020 min
Response: 250186
Conc: 1.73 ug/ml

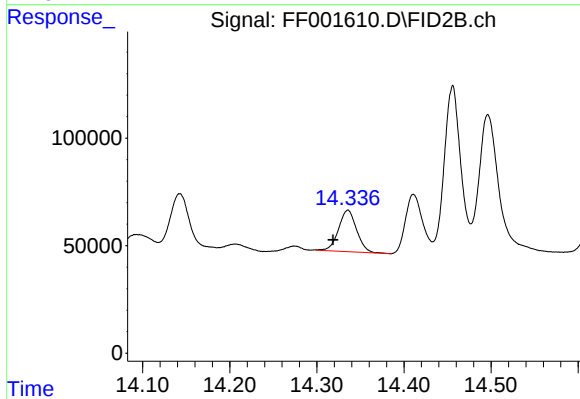

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.336 min
Delta R.T.: 0.017 min
Response: 278763
Conc: 2.22 ug/ml

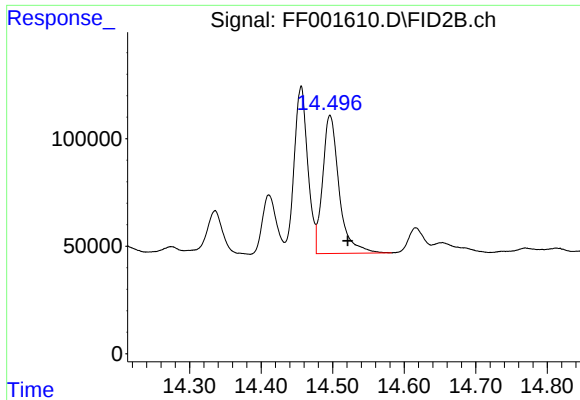

#10 N-TETRACOSANE


R.T.: 14.496 min
Delta R.T.: -0.025 min
Response: 1028562
Conc: 7.26 ug/ml

Instrument :
FID_F
ClientSampleId :

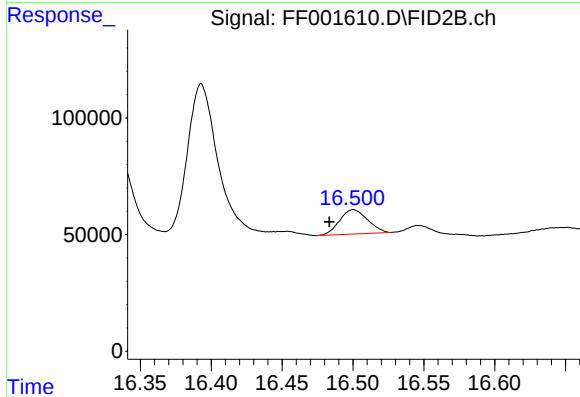

#12 N-OCTACOSANE

R.T.: 16.500 min
Delta R.T.: 0.017 min
Response: 143312
Conc: 1.03 ug/ml

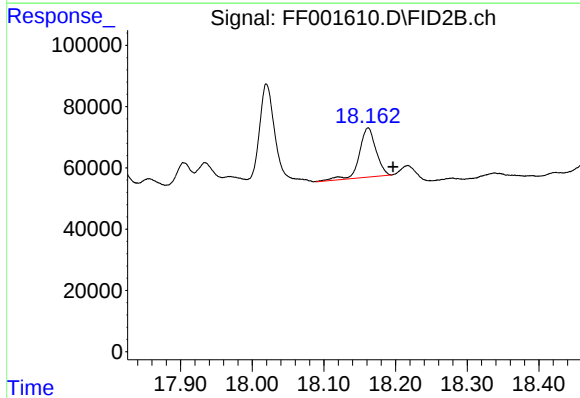

#14 N-DOTRIACONTANE

R.T.: 18.162 min
Delta R.T.: -0.035 min
Response: 259742
Conc: 2.02 ug/ml