

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
 Data File : FF001611.D
 Signal(s) : FID2B.ch
 Acq On : 01 Aug 2018 09:55
 Operator : AJ\SJ
 Sample : J4231-15 20X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 01 13:06:59 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Mon Jul 30 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.336	163724	1.303 ug/ml
Target Compounds			
4) N-TETRADECANE	7.853	134058	0.891 ug/ml
7) N-EICOSANE	12.206	270668	1.833 ug/ml
8) N-DOCOSANE	13.444	260820	1.799 ug/ml
10) N-TETRACOSANE	14.496	1612328	11.373 ug/ml
12) N-OCTACOSANE	16.499	183925	1.326 ug/ml
14) N-DOTRIACONTANE	18.161	443491	3.453 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
Data File : FF001611.D
Signal(s) : FID2B.ch
Acq On : 01 Aug 2018 09:55
Operator : AJ\SJ
Sample : J4231-15 20X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 13:06:59 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Mon Jul 30 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

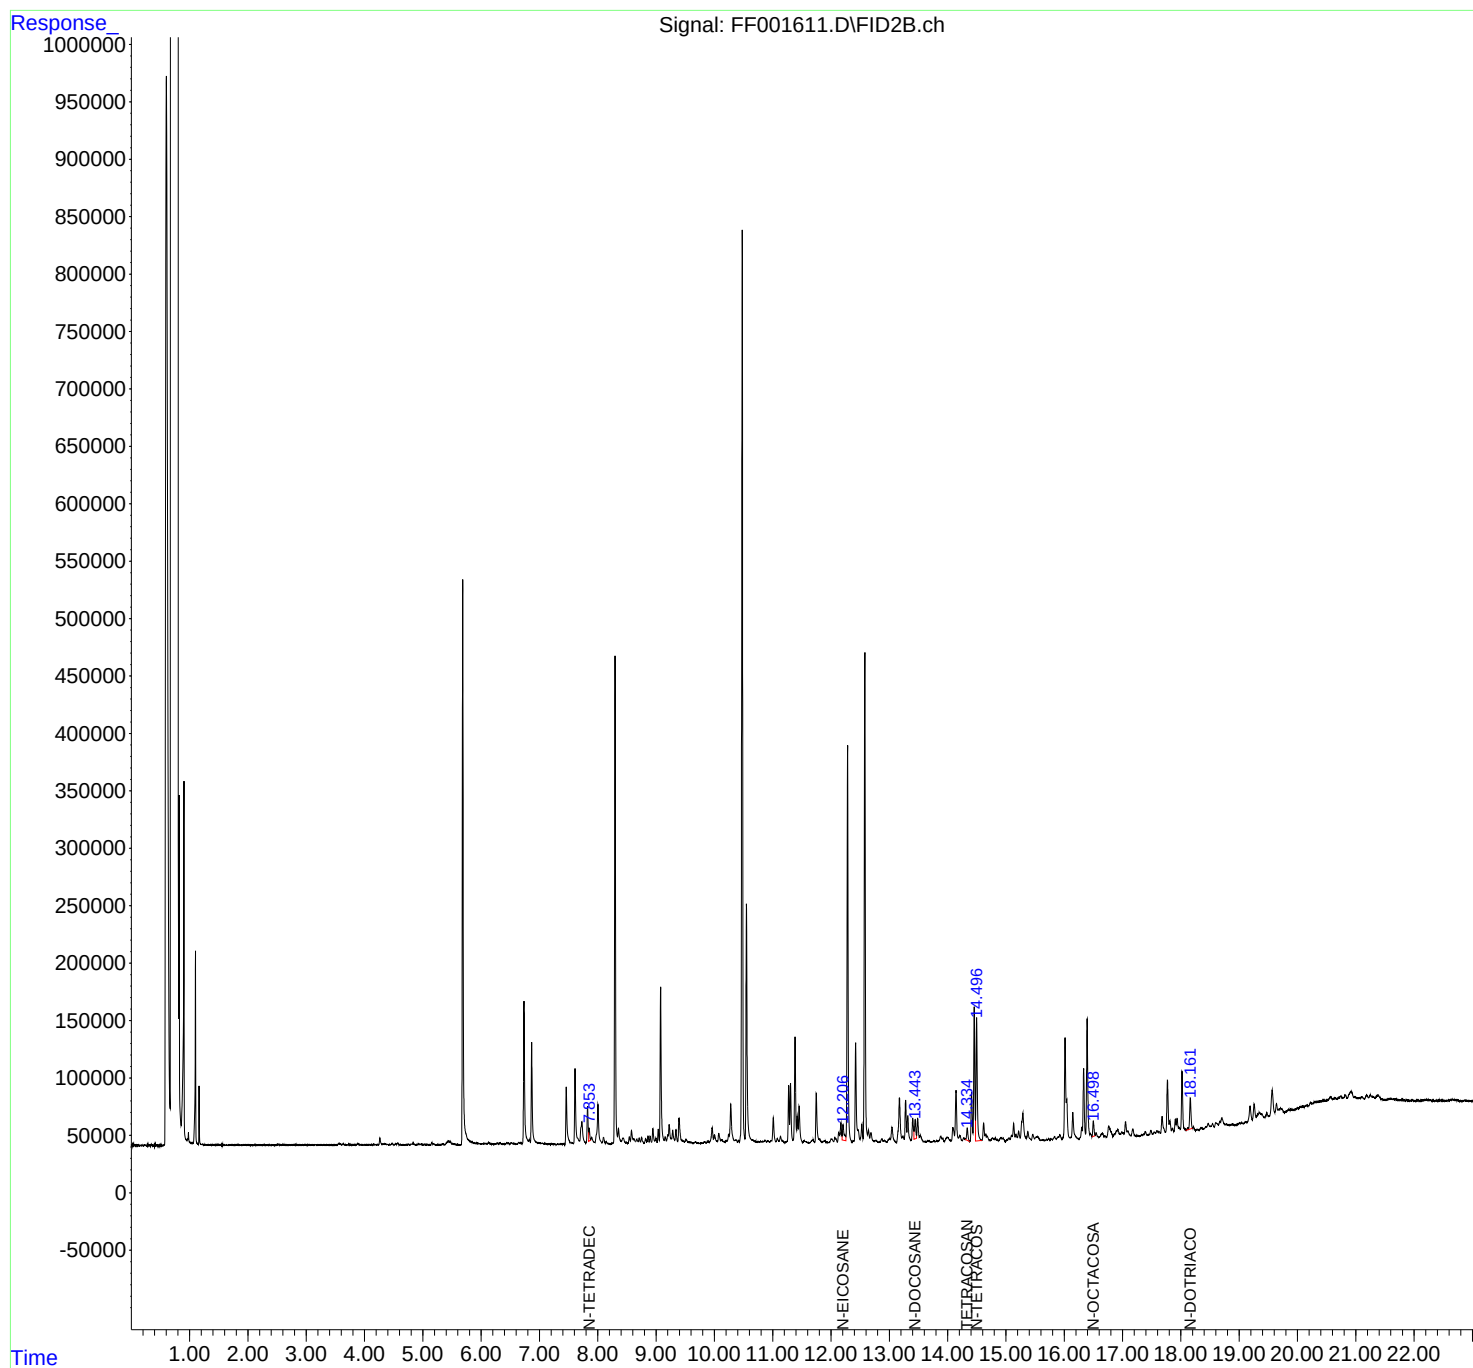


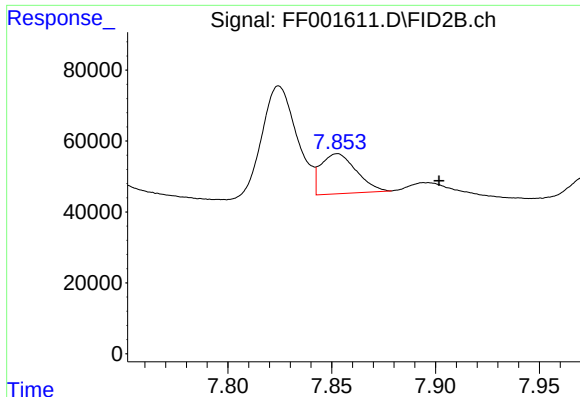

#4 N-TETRADECANE


R.T.: 7.853 min
Delta R.T.: -0.049 min
Response: 134058
Conc: 0.89 ug/ml

Instrument :
FID_F
ClientSampleId :

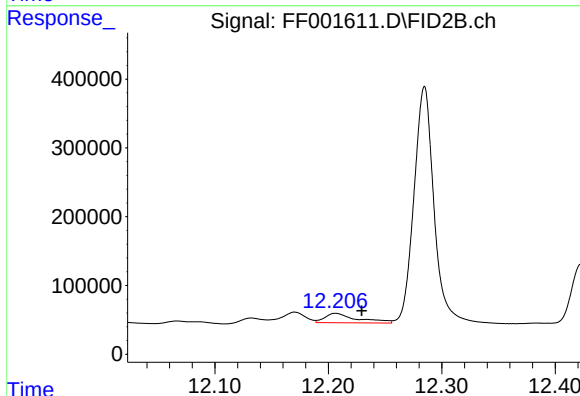


#7 N-EICOSANE

R.T.: 12.206 min
Delta R.T.: -0.023 min
Response: 270668
Conc: 1.83 ug/ml

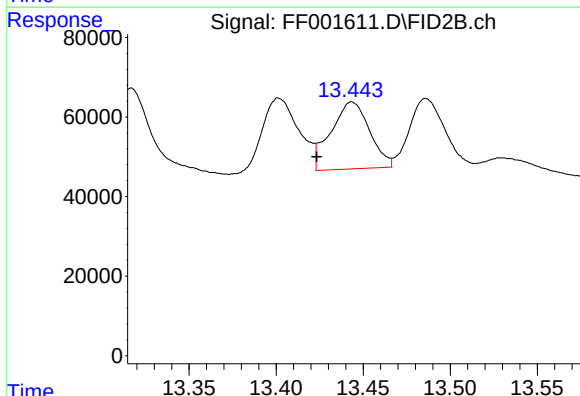


#8 N-DOCOSANE

R.T.: 13.444 min
Delta R.T.: 0.020 min
Response: 260820
Conc: 1.80 ug/ml

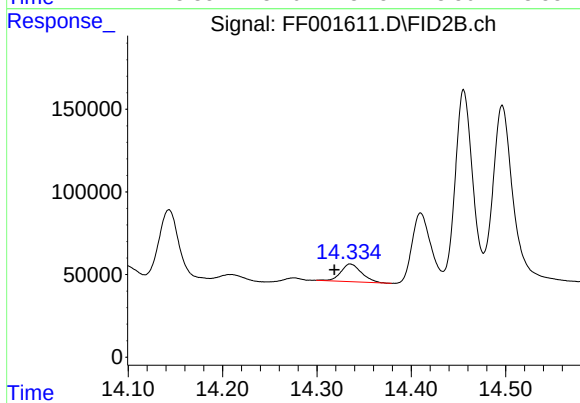

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.336 min
Delta R.T.: 0.017 min
Response: 163724
Conc: 1.30 ug/ml

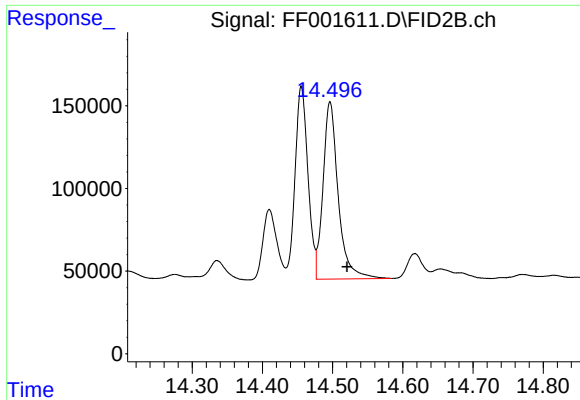

#10 N-TETRACOSANE


R.T.: 14.496 min
Delta R.T.: -0.024 min
Response: 1612328
Conc: 11.37 ug/ml

Instrument :
FID_F
ClientSampleId :

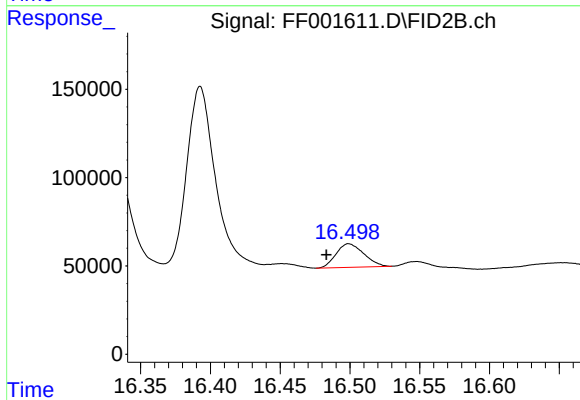

#12 N-OCTACOSANE

R.T.: 16.499 min
Delta R.T.: 0.016 min
Response: 183925
Conc: 1.33 ug/ml

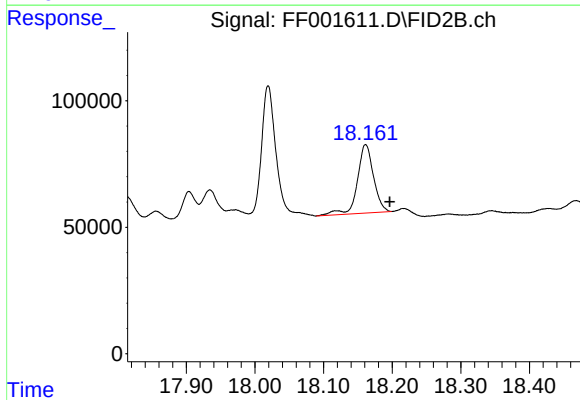

#14 N-DOTRIACONTANE

R.T.: 18.161 min
Delta R.T.: -0.035 min
Response: 443491
Conc: 3.45 ug/ml