

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
 Data File : FF001612.D
 Signal(s) : FID2B.ch
 Acq On : 01 Aug 2018 10:26
 Operator : AJ\SJ
 Sample : J4231-09 50X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 01 13:07:07 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Mon Jul 30 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.335	335625	2.671 ug/ml
Target Compounds			
5) N-HEXADECANE	9.507	133869	0.896 ug/ml
7) N-EICOSANE	12.238	249453	1.689 ug/ml
8) N-DOCOSANE	13.442	591948	4.083 ug/ml
10) N-TETRACOSANE	14.499	3491212	24.626 ug/ml
11) N-HEXACOSANE	15.537	227728	1.627 ug/ml
12) N-OCTACOSANE	16.497	592695	4.272 ug/ml
13) N-TRIACONTANE	17.391	105682	0.773 ug/ml
14) N-DOTRIACONTANE	18.160	822987	6.409 ug/ml
16) N-HEXATRIACONTANE	19.706	264167	2.388 ug/ml
18) N-TETRACONTANE	21.180	146334	1.482 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
Data File : FF001612.D
Signal(s) : FID2B.ch
Acq On : 01 Aug 2018 10:26
Operator : AJ\SJ
Sample : J4231-09 50X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 13:07:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Mon Jul 30 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

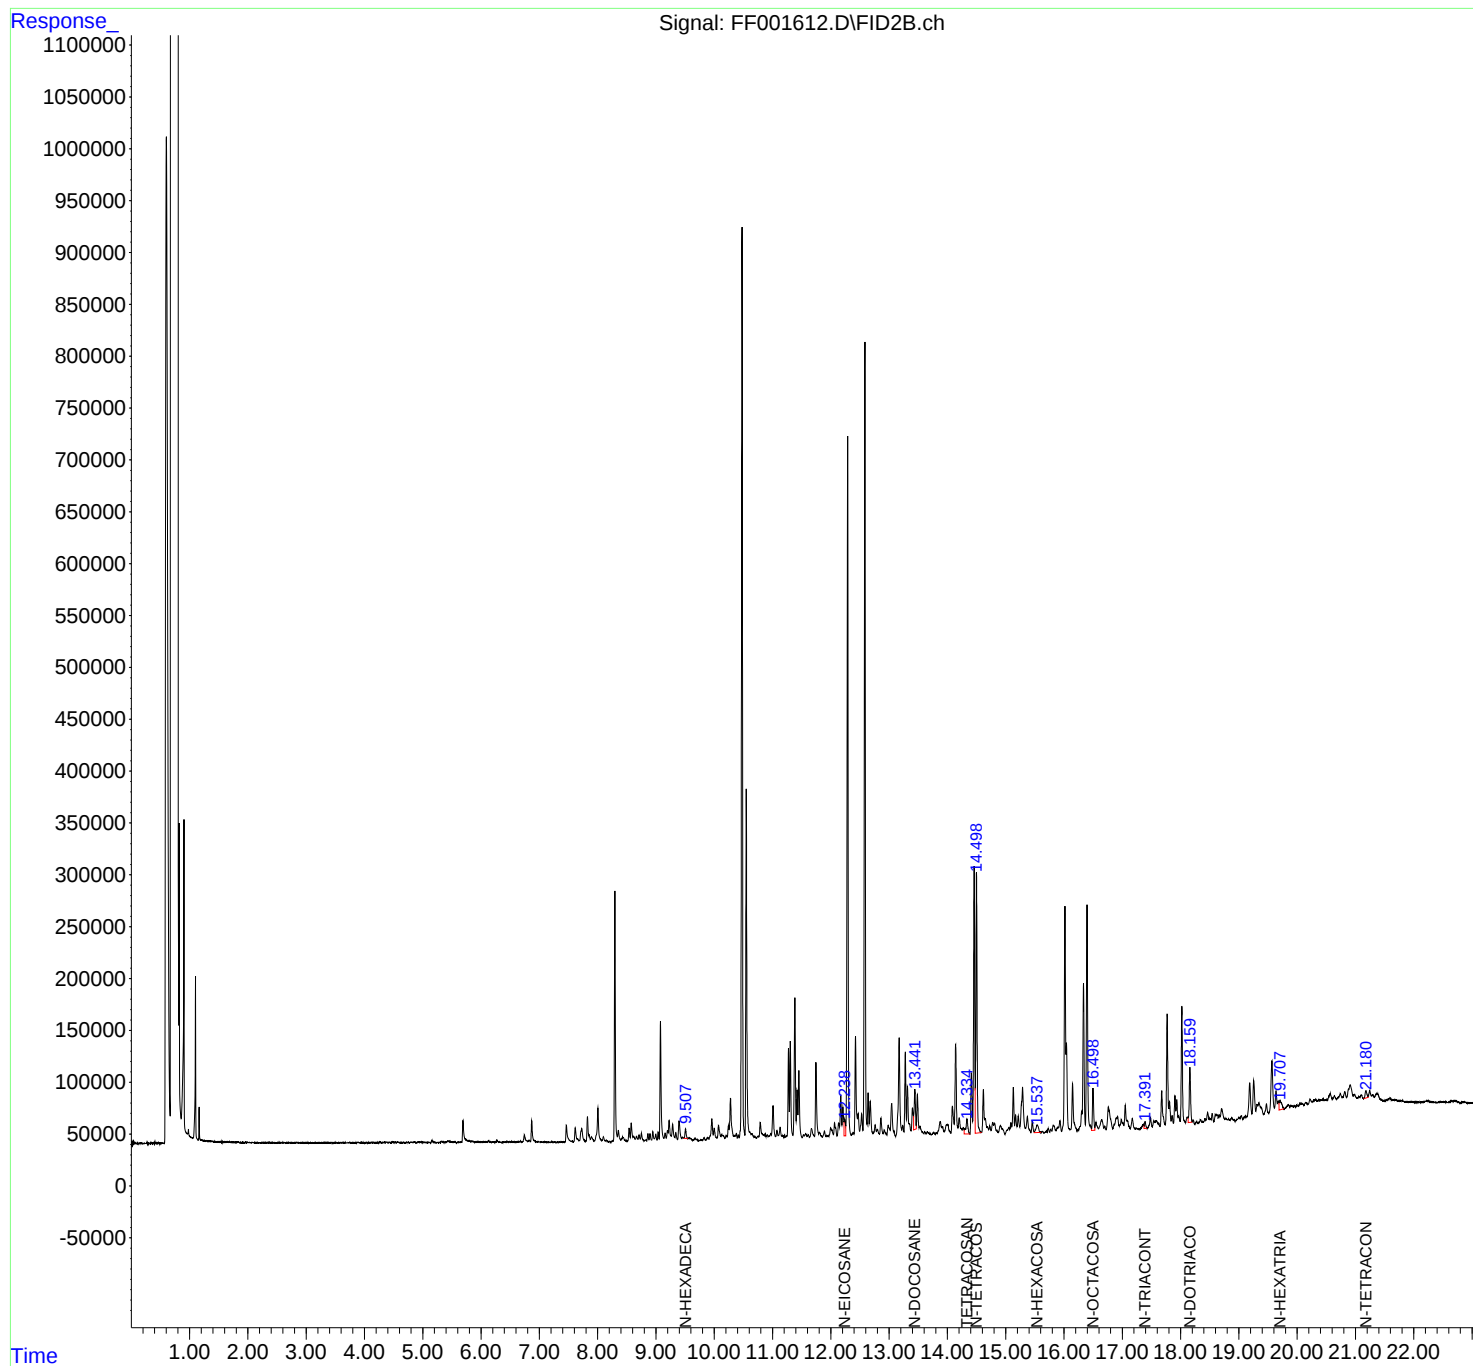


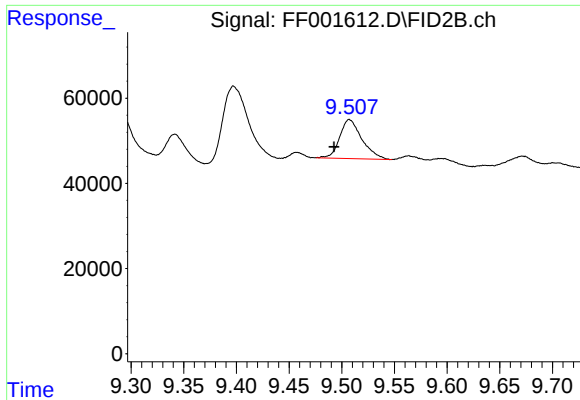

#5 N-HEXADECANE


R.T.: 9.507 min
Delta R.T.: 0.015 min
Response: 133869
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :

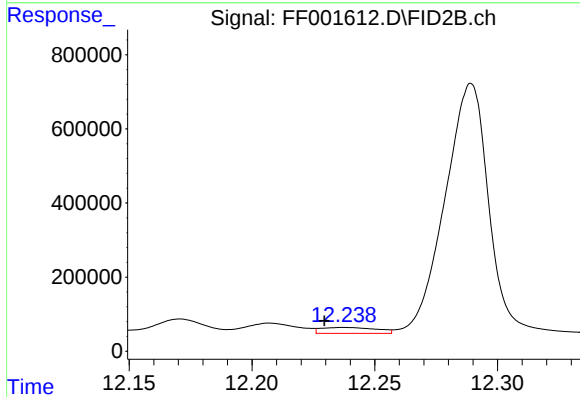


#7 N-EICOSANE

R.T.: 12.238 min
Delta R.T.: 0.008 min
Response: 249453
Conc: 1.69 ug/ml

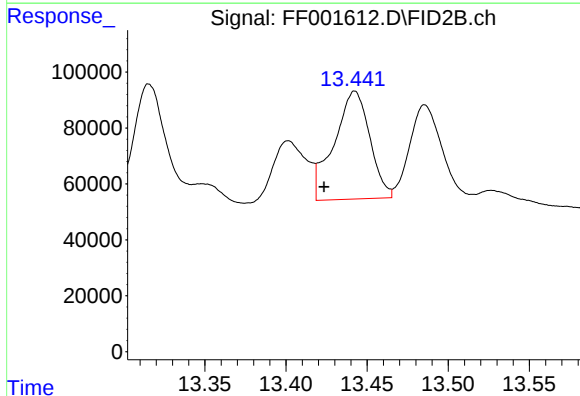


#8 N-DOCOSANE

R.T.: 13.442 min
Delta R.T.: 0.019 min
Response: 591948
Conc: 4.08 ug/ml

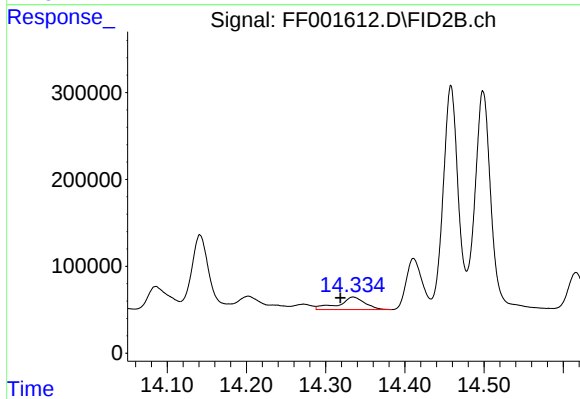

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.335 min
Delta R.T.: 0.016 min
Response: 335625
Conc: 2.67 ug/ml

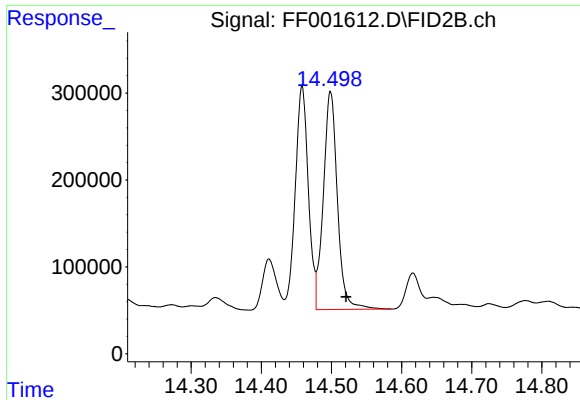

#10 N-TETRACOSANE


R.T.: 14.499 min
Delta R.T.: -0.022 min
Response: 3491212
Conc: 24.63 ug/ml

Instrument :
FID_F
ClientSampleId :

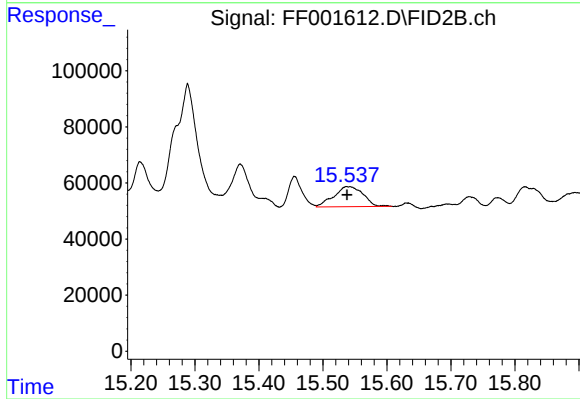


#11 N-HEXACOSANE

R.T.: 15.537 min
Delta R.T.: 0.000 min
Response: 227728
Conc: 1.63 ug/ml

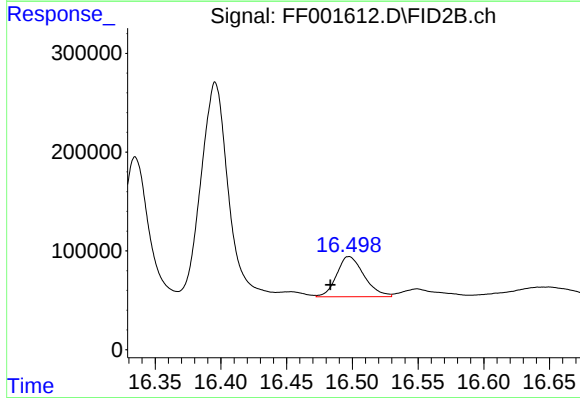


#12 N-OCTACOSANE

R.T.: 16.497 min
Delta R.T.: 0.014 min
Response: 592695
Conc: 4.27 ug/ml

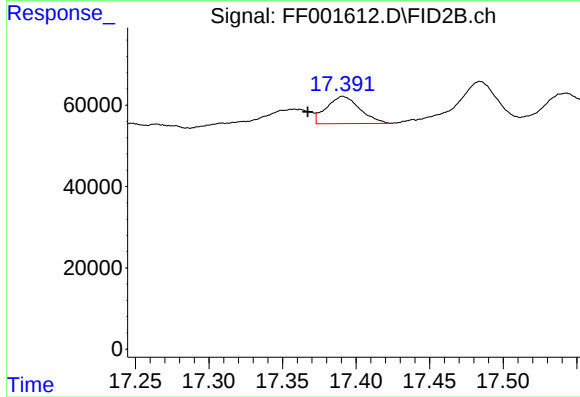

#13 N-TRIACONTANE


R.T.: 17.391 min
Delta R.T.: 0.024 min
Response: 105682
Conc: 0.77 ug/ml

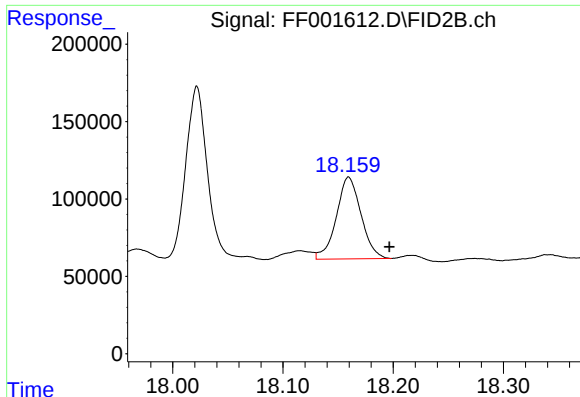

#14 N-DOTRIACONTANE


R.T.: 18.160 min
Delta R.T.: -0.037 min
Response: 822987
Conc: 6.41 ug/ml

Instrument :
FID_F
ClientSampleId :

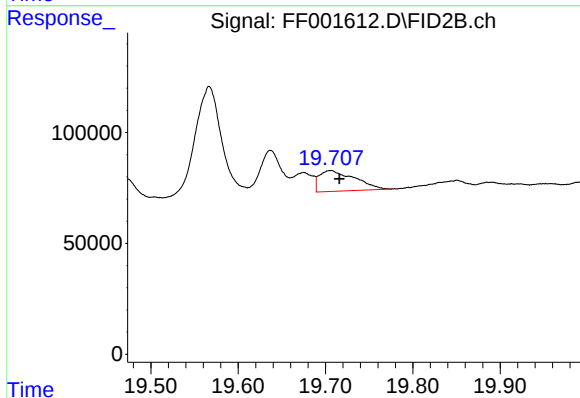

#16 N-HEXATRIACONTANE

R.T.: 19.706 min
Delta R.T.: -0.010 min
Response: 264167
Conc: 2.39 ug/ml

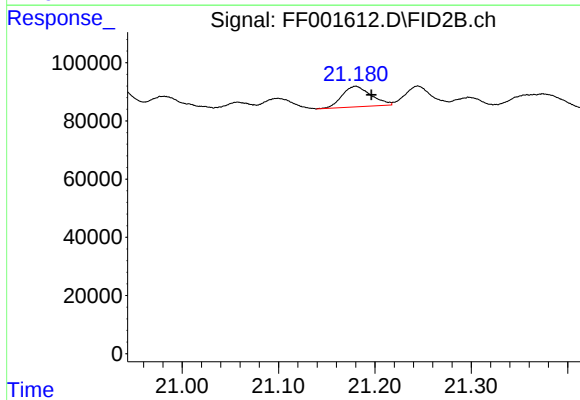

#18 N-TETRACONTANE

R.T.: 21.180 min
Delta R.T.: -0.016 min
Response: 146334
Conc: 1.48 ug/ml