

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
 Data File : FF001613.D
 Signal(s) : FID2B.ch
 Acq On : 01 Aug 2018 10:57
 Operator : AJ\SJ
 Sample : J3823-01 20X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 01 13:07:16 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Mon Jul 30 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.334	88375	0.703 ug/ml
Target Compounds			
3) N-DODECANE	6.129	91398	0.610 ug/ml
4) N-TETRADECANE	7.911	220769	1.467 ug/ml
5) N-HEXADECANE	9.504	323480	2.166 ug/ml
6) N-OCTADECANE	10.939	264259	1.768 ug/ml
7) N-EICOSANE	12.244	213059	1.443 ug/ml
8) N-DOCOSANE	13.441	172421	1.189 ug/ml
10) N-TETRACOSANE	14.530	510494	3.601 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
Data File : FF001613.D
Signal(s) : FID2B.ch
Acq On : 01 Aug 2018 10:57
Operator : AJ\SJ
Sample : J3823-01 20X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 13:07:16 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Mon Jul 30 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

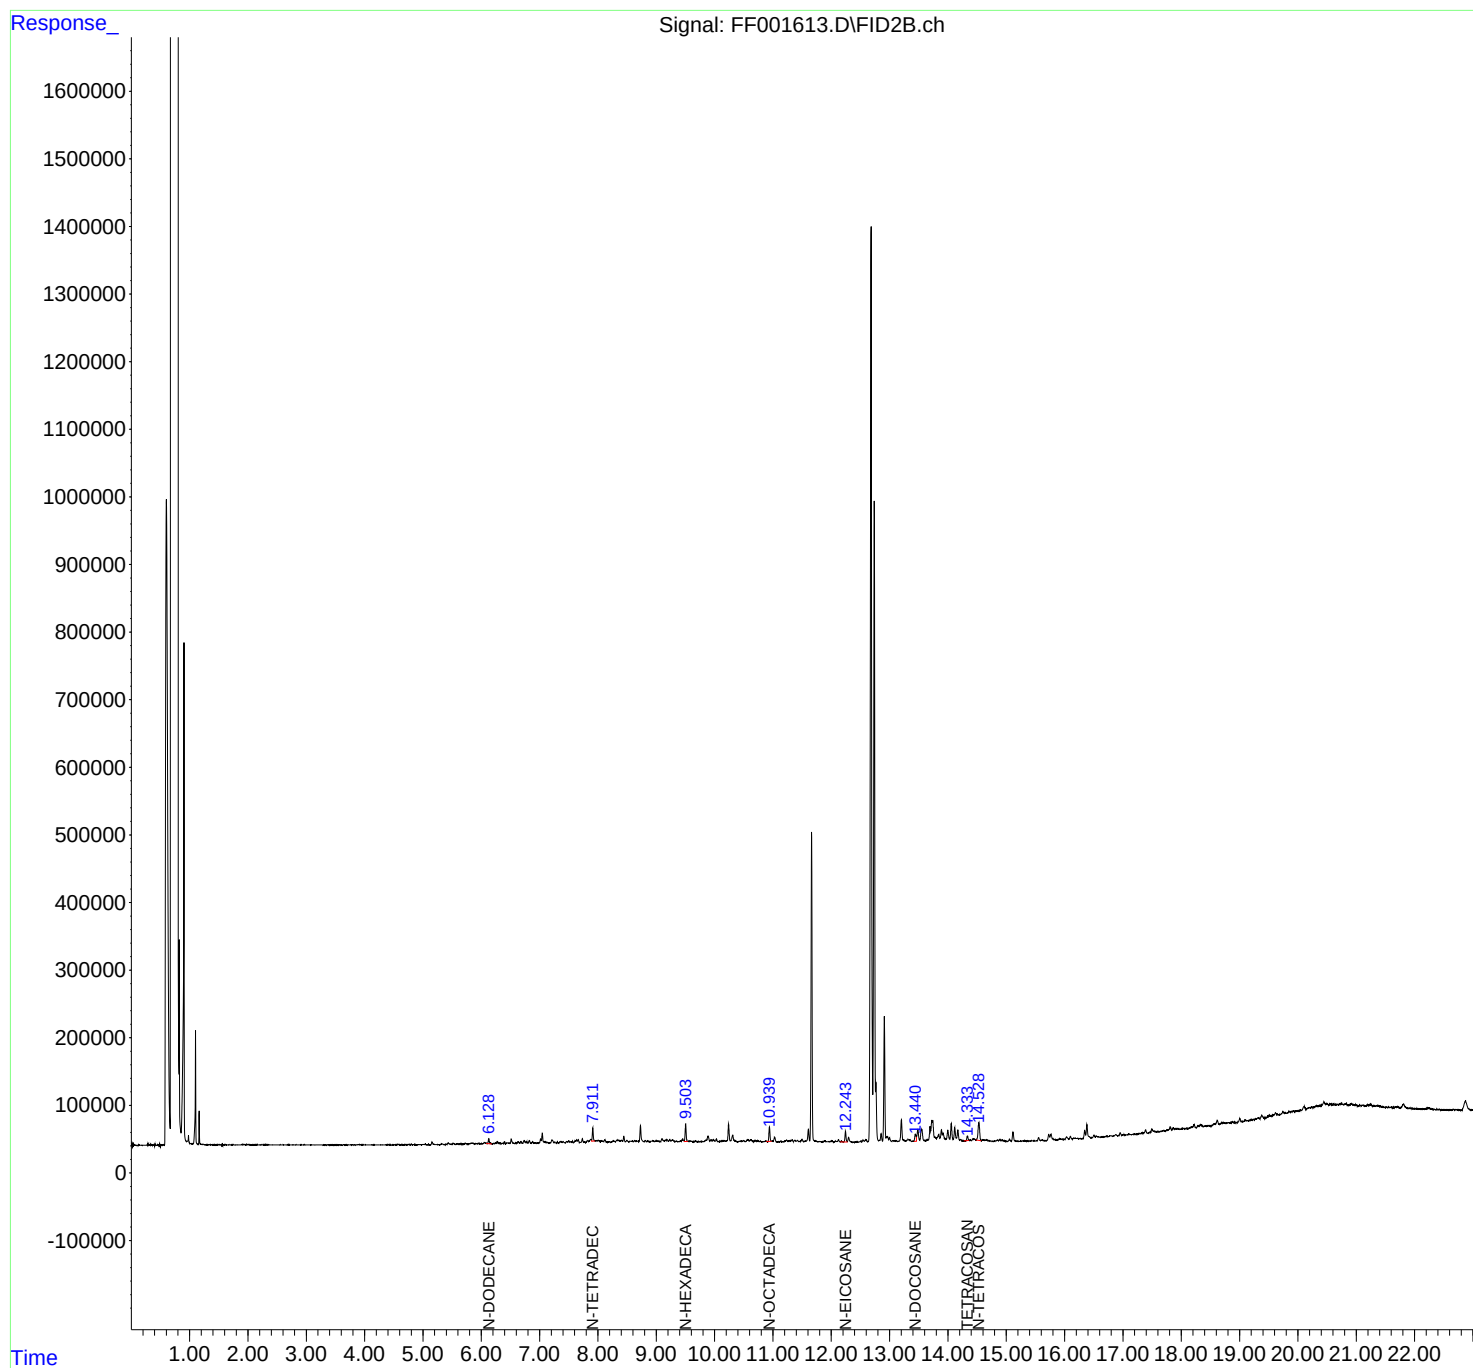


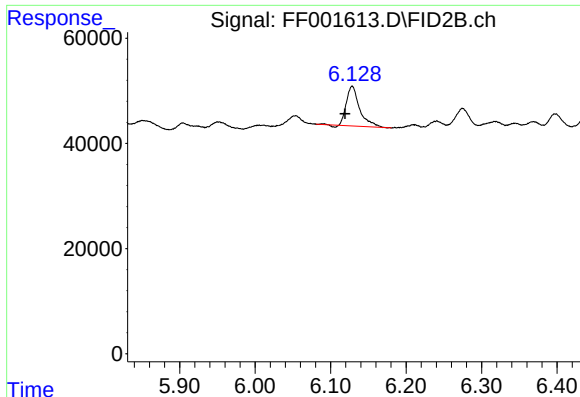

#3 N-DODECANE


R.T.: 6.129 min
Delta R.T.: 0.010 min
Response: 91398
Conc: 0.61 ug/ml

Instrument :
FID_F
ClientSampleId :

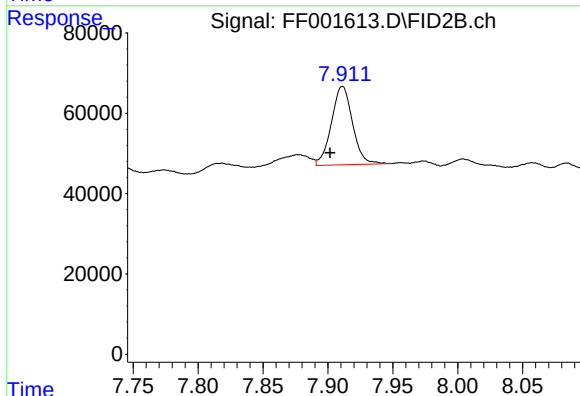


#4 N-TETRADECANE

R.T.: 7.911 min
Delta R.T.: 0.009 min
Response: 220769
Conc: 1.47 ug/ml

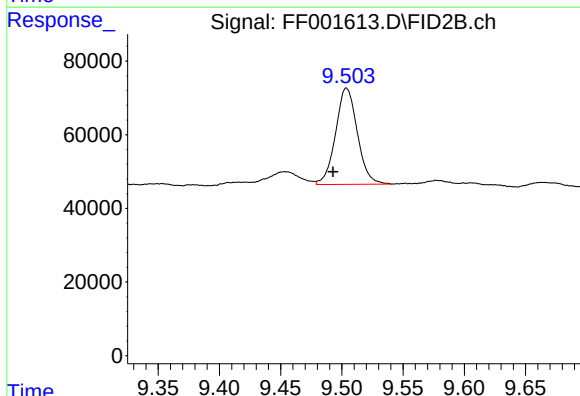


#5 N-HEXADECANE

R.T.: 9.504 min
Delta R.T.: 0.011 min
Response: 323480
Conc: 2.17 ug/ml

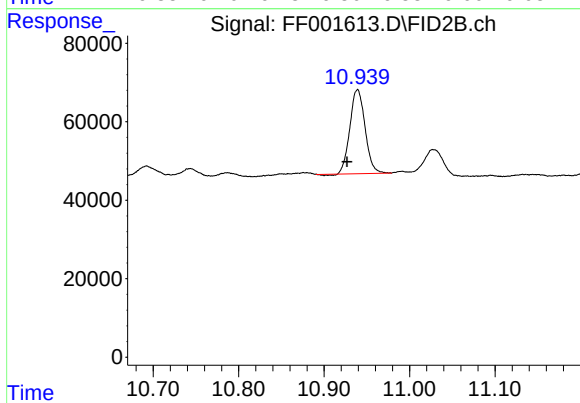

#6 N-OCTADECANE


R.T.: 10.939 min
Delta R.T.: 0.012 min
Response: 264259
Conc: 1.77 ug/ml

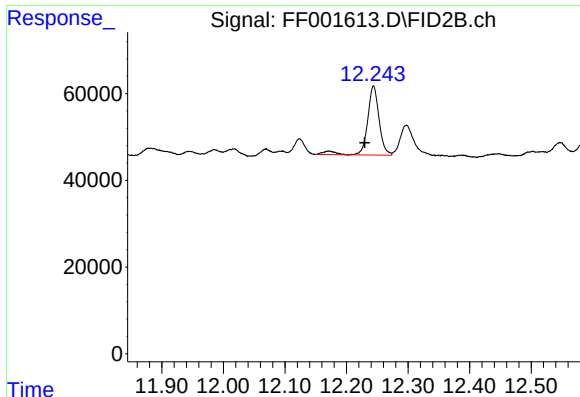

#7 N-EICOSANE


R.T.: 12.244 min
Delta R.T.: 0.014 min
Response: 213059
Conc: 1.44 ug/ml

Instrument :
FID_F
ClientSampleId :

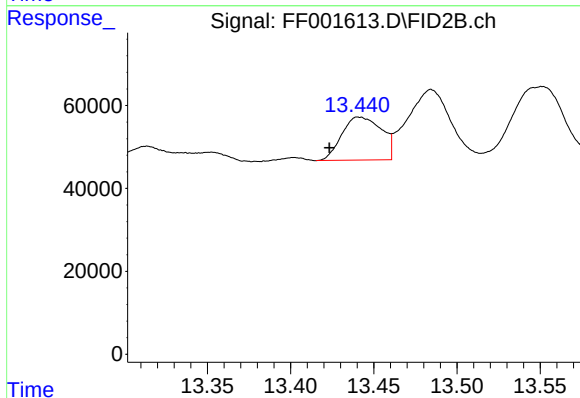


#8 N-DOCOSANE

R.T.: 13.441 min
Delta R.T.: 0.018 min
Response: 172421
Conc: 1.19 ug/ml

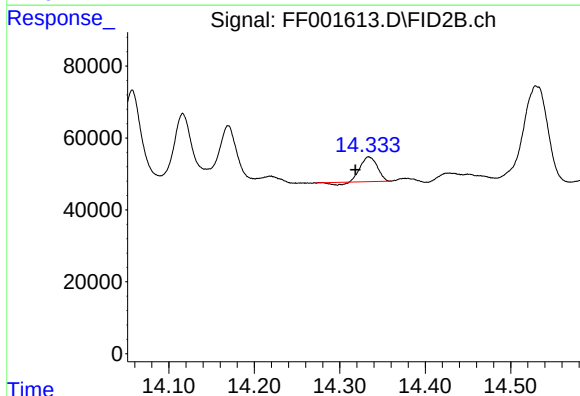

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.334 min
Delta R.T.: 0.016 min
Response: 88375
Conc: 0.70 ug/ml

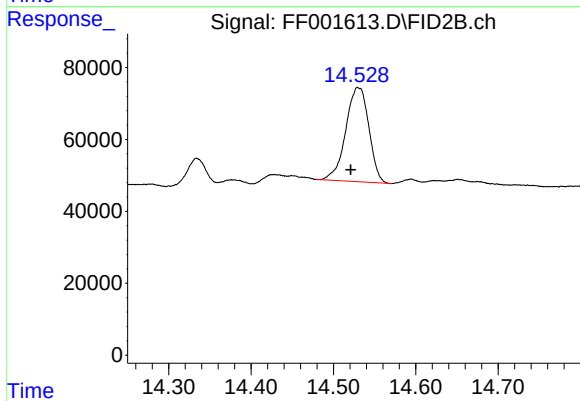

#10 N-TETRACOSANE

R.T.: 14.530 min
Delta R.T.: 0.009 min
Response: 510494
Conc: 3.60 ug/ml