

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
 Data File : FF001614.D
 Signal(s) : FID2B.ch
 Acq On : 01 Aug 2018 11:27
 Operator : AJ\SJ
 Sample : J4231-17 2X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 01 13:07:26 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Mon Jul 30 13:23:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.336	1003744	7.988 ug/ml
Target Compounds			
5) N-HEXADECANE	9.504	320494	2.146 ug/ml
7) N-EICOSANE	12.233	224804	1.522 ug/ml
8) N-DOCOSANE	13.415	232950	1.607 ug/ml
10) N-TETRACOSANE	14.497	1483003	10.461 ug/ml
11) N-HEXACOSANE	15.556	179739	1.284 ug/ml
12) N-OCTACOSANE	16.500	380853	2.745 ug/ml
13) N-TRIACONTANE	17.389	307888	2.252 ug/ml
14) N-DOTRIACONTANE	18.219	209008	1.628 ug/ml
15) N-TETRATRIACONTANE	19.003	162200	1.357 ug/ml
16) N-HEXATRIACONTANE	19.740	130870	1.183 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
Data File : FF001614.D
Signal(s) : FID2B.ch
Acq On : 01 Aug 2018 11:27
Operator : AJ\SJ
Sample : J4231-17 2X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 13:07:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Mon Jul 30 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

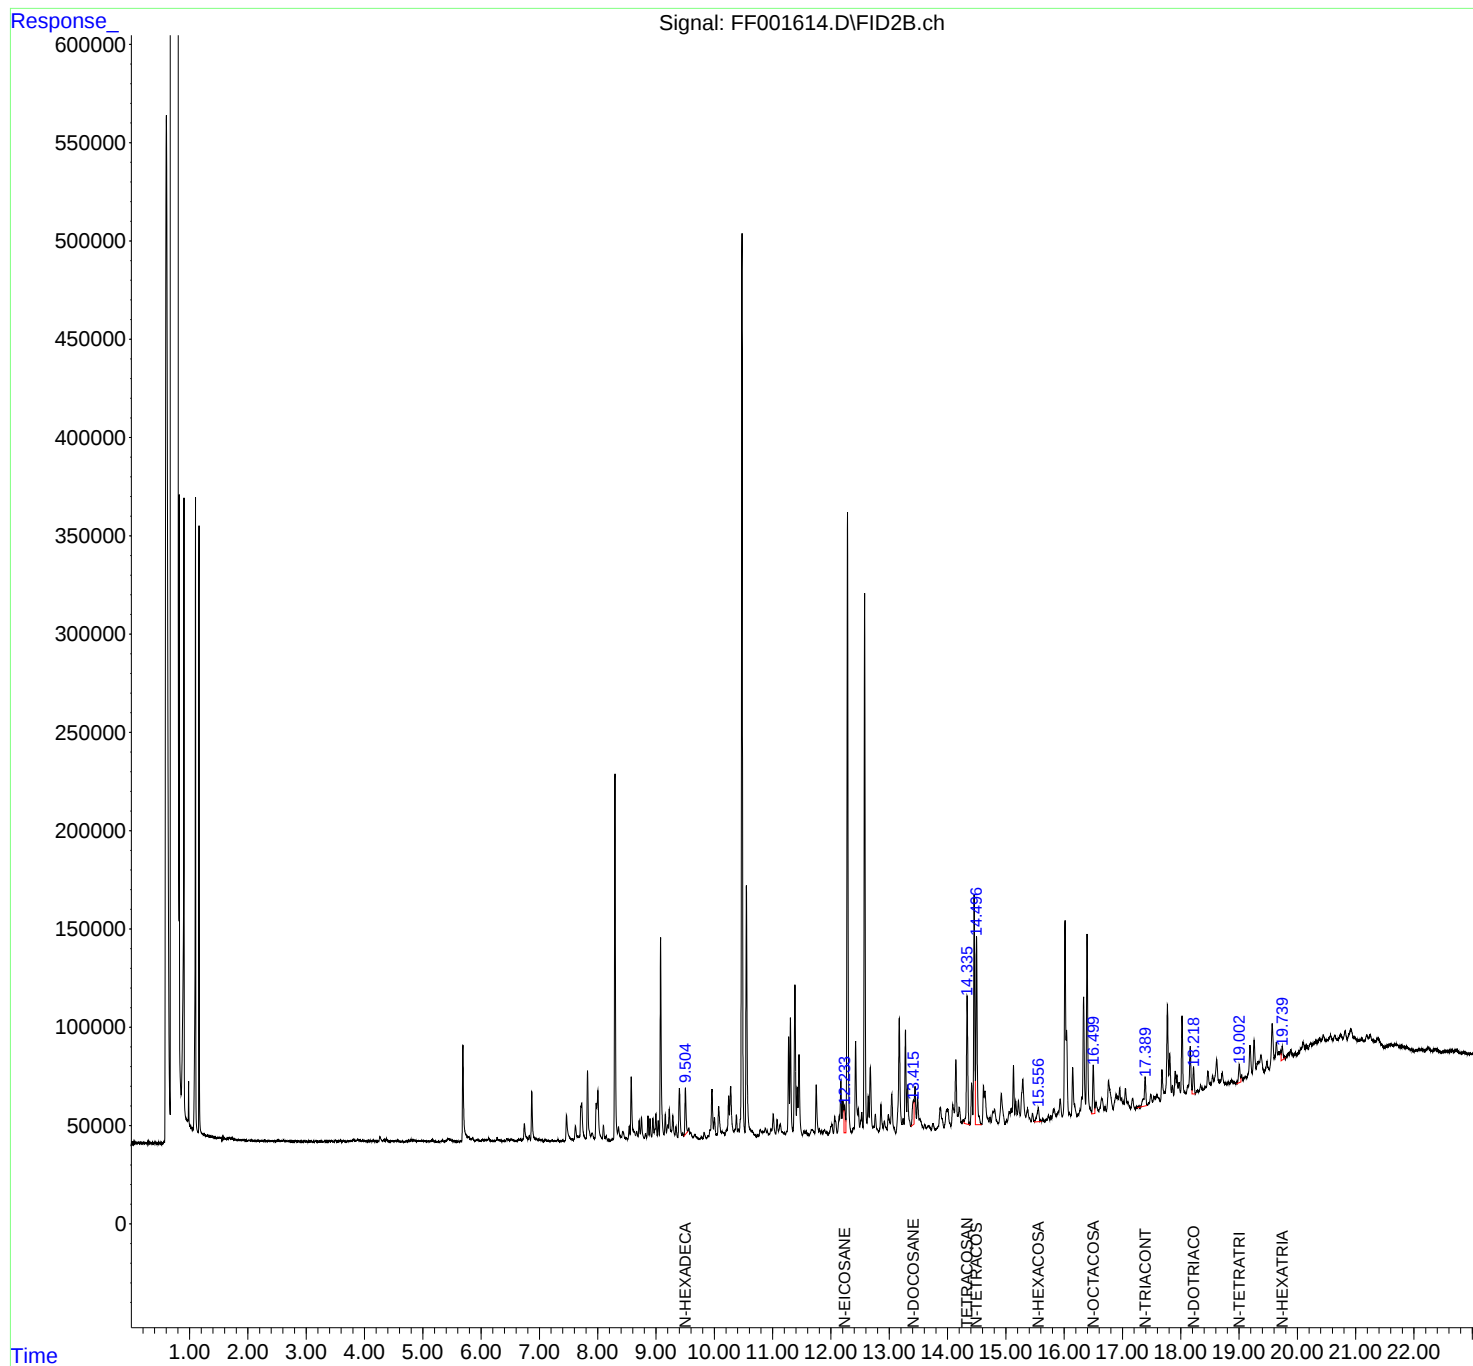


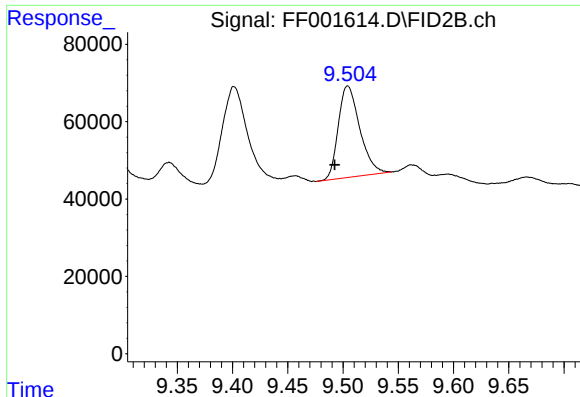

#5 N-HEXADECANE


R.T.: 9.504 min
Delta R.T.: 0.012 min
Response: 320494
Conc: 2.15 ug/ml

Instrument :
FID_F
ClientSampleId :

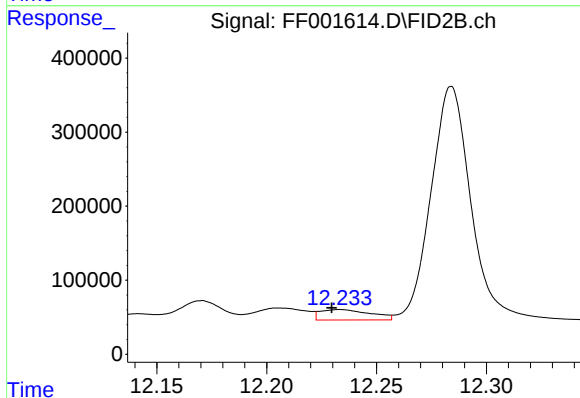


#7 N-EICOSANE

R.T.: 12.233 min
Delta R.T.: 0.004 min
Response: 224804
Conc: 1.52 ug/ml

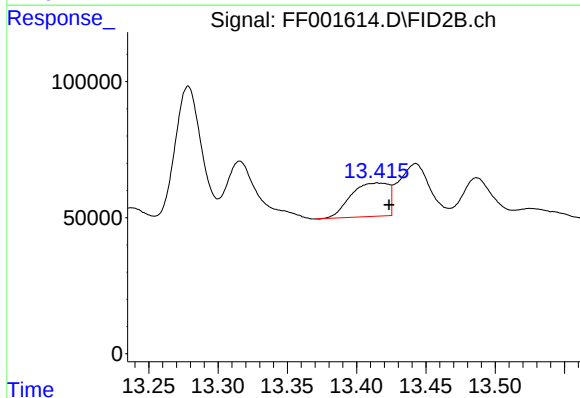


#8 N-DOCOSANE

R.T.: 13.415 min
Delta R.T.: -0.008 min
Response: 232950
Conc: 1.61 ug/ml

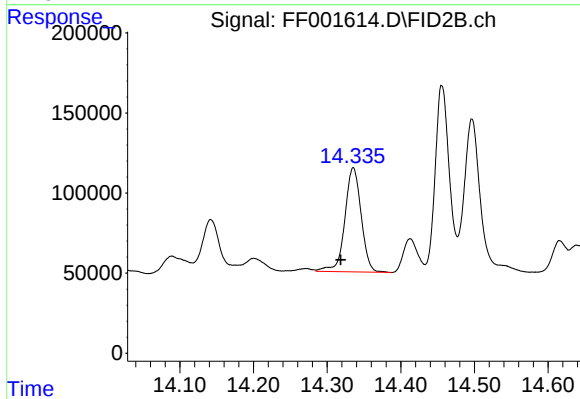

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.336 min
Delta R.T.: 0.017 min
Response: 1003744
Conc: 7.99 ug/ml

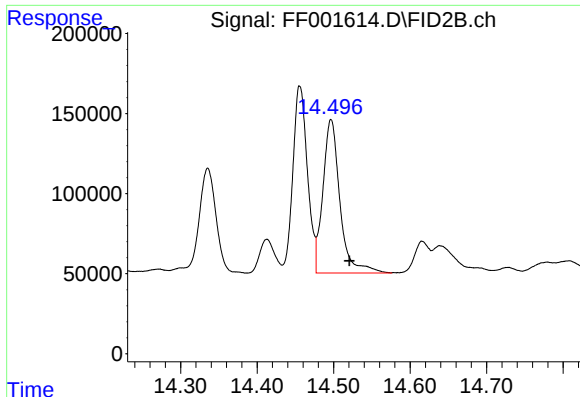

#10 N-TETRACOSANE


R.T.: 14.497 min
Delta R.T.: -0.024 min
Response: 1483003
Conc: 10.46 ug/ml

Instrument :
FID_F
ClientSampleId :

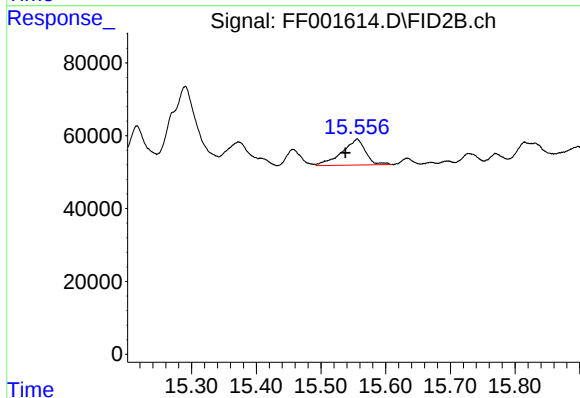


#11 N-HEXACOSANE

R.T.: 15.556 min
Delta R.T.: 0.018 min
Response: 179739
Conc: 1.28 ug/ml

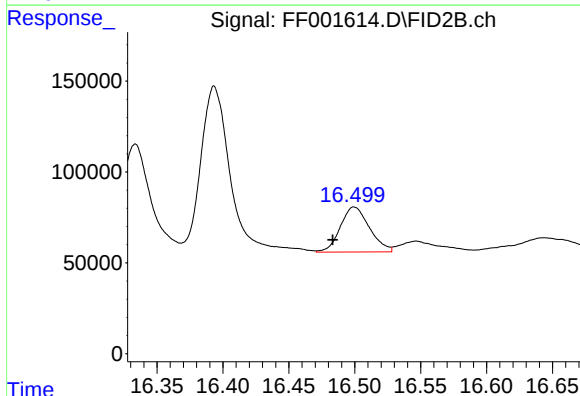


#12 N-OCTACOSANE

R.T.: 16.500 min
Delta R.T.: 0.016 min
Response: 380853
Conc: 2.74 ug/ml

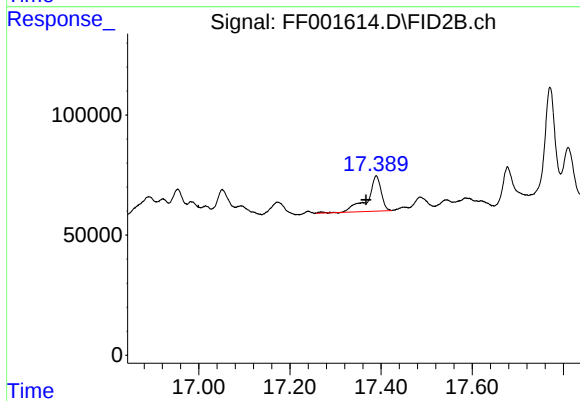

#13 N-TRIACONTANE


R.T.: 17.389 min
Delta R.T.: 0.022 min
Response: 307888
Conc: 2.25 ug/ml

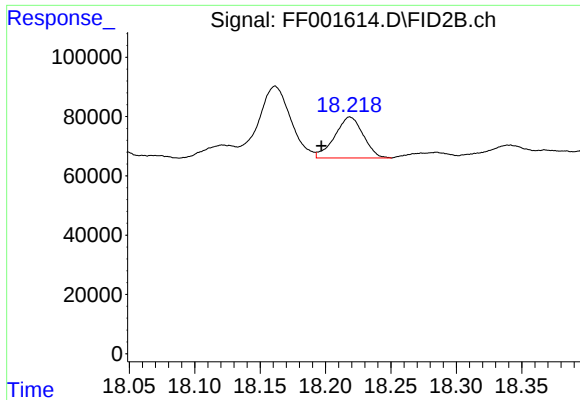

#14 N-DOTRIACONTANE


R.T.: 18.219 min
Delta R.T.: 0.022 min
Response: 209008
Conc: 1.63 ug/ml

Instrument :
FID_F
ClientSampleId :

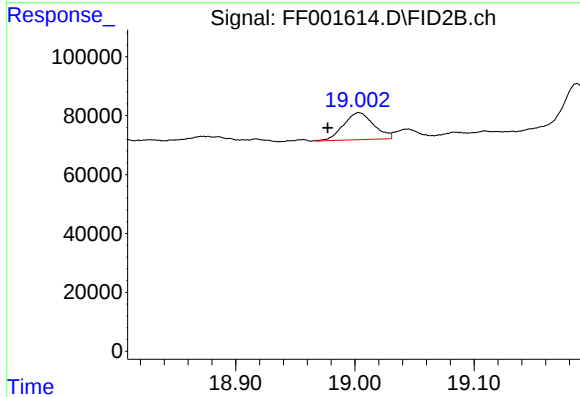

#15 N-TETRATRIACONTANE

R.T.: 19.003 min
Delta R.T.: 0.026 min
Response: 162200
Conc: 1.36 ug/ml

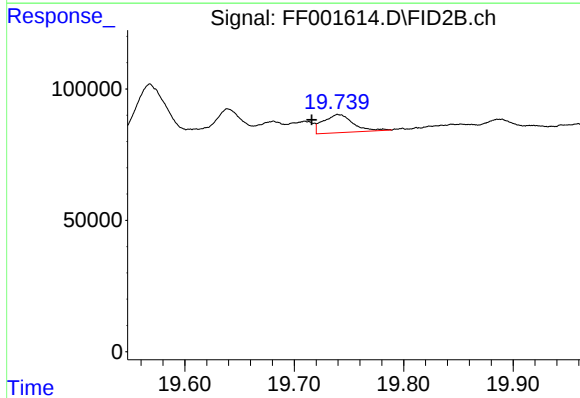

#16 N-HEXATRIACONTANE

R.T.: 19.740 min
Delta R.T.: 0.024 min
Response: 130870
Conc: 1.18 ug/ml