

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
Data File : FF001615.D
Signal(s) : FID2B.ch
Acq On : 01 Aug 2018 11:58
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 13:07:35 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Mon Jul 30 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.337	2458307	19.565 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.220	119168	0.928 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080118\
Data File : FF001615.D
Signal(s) : FID2B.ch
Acq On : 01 Aug 2018 11:58
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 13:07:35 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Mon Jul 30 13:23:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

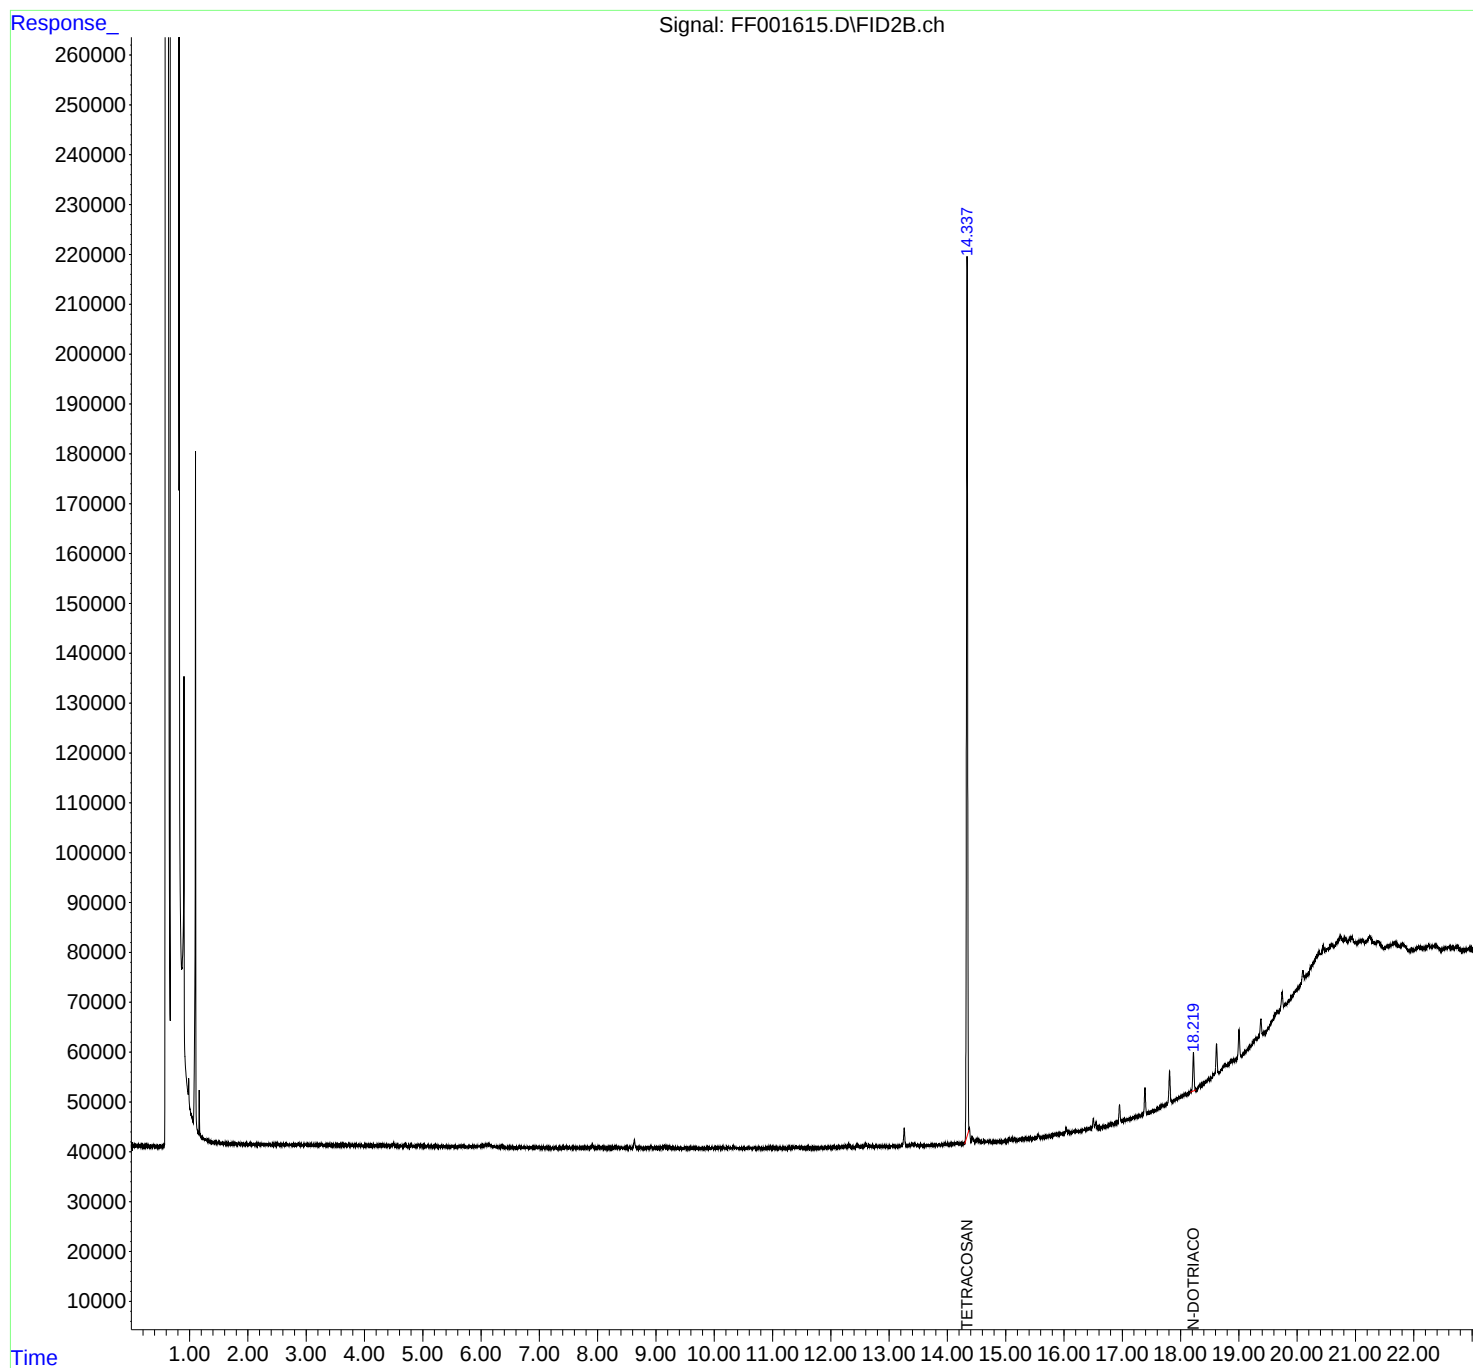


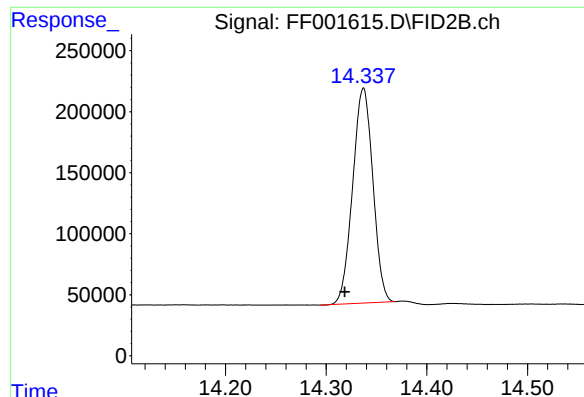

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.337 min
Delta R.T.: 0.019 min
Response: 2458307
Conc: 19.56 ug/ml

Instrument :
FID_F
ClientSampleId :

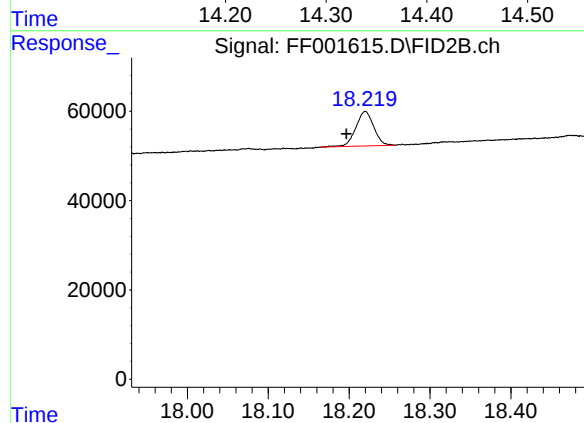

#14 N-DOTRIACONTANE

R.T.: 18.220 min
Delta R.T.: 0.023 min
Response: 119168
Conc: 0.93 ug/ml