

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080118\
 Data File : FG001910.D
 Signal(s) : FID1A.ch
 Acq On : 01 Aug 2018 07:22
 Operator : AJ\SJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 01 13:28:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
 Quant Title :
 QLast Update : Mon Jul 30 13:56:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.506	329361	2.613 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.636	97159	0.696 ug/ml
13) N-TRIACONTANE	17.524	132092	0.967 ug/ml
14) N-DOTRIACONTANE	18.355	176315	1.424 ug/ml
15) N-TETRATRIACONTANE	19.140	116628	1.073 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080118\
Data File : FG001910.D
Signal(s) : FID1A.ch
Acq On : 01 Aug 2018 07:22
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 13:28:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

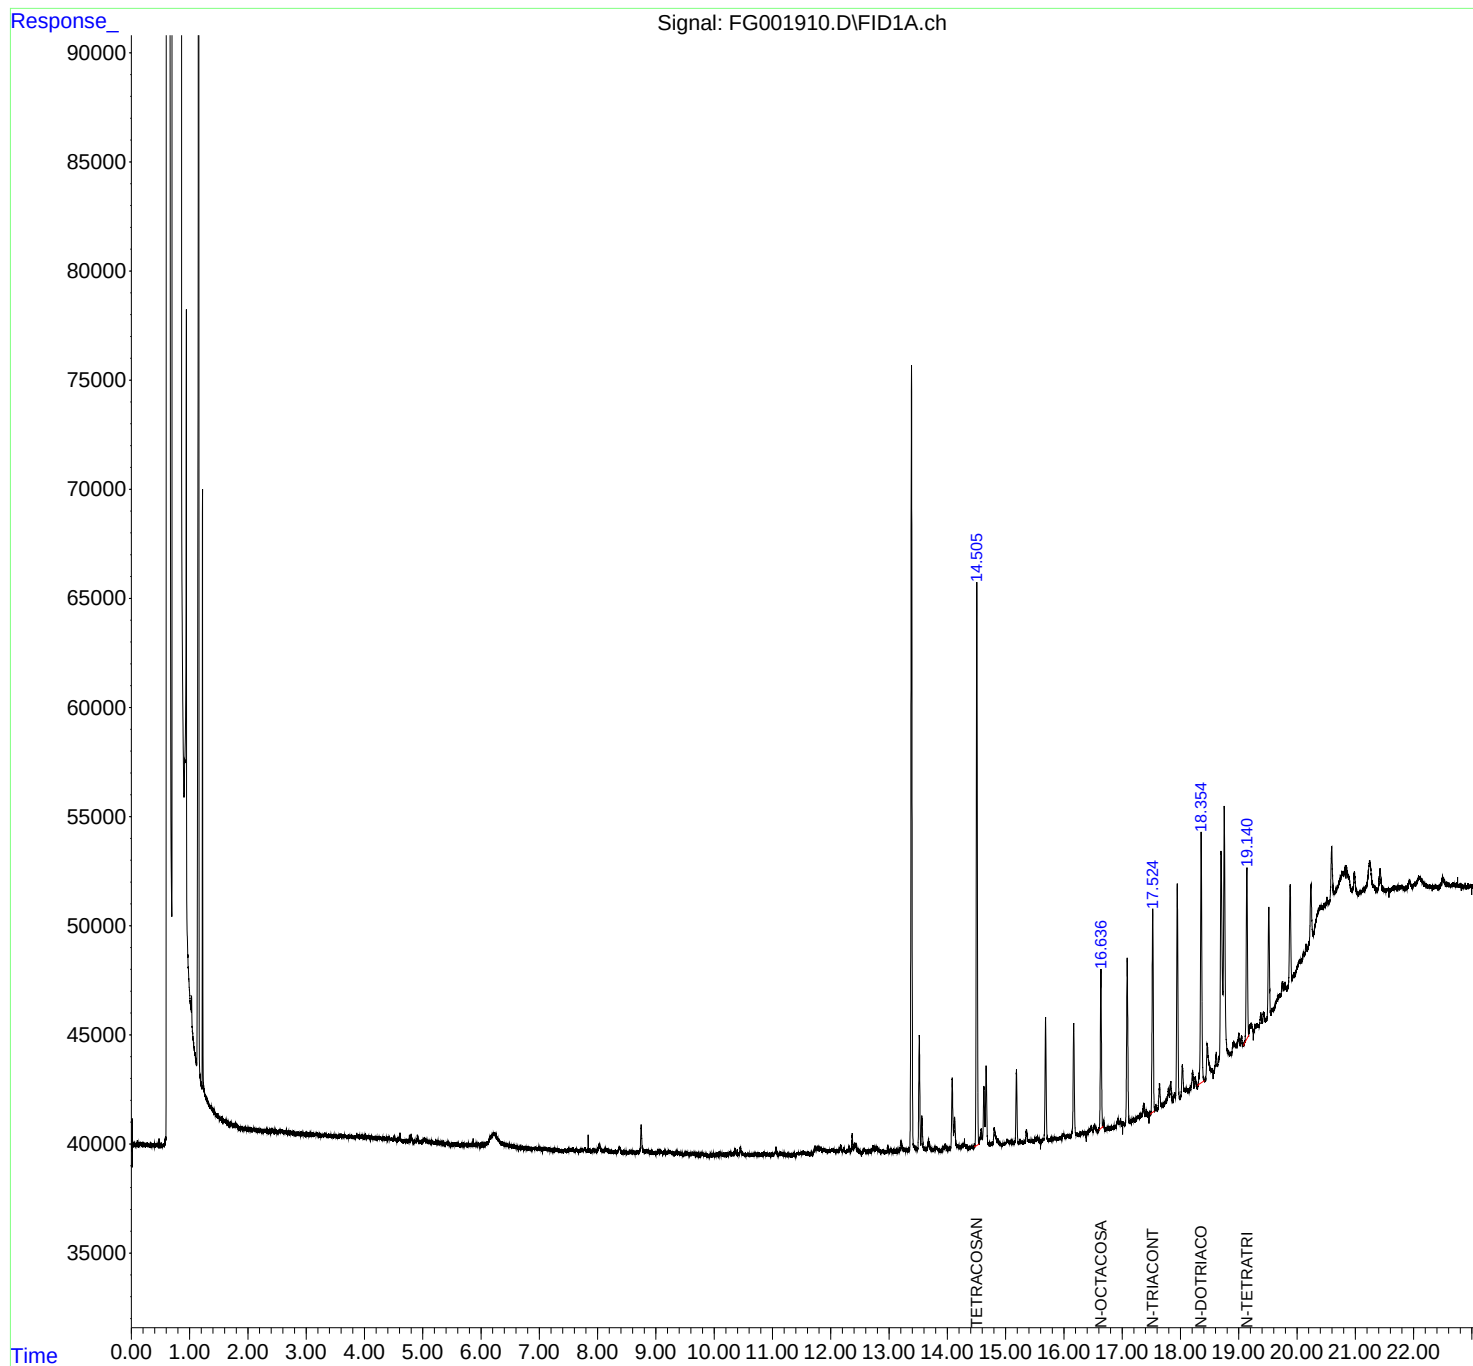


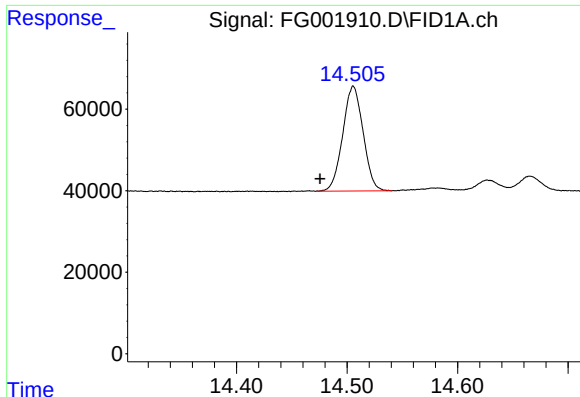

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.506 min
Delta R.T.: 0.030 min
Response: 329361
Conc: 2.61 ug/ml

Instrument :
FID_F
ClientSampleId :

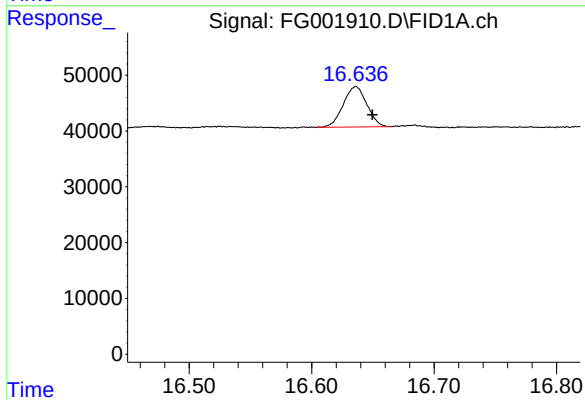


#12 N-OCTACOSANE

R.T.: 16.636 min
Delta R.T.: -0.013 min
Response: 97159
Conc: 0.70 ug/ml

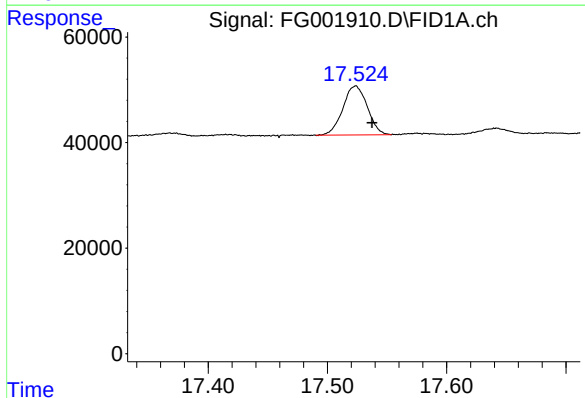


#13 N-TRIACONTANE

R.T.: 17.524 min
Delta R.T.: -0.014 min
Response: 132092
Conc: 0.97 ug/ml

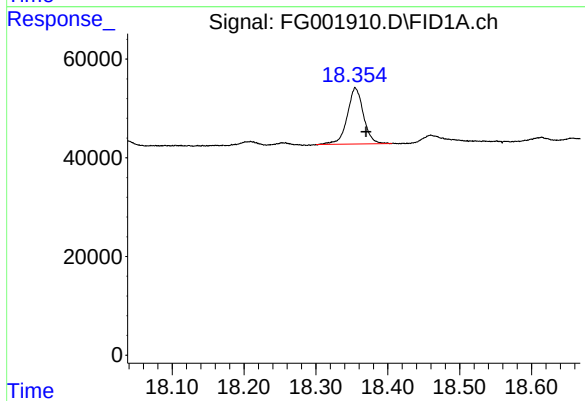

#14 N-DOTRIACONTANE

R.T.: 18.355 min
Delta R.T.: -0.015 min
Response: 176315
Conc: 1.42 ug/ml

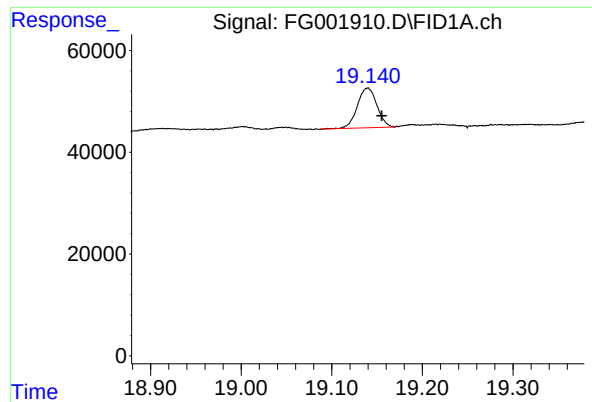

#15 N-TETRATRIACONTANE

R.T.: 19.140 min
Delta R.T.: -0.016 min
Response: 116628
Conc: 1.07 ug/ml

Instrument :
FID_F
ClientSampleId :