

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080118\
 Data File : FG001913.D
 Signal(s) : FID1A.ch
 Acq On : 01 Aug 2018 08:54
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 01 13:28:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
 Quant Title :
 QLast Update : Mon Jul 30 13:56:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.236	2650235	17.641 ug/ml
12) N-OCTACOSANE	16.637	2287084	16.393 ug/ml
13) N-TRIACONTANE	17.523	157483	1.153 ug/ml
14) N-DOTRIACONTANE	18.356	220367	1.779 ug/ml
15) N-TETRATRIACONTANE	19.142	204918	1.885 ug/ml
16) N-HEXATRIACONTANE	19.884	209716	2.183 ug/ml
17) N-OCTATRIACONTANE	20.596	277849	3.298 ug/ml
18) N-TETRACONTANE	21.428	431310	5.200 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080118\
Data File : FG001913.D
Signal(s) : FID1A.ch
Acq On : 01 Aug 2018 08:54
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 13:28:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

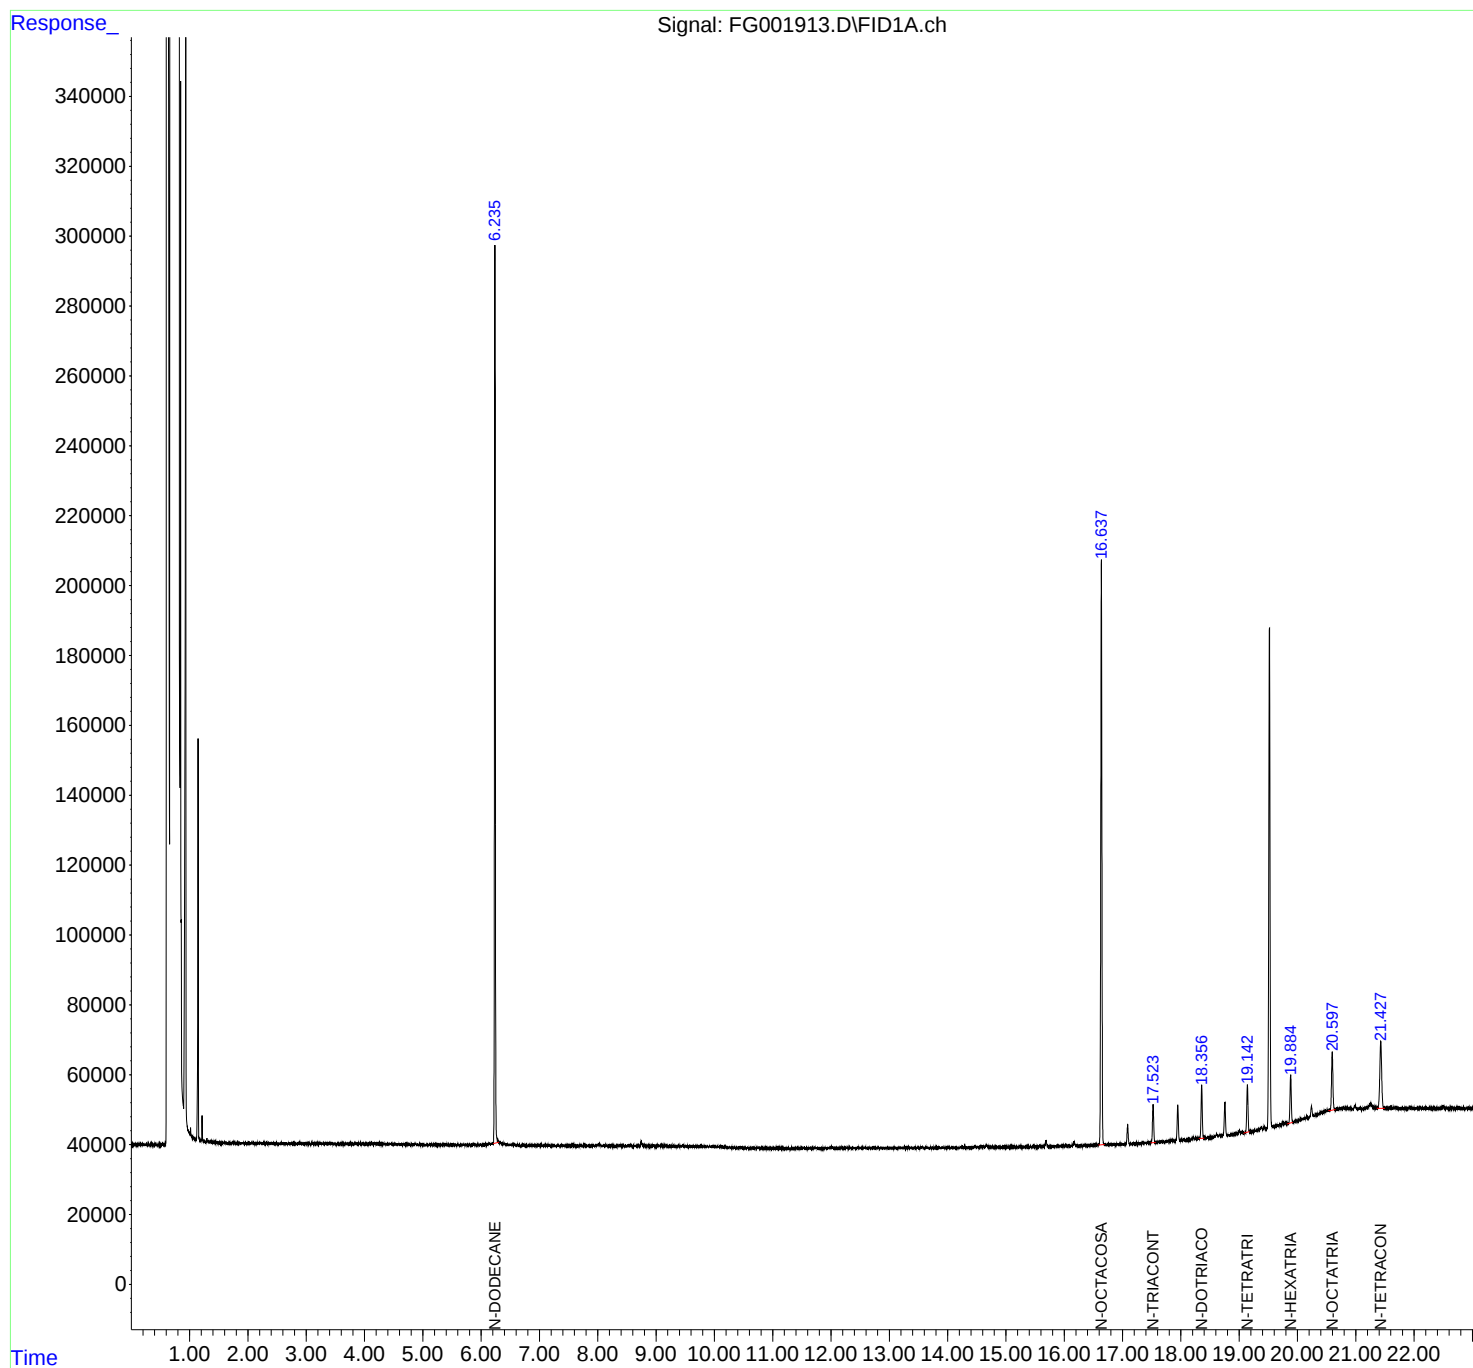


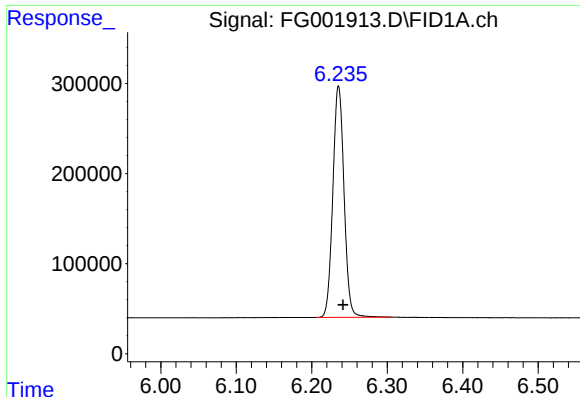

#3 N-DODECANE


R.T.: 6.236 min
Delta R.T.: -0.006 min
Response: 2650235
Conc: 17.64 ug/ml

Instrument :
FID_F
ClientSampleId :

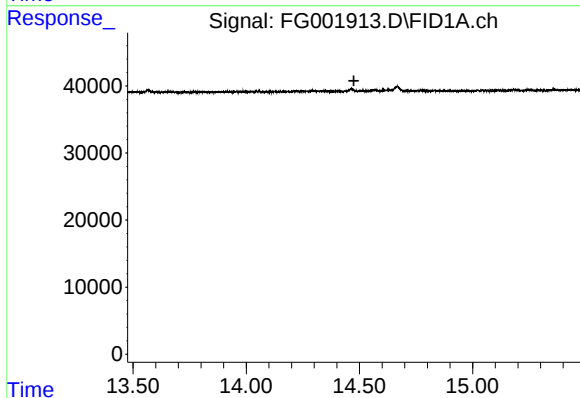


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.475 min
Response: 0
Conc: N.D.

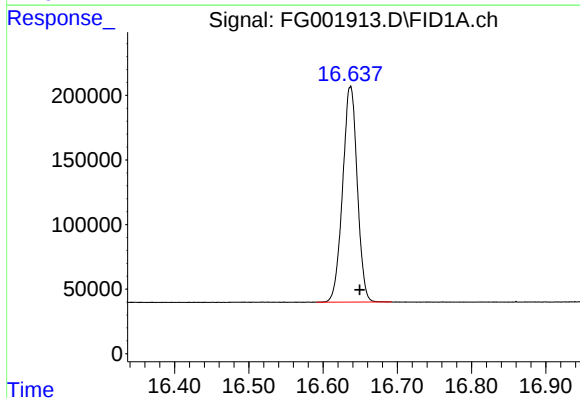


#12 N-OCTACOSANE

R.T.: 16.637 min
Delta R.T.: -0.013 min
Response: 2287084
Conc: 16.39 ug/ml

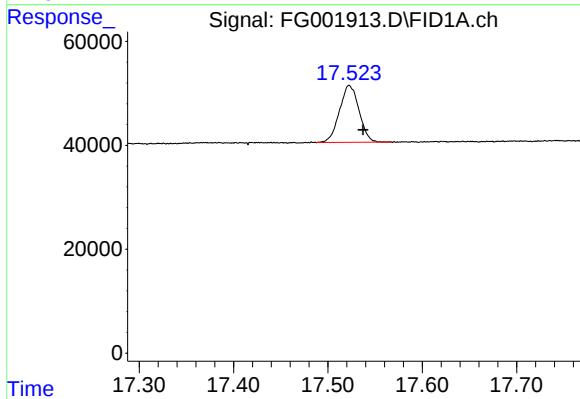

#13 N-TRIACONTANE


R.T.: 17.523 min
Delta R.T.: -0.015 min
Response: 157483
Conc: 1.15 ug/ml

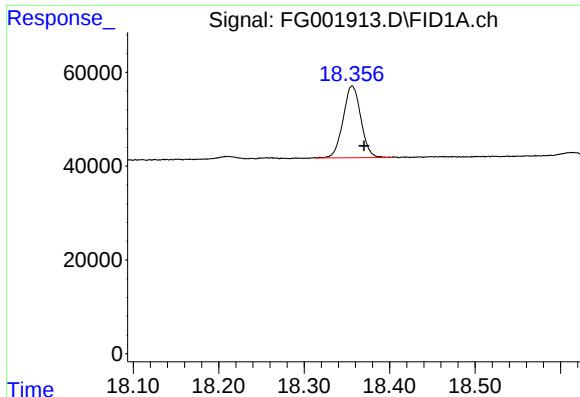

#14 N-DOTRIACONTANE


R.T.: 18.356 min
Delta R.T.: -0.014 min
Response: 220367
Conc: 1.78 ug/ml

Instrument :
FID_F
ClientSampleId :

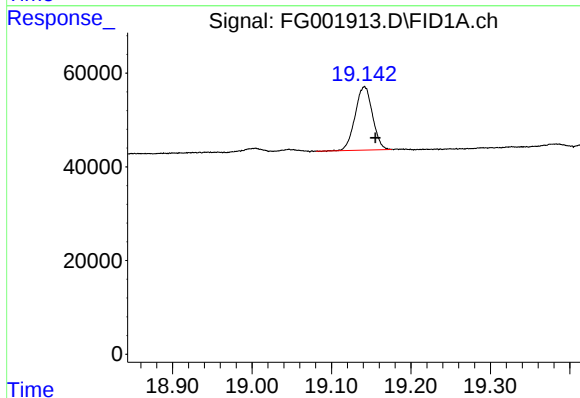


#15 N-TETRATRIACONTANE

R.T.: 19.142 min
Delta R.T.: -0.014 min
Response: 204918
Conc: 1.88 ug/ml

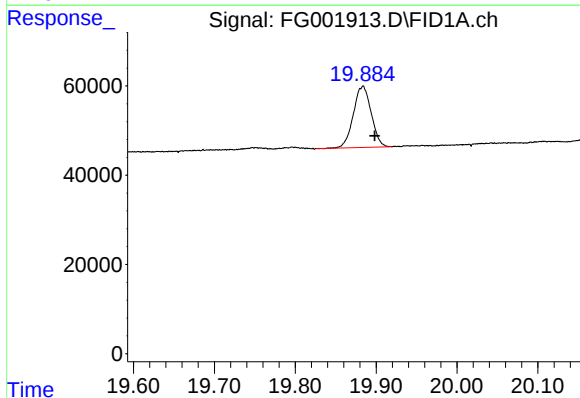


#16 N-HEXATRIACONTANE

R.T.: 19.884 min
Delta R.T.: -0.015 min
Response: 209716
Conc: 2.18 ug/ml

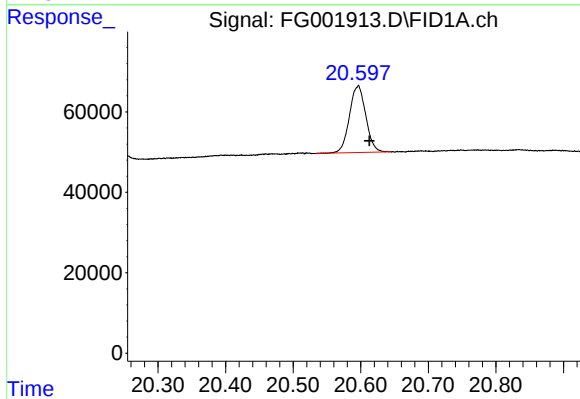

#17 N-OCTATRIACONTANE

R.T.: 20.596 min
Delta R.T.: -0.016 min
Response: 277849
Conc: 3.30 ug/ml

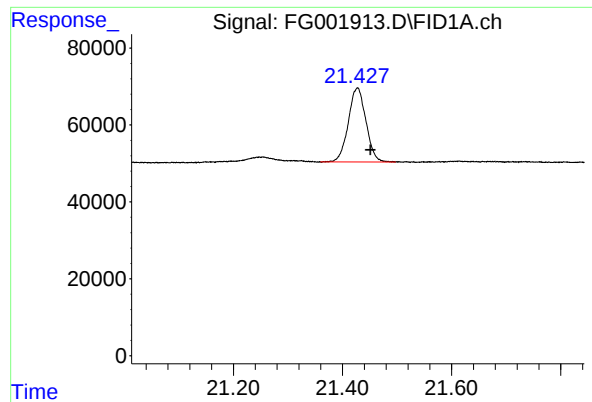

#18 N-TETRACONTANE

R.T.: 21.428 min
Delta R.T.: -0.023 min
Response: 431310
Conc: 5.20 ug/ml

Instrument :
FID_F
ClientSampleId :