

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080224\
 Data File : FF014377.D
 Signal(s) : FID2B.ch
 Acq On : 02 Aug 2024 16:31
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 03 02:15:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072324.M
 Quant Title :
 QLast Update : Tue Jul 23 14:43:21 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) N-HEXACOSANE	16.144	102871	0.800 ug/ml
12) N-OCTACOSANE	17.088	83423	0.664 ug/ml
13) N-TRIACONTANE	17.985	451678	3.702 ug/ml
14) N-DOTRIACONTANE	18.795	411565	3.508 ug/ml
15) N-TETRATRIACONTANE	19.581	567085	5.956 ug/ml
16) N-HEXATRIACONTANE	20.338	363369	4.883 ug/ml
17) N-OCTATRIACONTANE	21.037	472577	7.004 ug/ml
18) N-TETRACONTANE	21.928	164931	2.622 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080224\
Data File : FF014377.D
Signal(s) : FID2B.ch
Acq On : 02 Aug 2024 16:31
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 03 02:15:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:21 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

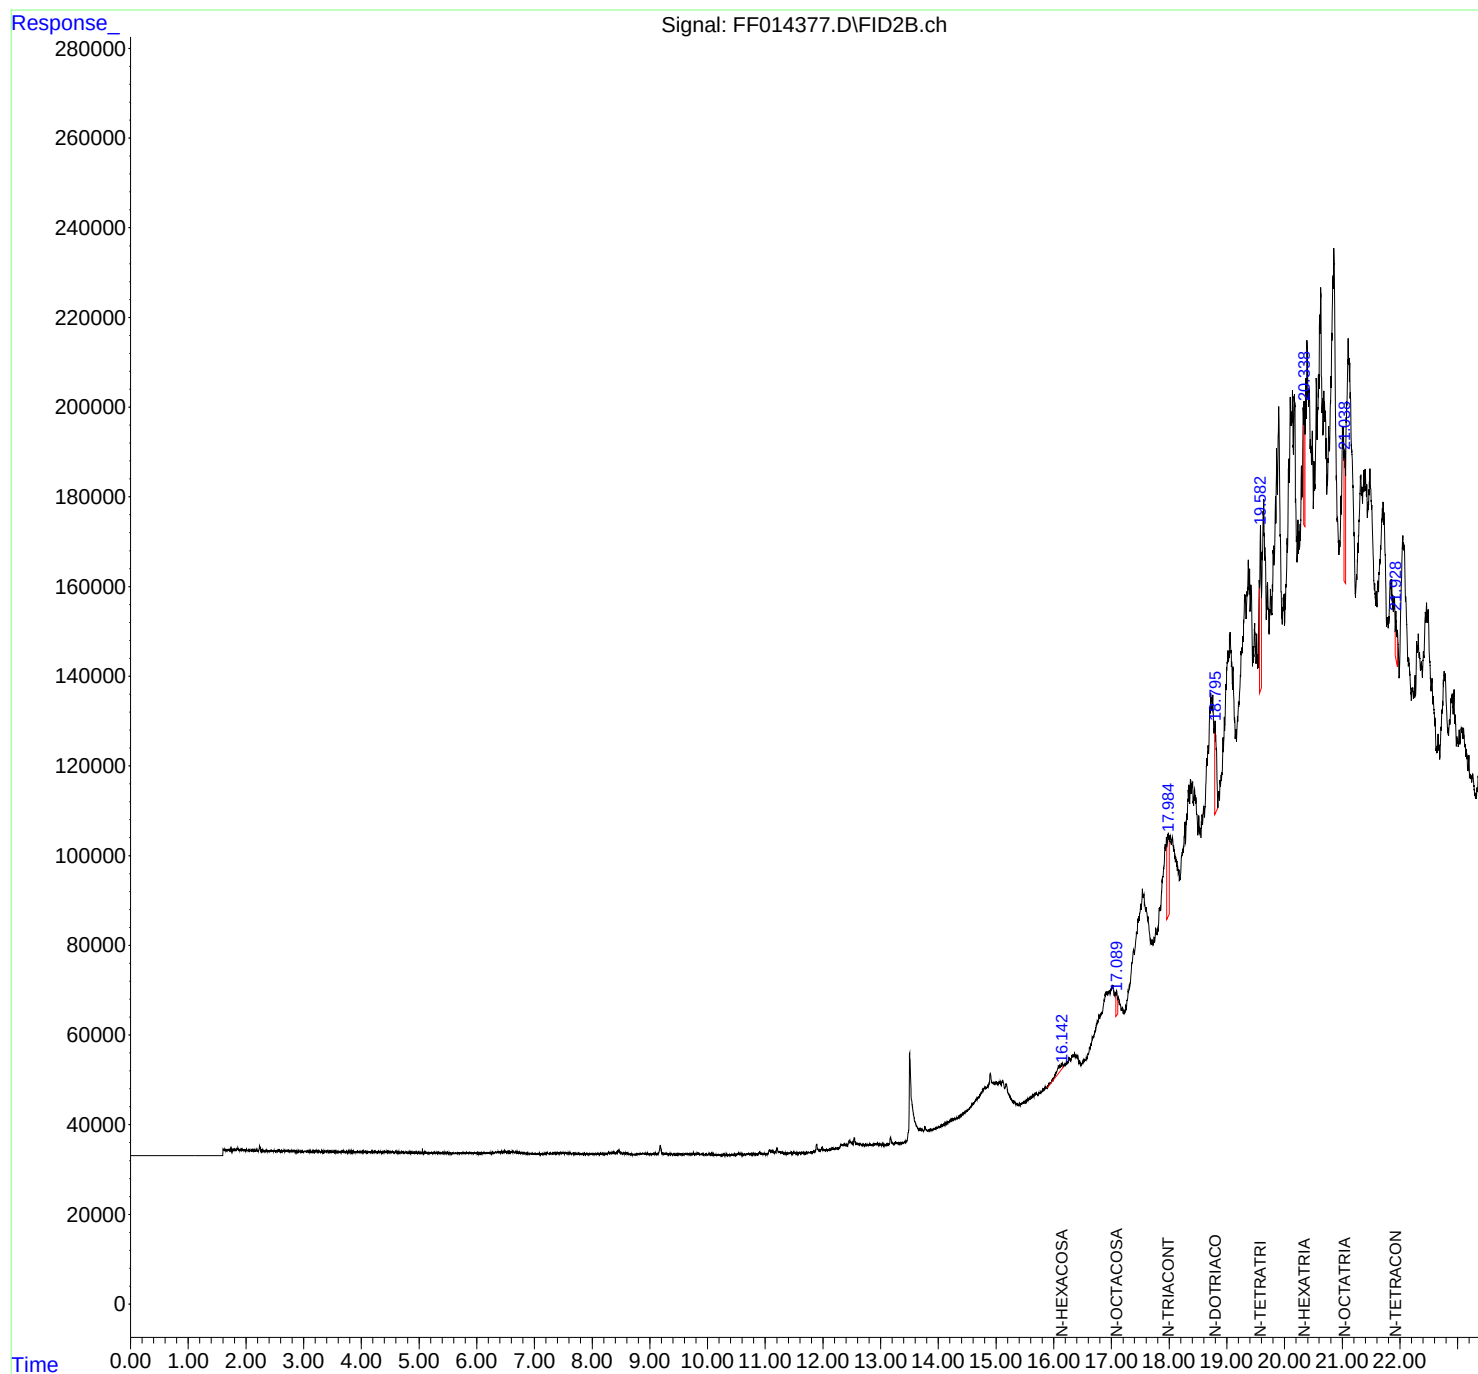


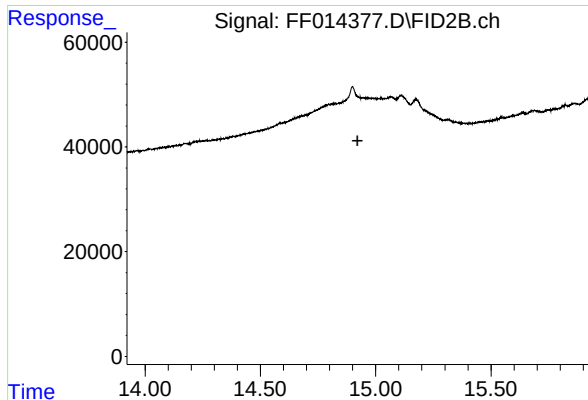

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.921 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

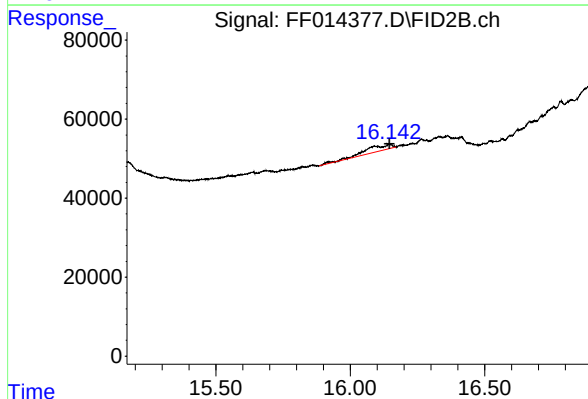


#11 N-HEXACOSANE

R.T.: 16.144 min
Delta R.T.: -0.004 min
Response: 102871
Conc: 0.80 ug/ml

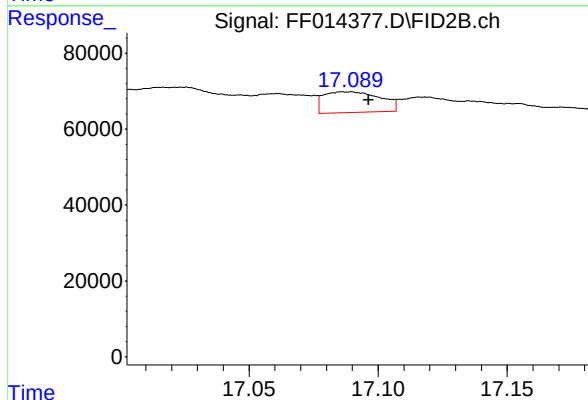


#12 N-OCTACOSANE

R.T.: 17.088 min
Delta R.T.: -0.008 min
Response: 83423
Conc: 0.66 ug/ml

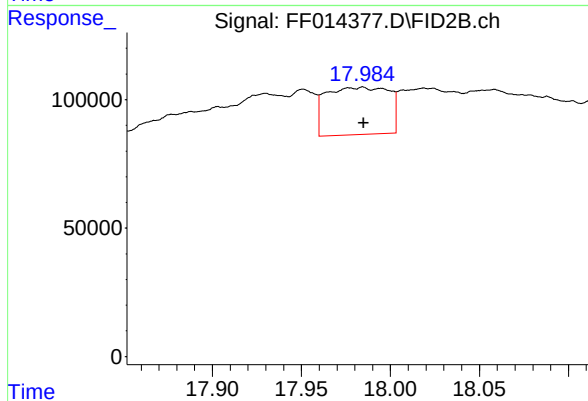

#13 N-TRIACONTANE


R.T.: 17.985 min
Delta R.T.: 0.000 min
Response: 451678
Conc: 3.70 ug/ml

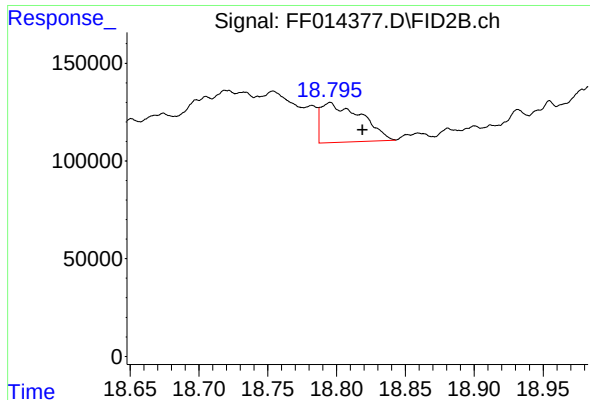

#14 N-DOTRIACONTANE


R.T.: 18.795 min
Delta R.T.: -0.024 min
Response: 411565
Conc: 3.51 ug/ml

Instrument :
FID_F
ClientSampleId :

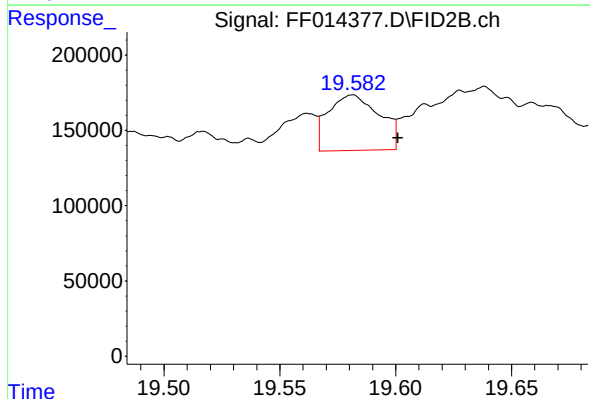


#15 N-TETRATRIACONTANE

R.T.: 19.581 min
Delta R.T.: -0.020 min
Response: 567085
Conc: 5.96 ug/ml

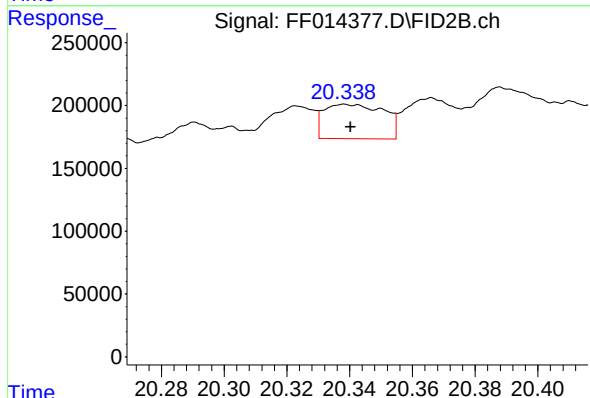


#16 N-HEXATRIACONTANE

R.T.: 20.338 min
Delta R.T.: -0.002 min
Response: 363369
Conc: 4.88 ug/ml

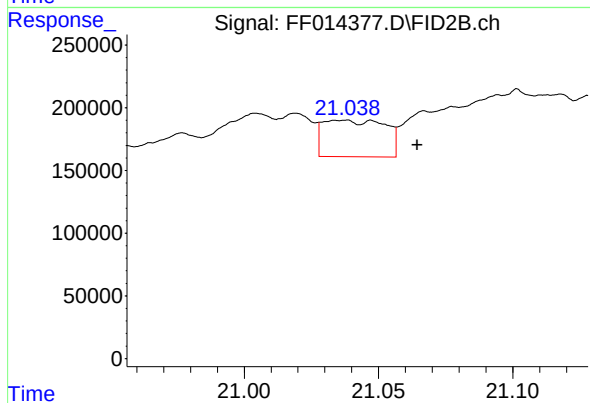

#17 N-OCTATRIACONTANE

R.T.: 21.037 min
Delta R.T.: -0.027 min
Response: 472577
Conc: 7.00 ug/ml

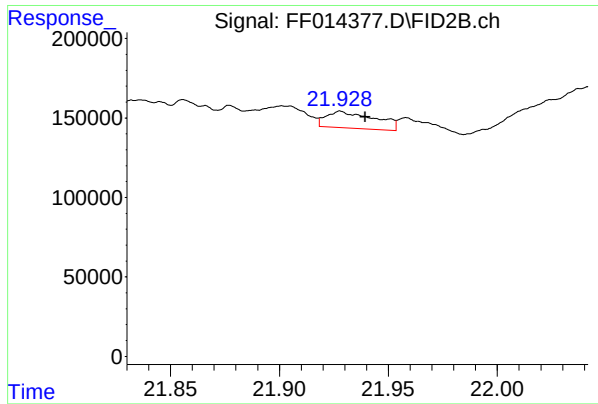

#18 N-TETRACONTANE

R.T.: 21.928 min
Delta R.T.: -0.011 min
Response: 164931
Conc: 2.62 ug/ml

Instrument :
FID_F
ClientSampleId :