

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080318\
 Data File : FF001647.D
 Signal(s) : FID2B.ch
 Acq On : 03 Aug 2018 08:45
 Operator : AJ\SJ
 Sample : J4307-06
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 03 12:38:00 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.339	1035839	8.201 ug/ml
Target Compounds			
4) N-TETRADECANE	7.971f	305471	2.027 ug/ml
7) N-EICOSANE	12.288f	844397	5.665 ug/ml
10) N-TETRACOSANE	14.504	571848	4.009 ug/ml
11) N-HEXACOSANE	15.558	116914	0.830 ug/ml
12) N-OCTACOSANE	16.508	261868	1.868 ug/ml
13) N-TRIACONTANE	17.391	399383	2.885 ug/ml
14) N-DOTRIACONTANE	18.179	272580	2.089 ug/ml
15) N-TETRATRIACONTANE	19.002	114091	0.944 ug/ml
16) N-HEXATRIACONTANE	19.703	361849	3.252 ug/ml
17) N-OCTATRIACONTANE	20.434	184951	1.856 ug/ml
18) N-TETRACONTANE	21.210	76050	0.763 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080318\
Data File : FF001647.D
Signal(s) : FID2B.ch
Acq On : 03 Aug 2018 08:45
Operator : AJ\SJ
Sample : J4307-06
Misc :
ALS Vial : 75 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 03 12:38:00 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

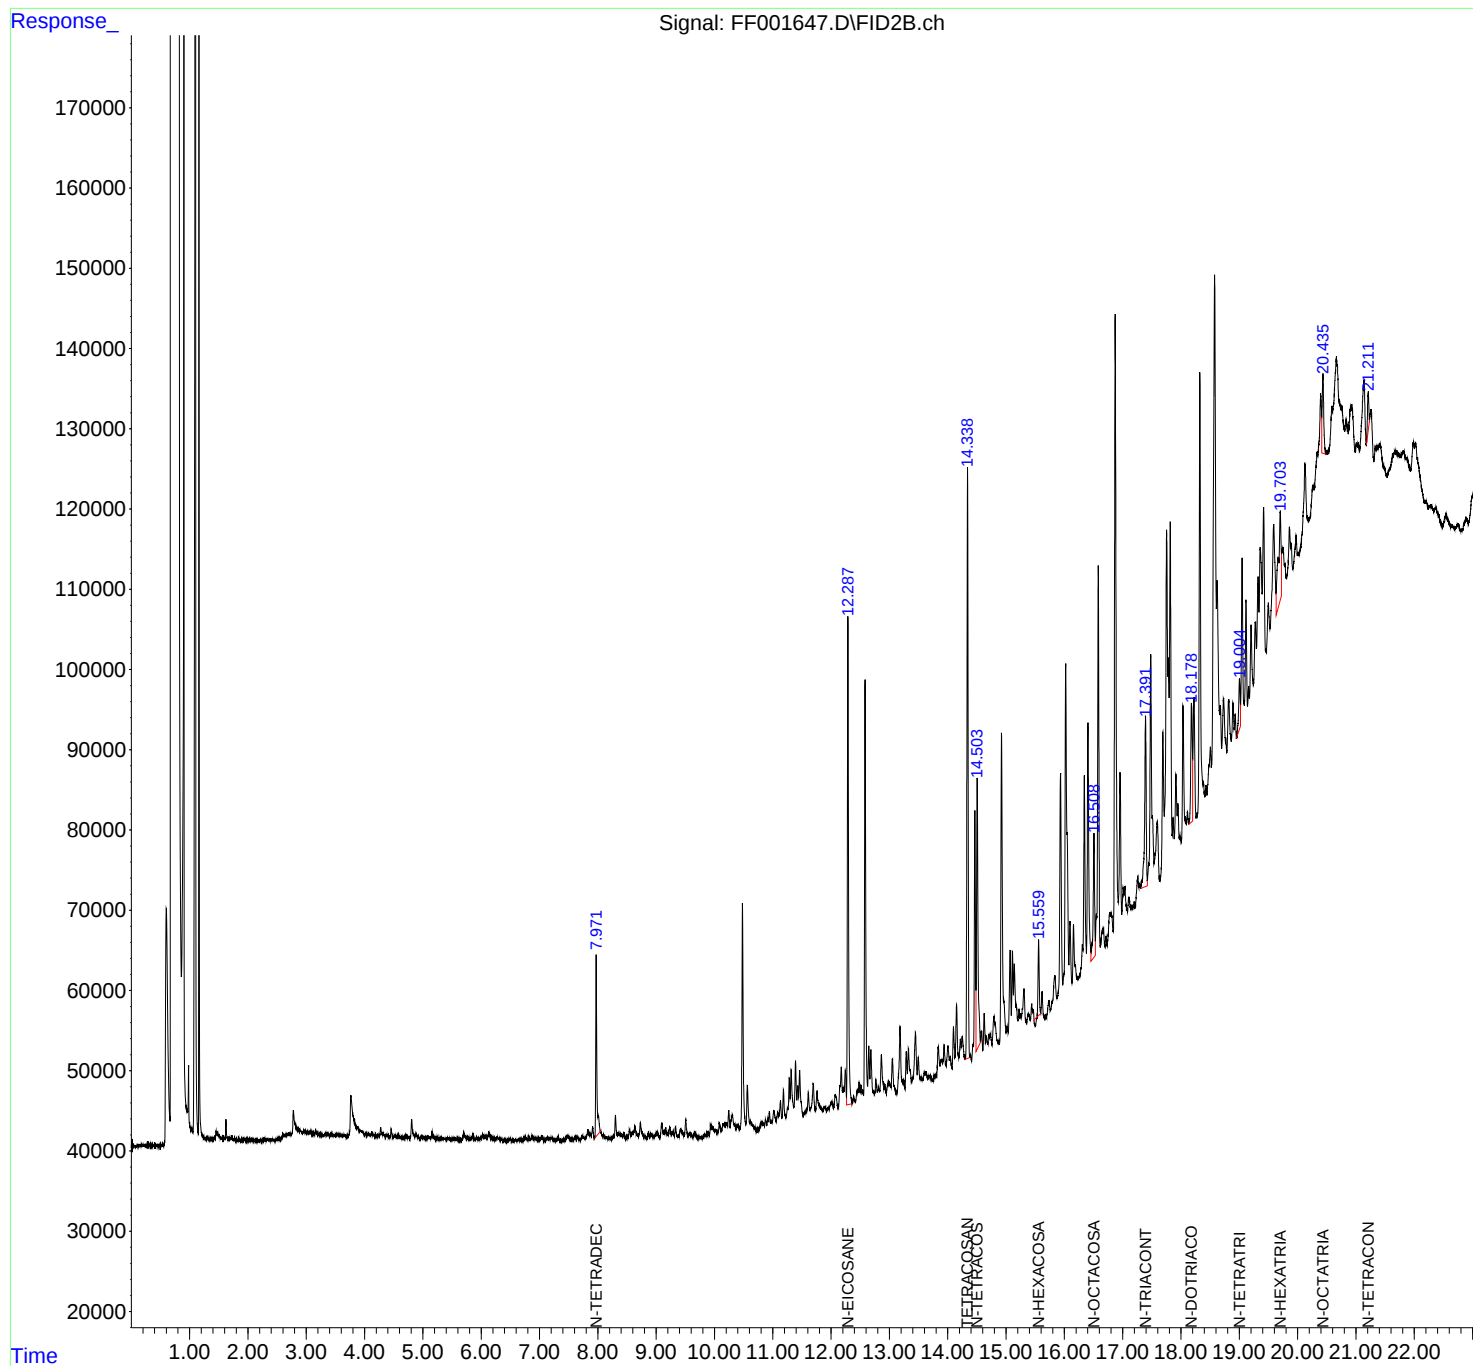

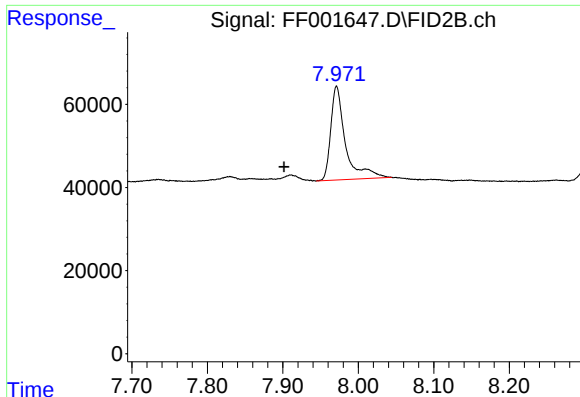


#4 N-TETRADECANE

R.T.: 7.971 min
Delta R.T.: 0.070 min
Response: 305471
Conc: 2.03 ug/ml

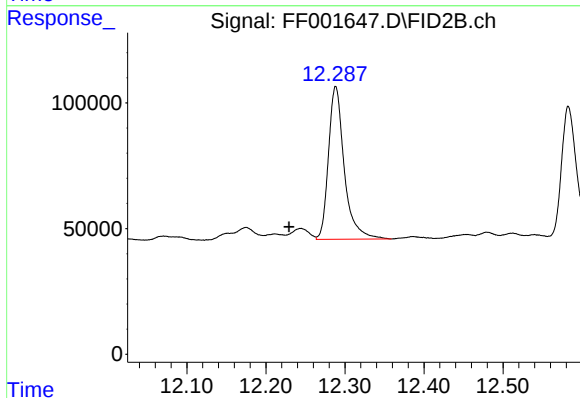


#7 N-EICOSANE

R.T.: 12.288 min
Delta R.T.: 0.059 min
Response: 844397
Conc: 5.67 ug/ml

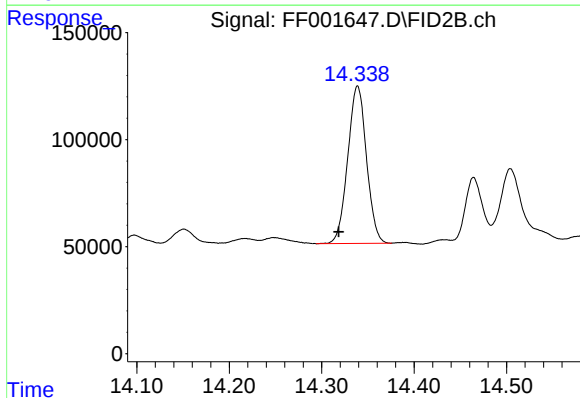


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.339 min
Delta R.T.: 0.020 min
Response: 1035839
Conc: 8.20 ug/ml

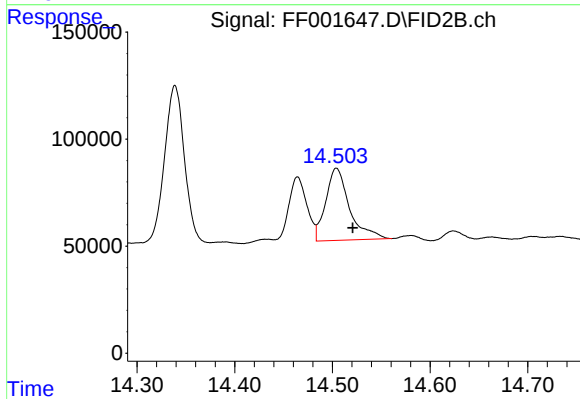


#10 N-TETRACOSANE

R.T.: 14.504 min
Delta R.T.: -0.017 min
Response: 571848
Conc: 4.01 ug/ml

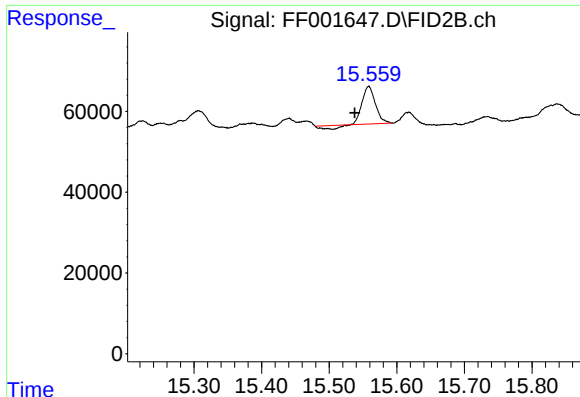


#11 N-HEXACOSANE

R.T.: 15.558 min
Delta R.T.: 0.021 min
Response: 116914
Conc: 0.83 ug/ml

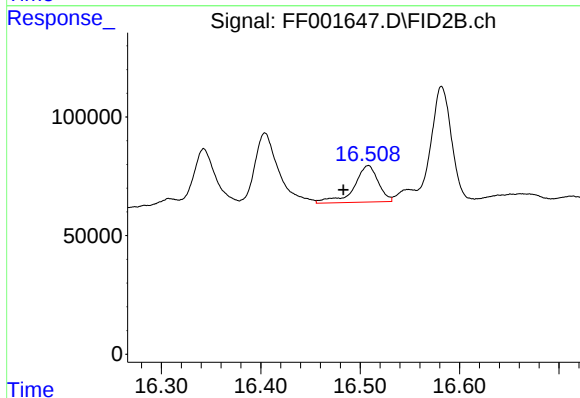


#12 N-OCTACOSANE

R.T.: 16.508 min
Delta R.T.: 0.025 min
Response: 261868
Conc: 1.87 ug/ml

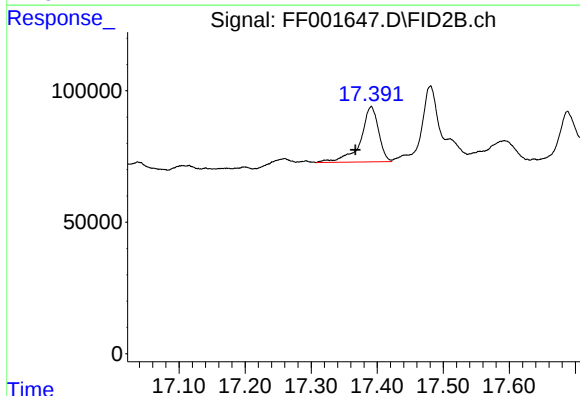


#13 N-TRIACONTANE

R.T.: 17.391 min
Delta R.T.: 0.024 min
Response: 399383
Conc: 2.88 ug/ml

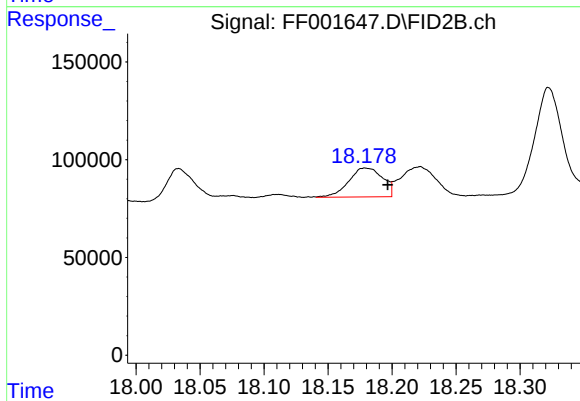


#14 N-DOTRIACONTANE

R.T.: 18.179 min
Delta R.T.: -0.018 min
Response: 272580
Conc: 2.09 ug/ml

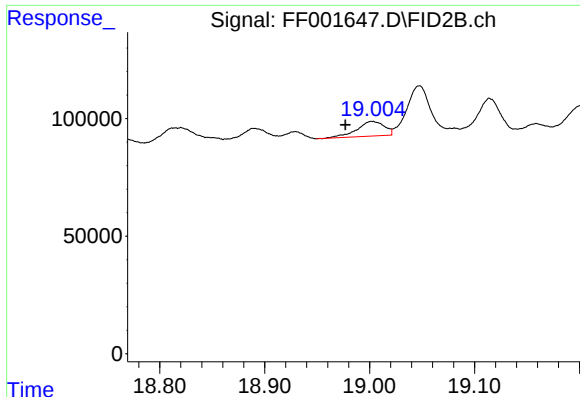


#15 N-TETRATRIACONTANE

R.T.: 19.002 min
Delta R.T.: 0.025 min
Response: 114091
Conc: 0.94 ug/ml

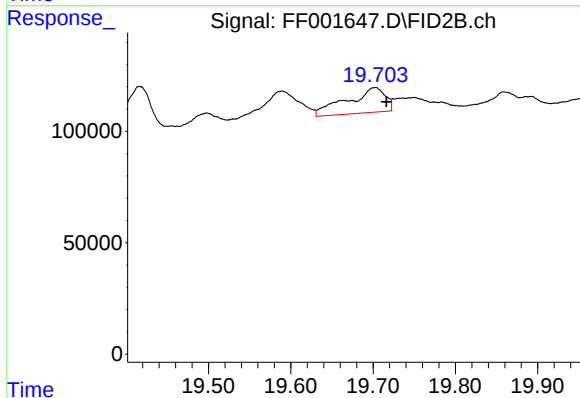


#16 N-HEXATRIACONTANE

R.T.: 19.703 min
Delta R.T.: -0.013 min
Response: 361849
Conc: 3.25 ug/ml

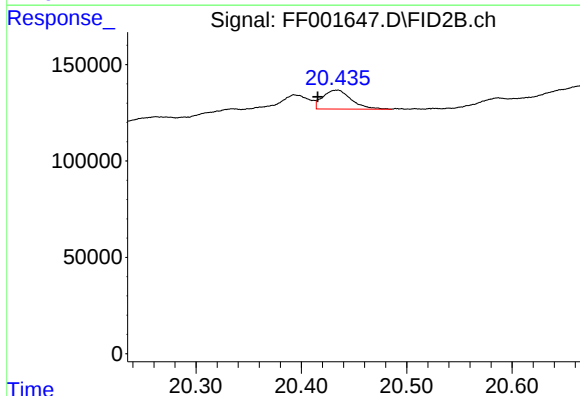

#17 N-OCTATRIACONTANE

R.T.: 20.434 min
Delta R.T.: 0.019 min
Response: 184951
Conc: 1.86 ug/ml

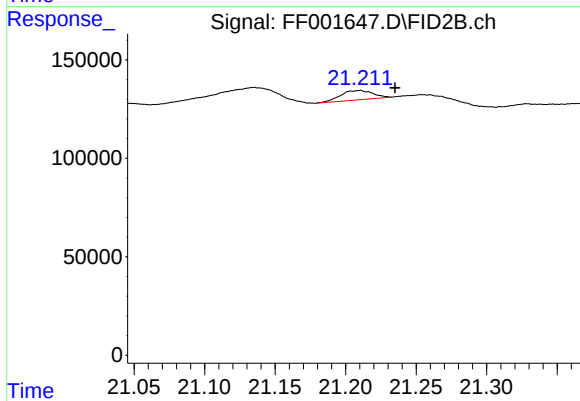

#18 N-TETRACONTANE

R.T.: 21.210 min
Delta R.T.: -0.025 min
Response: 76050
Conc: 0.76 ug/ml