

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080318\
 Data File : FF001656.D
 Signal(s) : FID2B.ch
 Acq On : 03 Aug 2018 13:20
 Operator : AJ\SJ
 Sample : J4307-13
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 04 01:56:26 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.338	1244688	9.855 ug/ml
Target Compounds			
4) N-TETRADECANE	7.970f	326247	2.165 ug/ml
7) N-EICOSANE	12.289f	369242	2.477 ug/ml
10) N-TETRACOSANE	14.502	645548	4.525 ug/ml
12) N-OCTACOSANE	16.507	131983	0.941 ug/ml
13) N-TRIACONTANE	17.392	193763	1.400 ug/ml
14) N-DOTRIACONTANE	18.184	165416	1.268 ug/ml
15) N-TETRATRIACONTANE	19.001	101949	0.843 ug/ml
16) N-HEXATRIACONTANE	19.704	94916	0.853 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080318\
Data File : FF001656.D
Signal(s) : FID2B.ch
Acq On : 03 Aug 2018 13:20
Operator : AJ\SJ
Sample : J4307-13
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 04 01:56:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

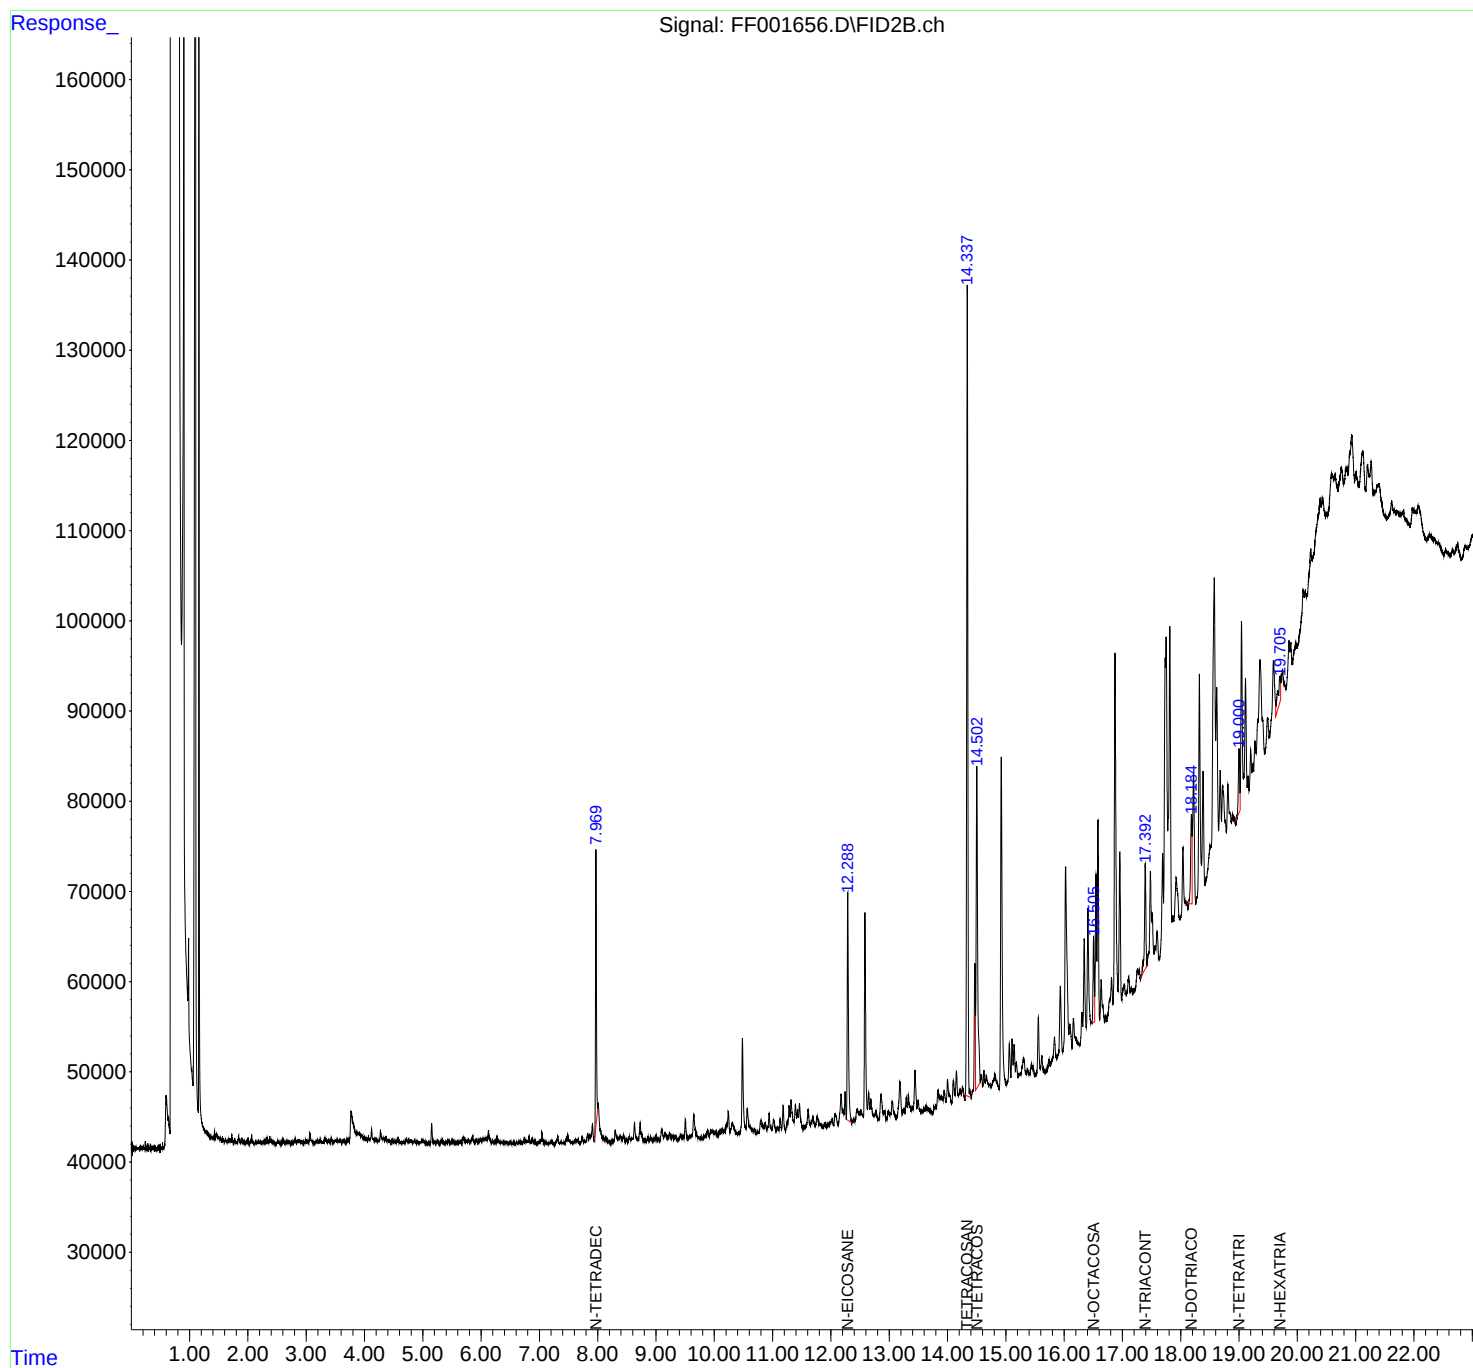

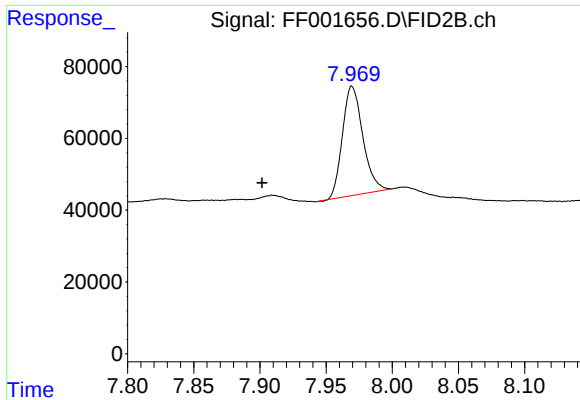


#4 N-TETRADECANE

R.T.: 7.970 min
Delta R.T.: 0.068 min
Response: 326247
Conc: 2.16 ug/ml

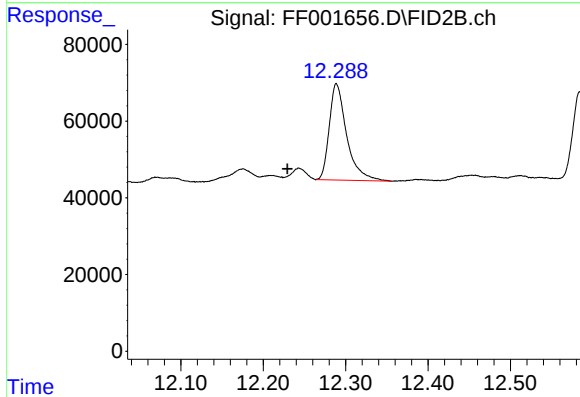


#7 N-EICOSANE

R.T.: 12.289 min
Delta R.T.: 0.059 min
Response: 369242
Conc: 2.48 ug/ml

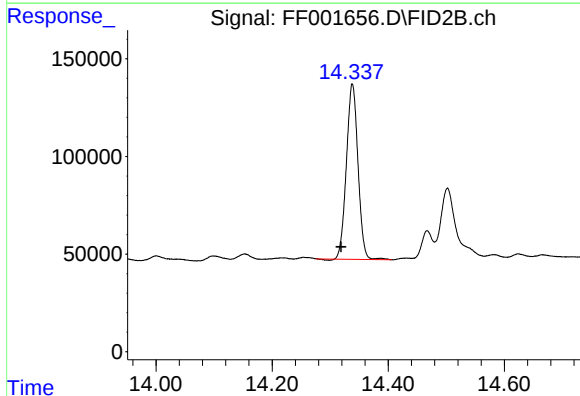


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.338 min
Delta R.T.: 0.020 min
Response: 1244688
Conc: 9.85 ug/ml

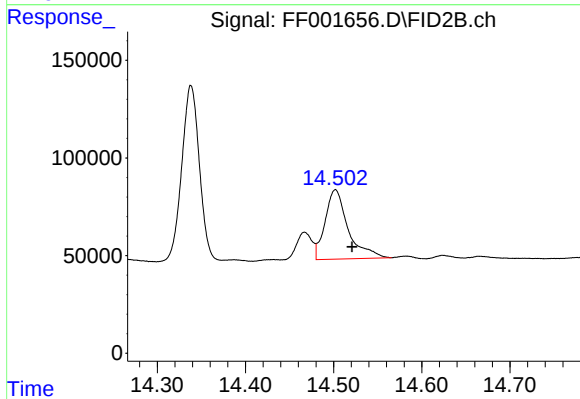


#10 N-TETRACOSANE

R.T.: 14.502 min
Delta R.T.: -0.019 min
Response: 645548
Conc: 4.53 ug/ml

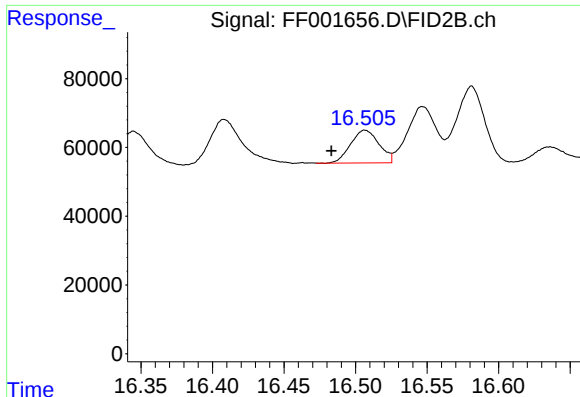


#12 N-OCTACOSANE

R.T.: 16.507 min
Delta R.T.: 0.023 min
Response: 131983
Conc: 0.94 ug/ml

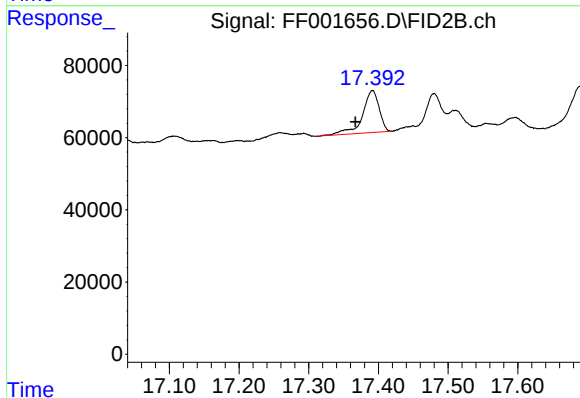


#13 N-TRIACONTANE

R.T.: 17.392 min
Delta R.T.: 0.024 min
Response: 193763
Conc: 1.40 ug/ml

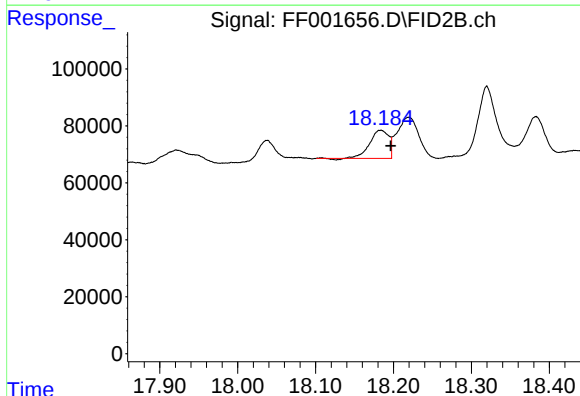


#14 N-DOTRIACONTANE

R.T.: 18.184 min
Delta R.T.: -0.013 min
Response: 165416
Conc: 1.27 ug/ml

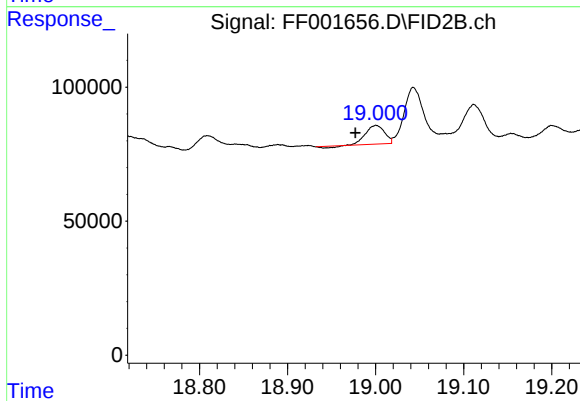

#15 N-TETRATRIACONTANE

R.T.: 19.001 min
Delta R.T.: 0.024 min
Response: 101949
Conc: 0.84 ug/ml

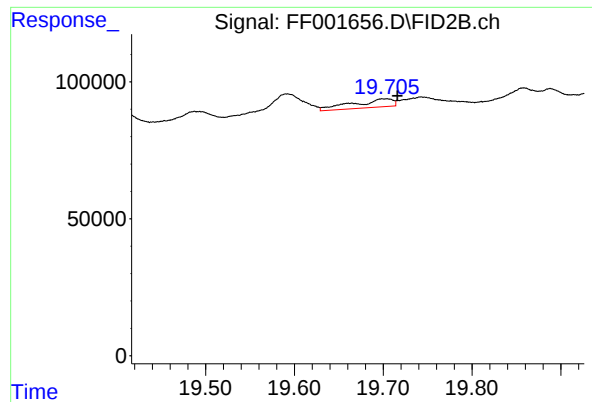

#16 N-HEXATRIACONTANE

R.T.: 19.704 min
Delta R.T.: -0.012 min
Response: 94916
Conc: 0.85 ug/ml