

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080322\
 Data File : FF011140.D
 Signal(s) : FID2B.ch
 Acq On : 03 Aug 2022 15:58
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 03 20:24:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
 Quant Title :
 QLast Update : Thu Jul 28 14:46:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.800	1671945	15.383 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.856	68617	0.574 ug/ml
14)	N-DOTRIACONTANE	18.688	96205	0.814 ug/ml
15)	N-TETRATRIACONTANE	19.469	72638	0.651 ug/ml
16)	N-HEXATRIACONTANE	20.207	44524	0.438 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080322\
Data File : FF011140.D
Signal(s) : FID2B.ch
Acq On : 03 Aug 2022 15:58
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 03 20:24:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

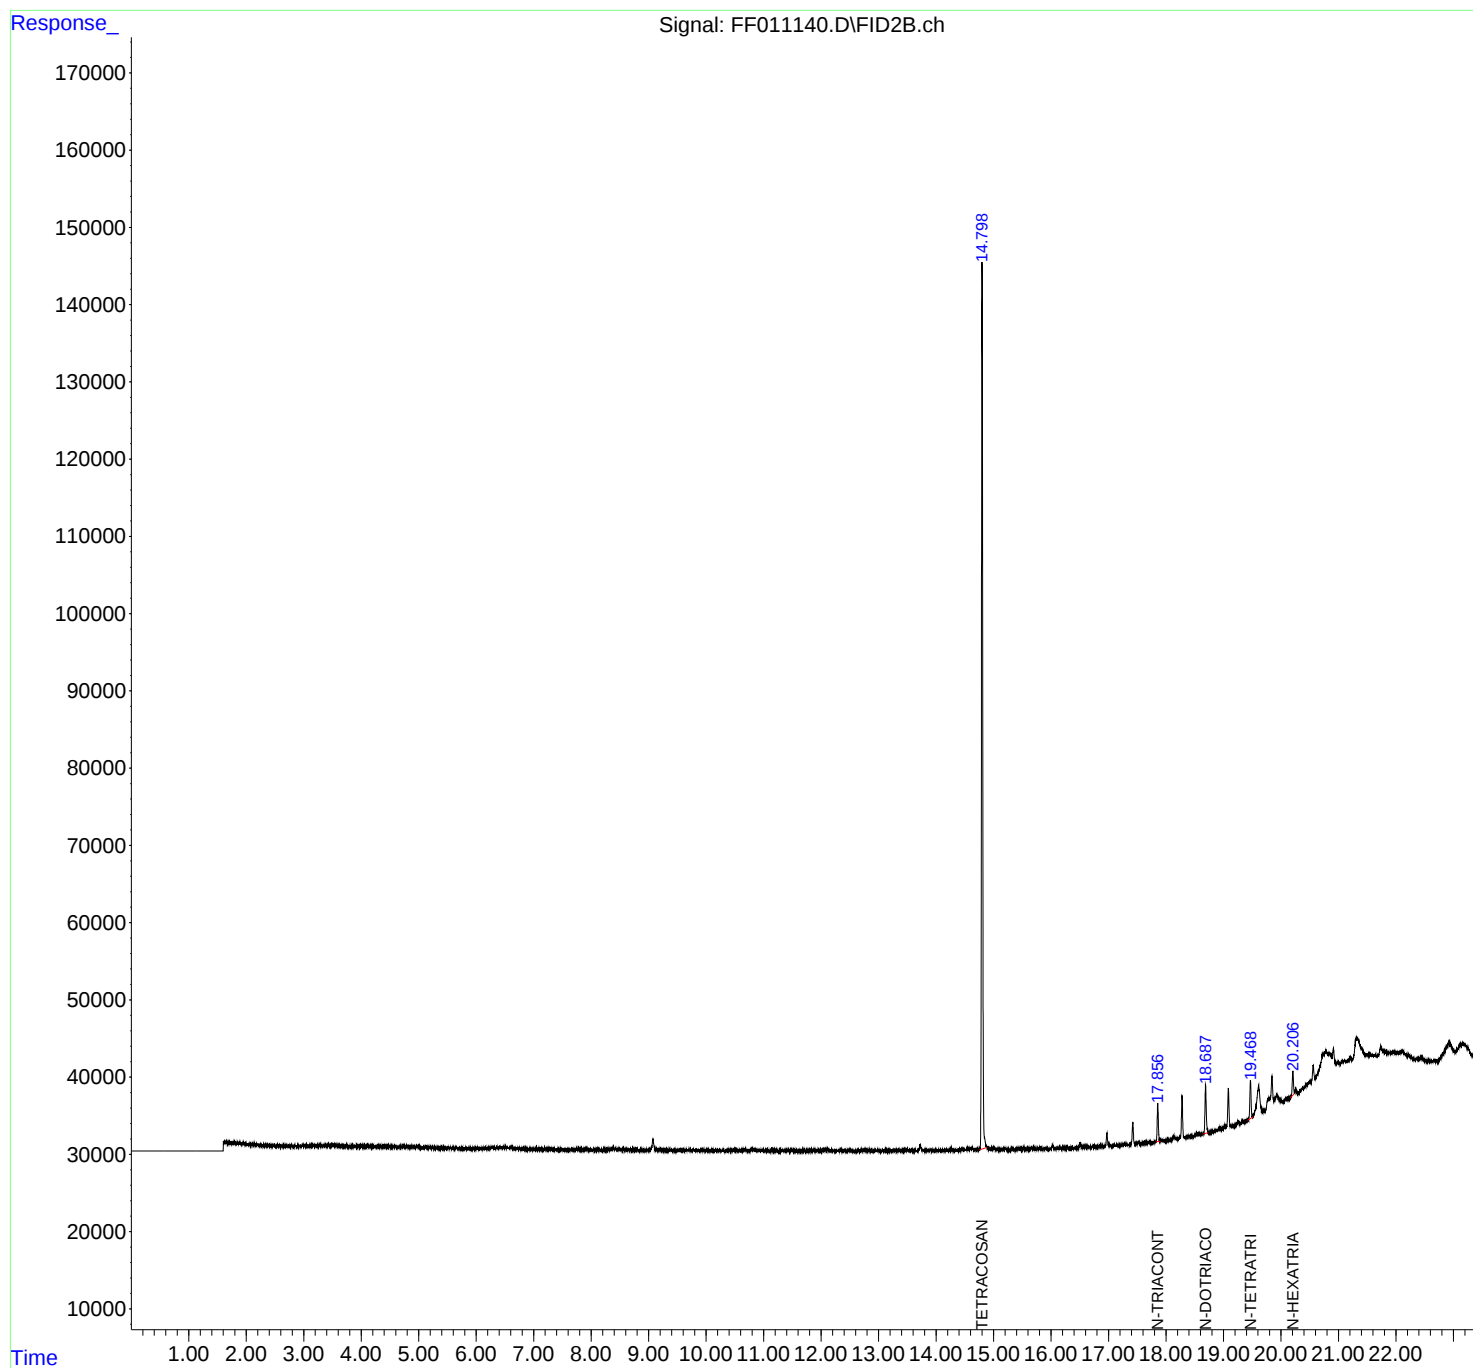

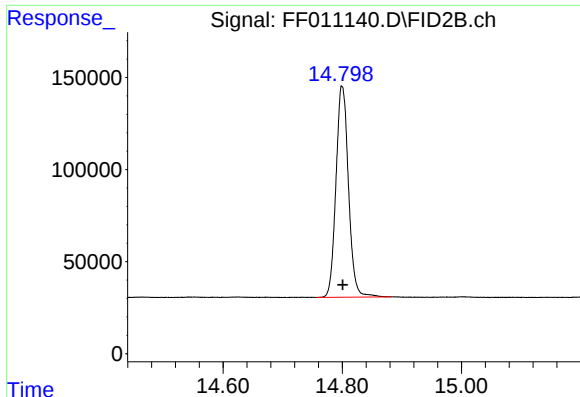


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.800 min
Delta R.T.: -0.001 min
Response: 1671945
Conc: 15.38 ug/ml

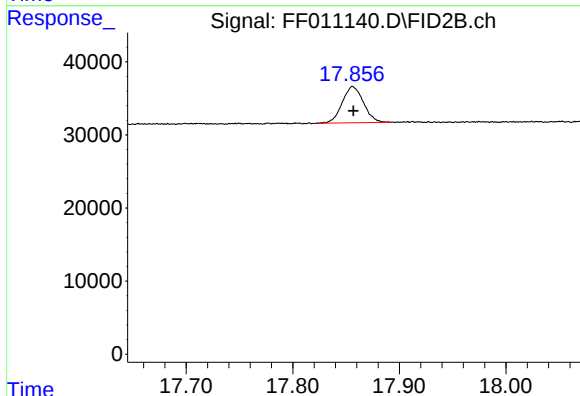


#13 N-TRIACONTANE

R.T.: 17.856 min
Delta R.T.: 0.000 min
Response: 68617
Conc: 0.57 ug/ml

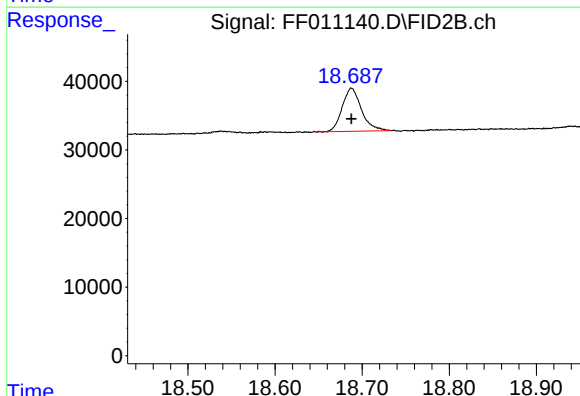


#14 N-DOTRIACONTANE

R.T.: 18.688 min
Delta R.T.: 0.000 min
Response: 96205
Conc: 0.81 ug/ml

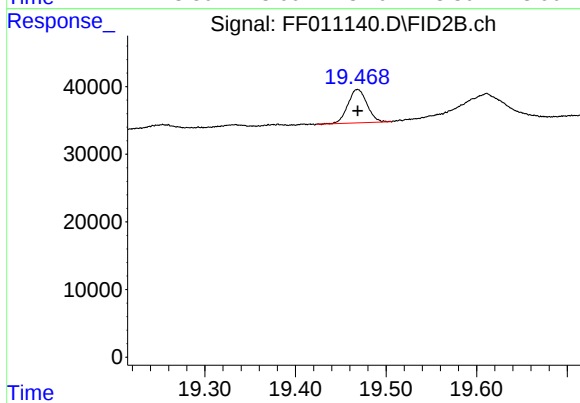

#15 N-TETRATRIACONTANE

R.T.: 19.469 min
Delta R.T.: 0.000 min
Response: 72638
Conc: 0.65 ug/ml

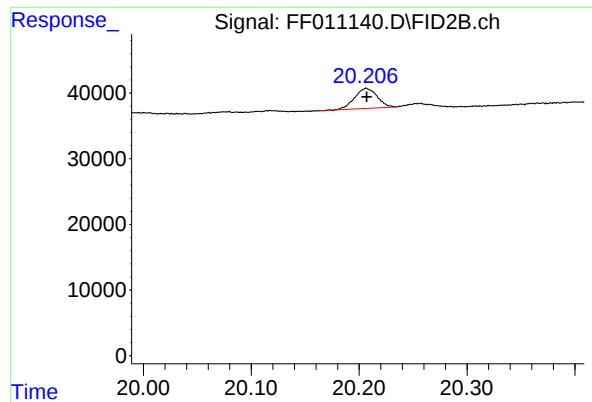

#16 N-HEXATRIACONTANE

R.T.: 20.207 min
Delta R.T.: 0.000 min
Response: 44524
Conc: 0.44 ug/ml