

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080519\
 Data File : FF0805164.D
 Signal(s) : FID2B.ch
 Acq On : 05 Aug 2019 14:27
 Operator : DD\AJ
 Sample : PB121966BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 06 00:32:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
 Quant Title :
 QLast Update : Tue Jul 30 14:33:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.654	2061086	18.715 ug/ml
Target Compounds			
2) N-DECANE	4.377	2940699	20.411 ug/ml
3) N-DODECANE	6.397	2986464	20.468 ug/ml
4) N-TETRADECANE	8.191	2935999	20.398 ug/ml
5) N-HEXADECANE	9.792	2889680	20.380 ug/ml
6) N-OCTADECANE	11.235	2820773	20.601 ug/ml
7) N-EICOSANE	12.548	2737944	20.406 ug/ml
8) N-DOCOSANE	13.751	2645383	20.447 ug/ml
10) N-TETRACOSANE	14.858	2609665	20.714 ug/ml
11) N-HEXACOSANE	15.883	2558156	20.703 ug/ml
12) N-OCTACOSANE	16.838	2568493	20.562 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080519\
Data File : FF005164.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2019 14:27
Operator : DD\AJ
Sample : PB121966BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 06 00:32:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

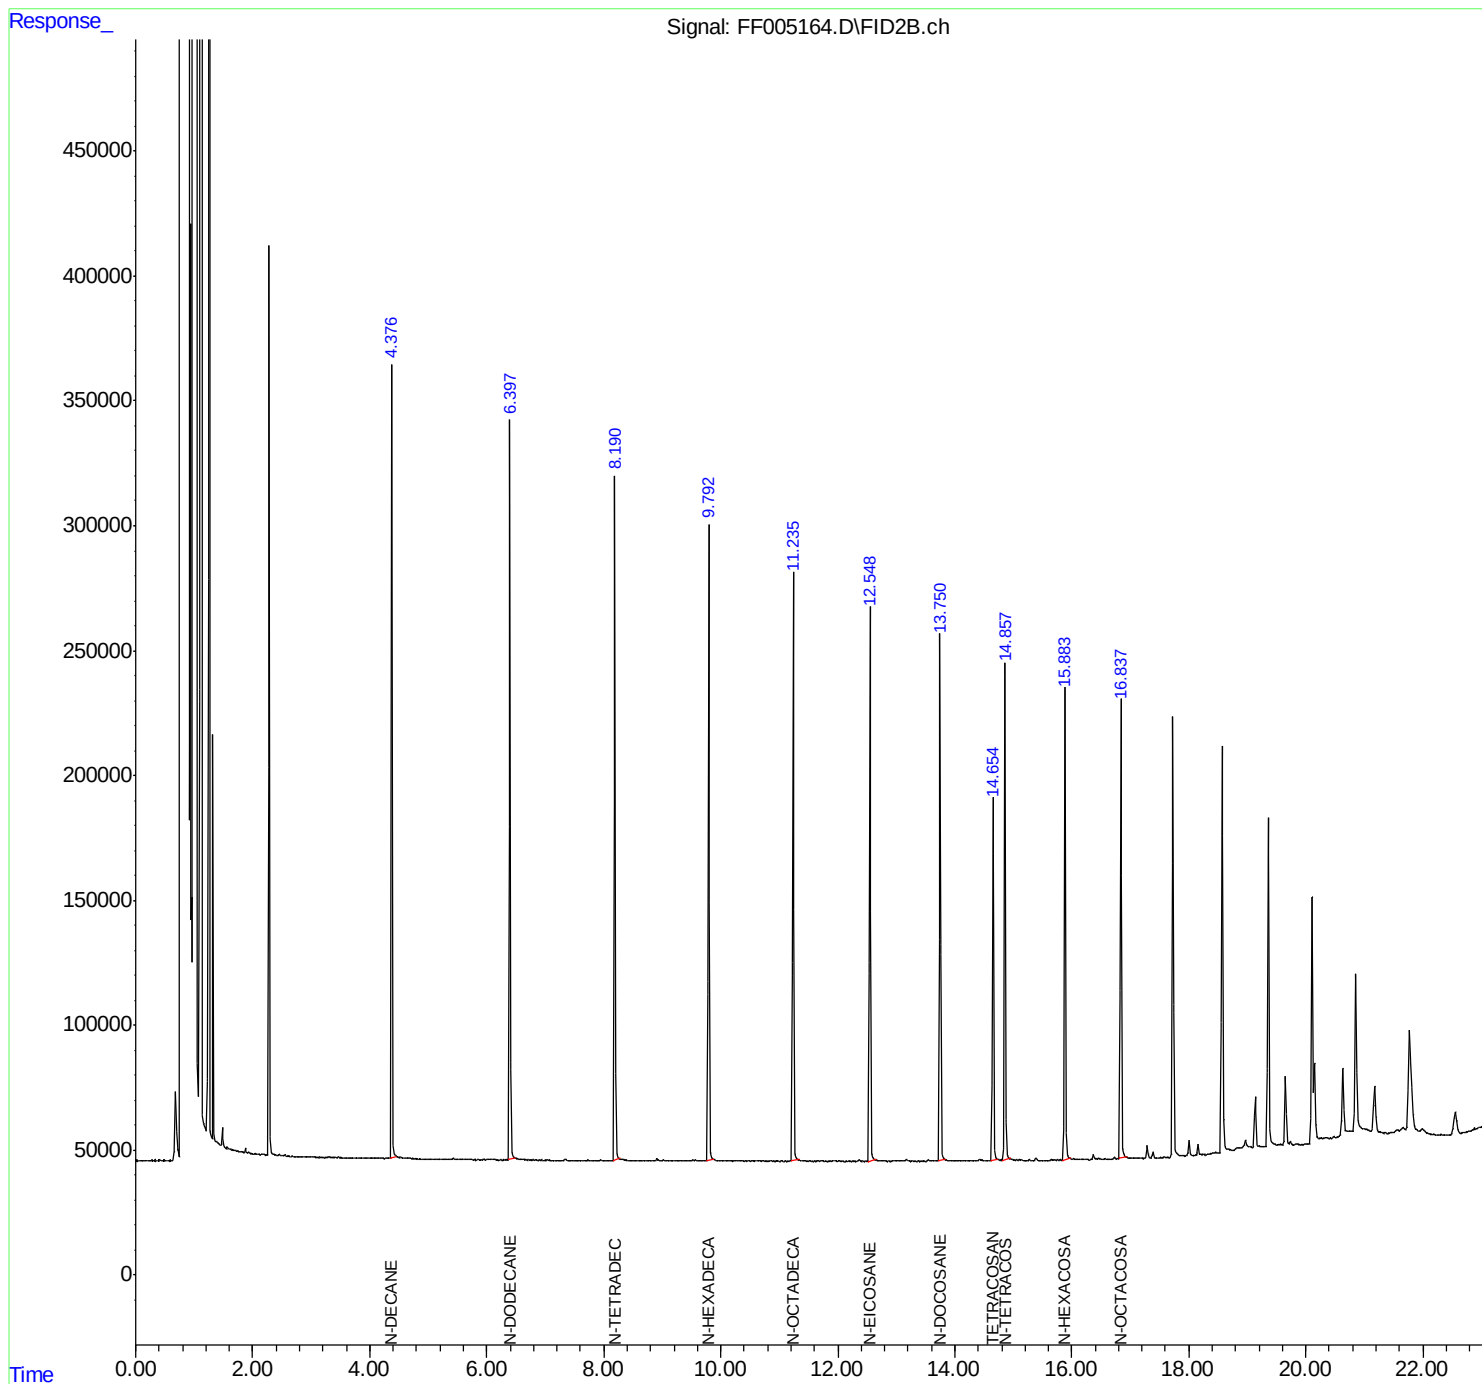

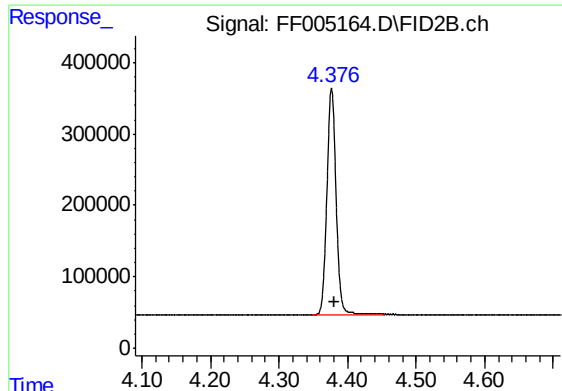


#2 N-DECANE

R.T.: 4.377 min
Delta R.T.: -0.004 min
Response: 2940699
Conc: 20.41 ug/ml

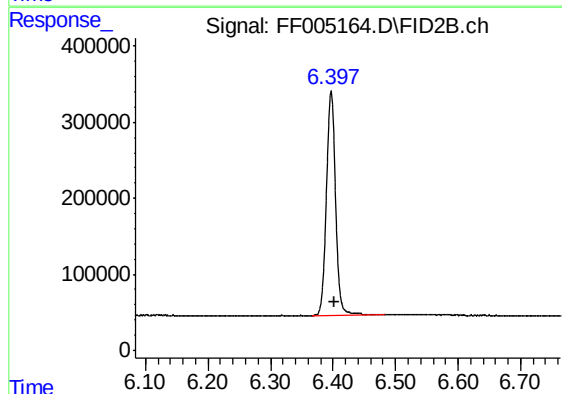


#3 N-DODECANE

R.T.: 6.397 min
Delta R.T.: -0.005 min
Response: 2986464
Conc: 20.47 ug/ml

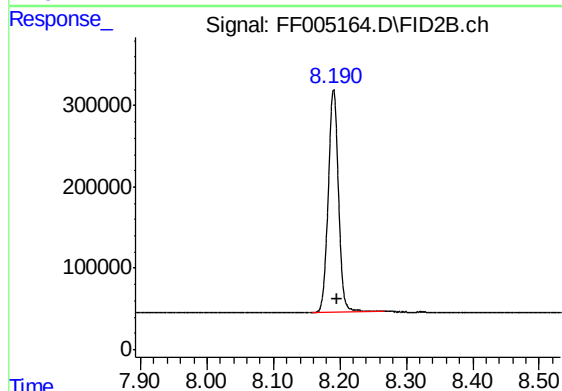


#4 N-TETRADECANE

R.T.: 8.191 min
Delta R.T.: -0.005 min
Response: 2935999
Conc: 20.40 ug/ml

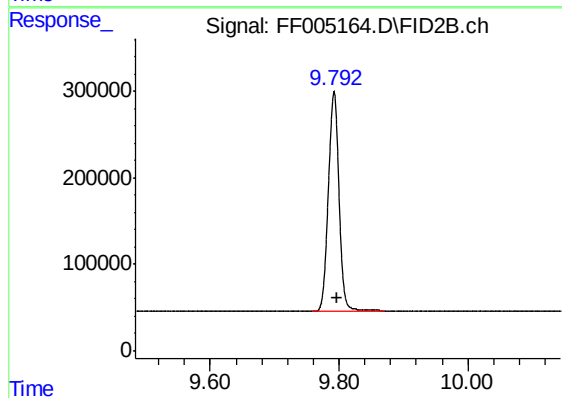


#5 N-HEXADECANE

R.T.: 9.792 min
Delta R.T.: -0.005 min
Response: 2889680
Conc: 20.38 ug/ml

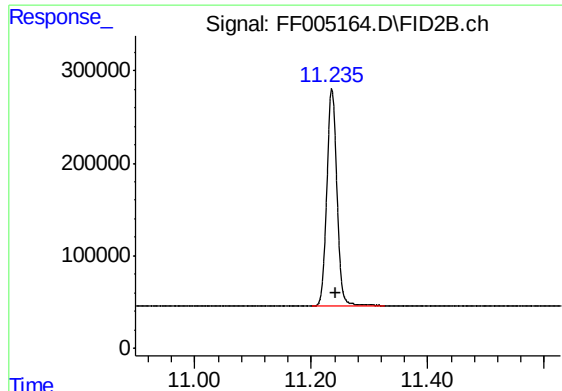


#6 N-OCTADECANE

R.T.: 11.235 min
Delta R.T.: -0.006 min
Response: 2820773
Conc: 20.60 ug/ml

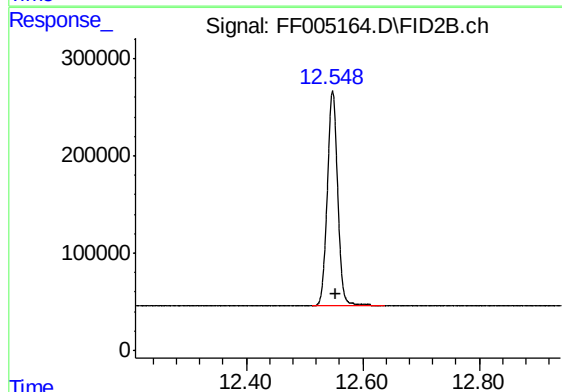


#7 N-EICOSANE

R.T.: 12.548 min
Delta R.T.: -0.006 min
Response: 2737944
Conc: 20.41 ug/ml

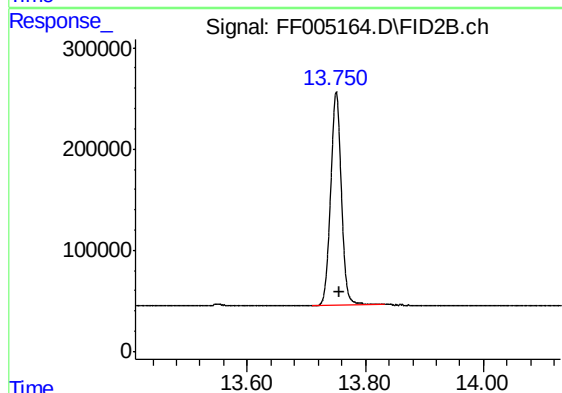


#8 N-DOCOSANE

R.T.: 13.751 min
Delta R.T.: -0.006 min
Response: 2645383
Conc: 20.45 ug/ml

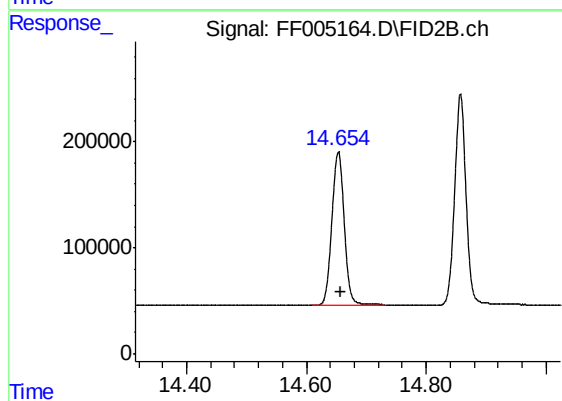


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.654 min
Delta R.T.: -0.005 min
Response: 2061086
Conc: 18.72 ug/ml

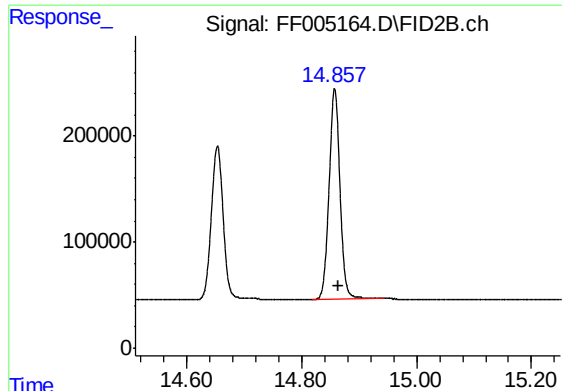


#10 N-TETRACOSANE

R.T.: 14.858 min
Delta R.T.: -0.006 min
Response: 2609665
Conc: 20.71 ug/ml

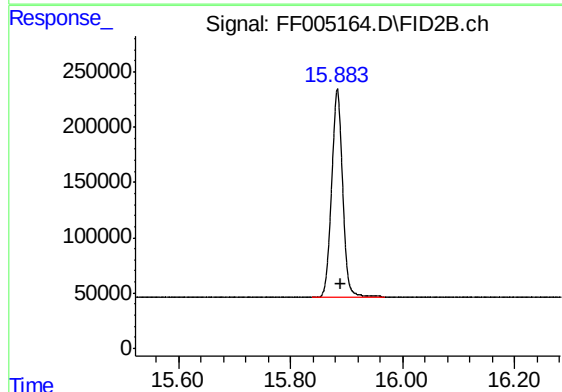

#11 N-HEXACOSANE

R.T.: 15.883 min
Delta R.T.: -0.006 min
Response: 2558156
Conc: 20.70 ug/ml

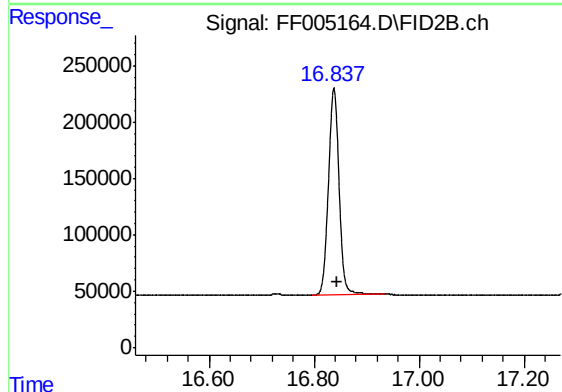

#12 N-OCTACOSANE

R.T.: 16.838 min
Delta R.T.: -0.006 min
Response: 2568493
Conc: 20.56 ug/ml