

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080519\
 Data File : FF0805173.D
 Signal(s) : FID2B.ch
 Acq On : 05 Aug 2019 19:01
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 06 00:35:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
 Quant Title :
 QLast Update : Tue Jul 30 14:33:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.658	5376929	48.824 ug/ml
Target Compounds			
2) N-DECANE	4.379	7314585	50.770 ug/ml
3) N-DODECANE	6.401	7247243	49.669 ug/ml
4) N-TETRADECANE	8.195	7039941	48.911 ug/ml
5) N-HEXADECANE	9.797	6900058	48.665 ug/ml
6) N-OCTADECANE	11.241	6649685	48.565 ug/ml
7) N-EICOSANE	12.554	6501358	48.455 ug/ml
8) N-DOCOSANE	13.756	6269310	48.458 ug/ml
10) N-TETRACOSANE	14.864	6141357	48.746 ug/ml
11) N-HEXACOSANE	15.889	6118573	49.518 ug/ml
12) N-OCTACOSANE	16.843	6201841	49.649 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080519\
Data File : FF05173.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2019 19:01
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 06 00:35:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073019.M
Quant Title :
QLast Update : Tue Jul 30 14:33:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

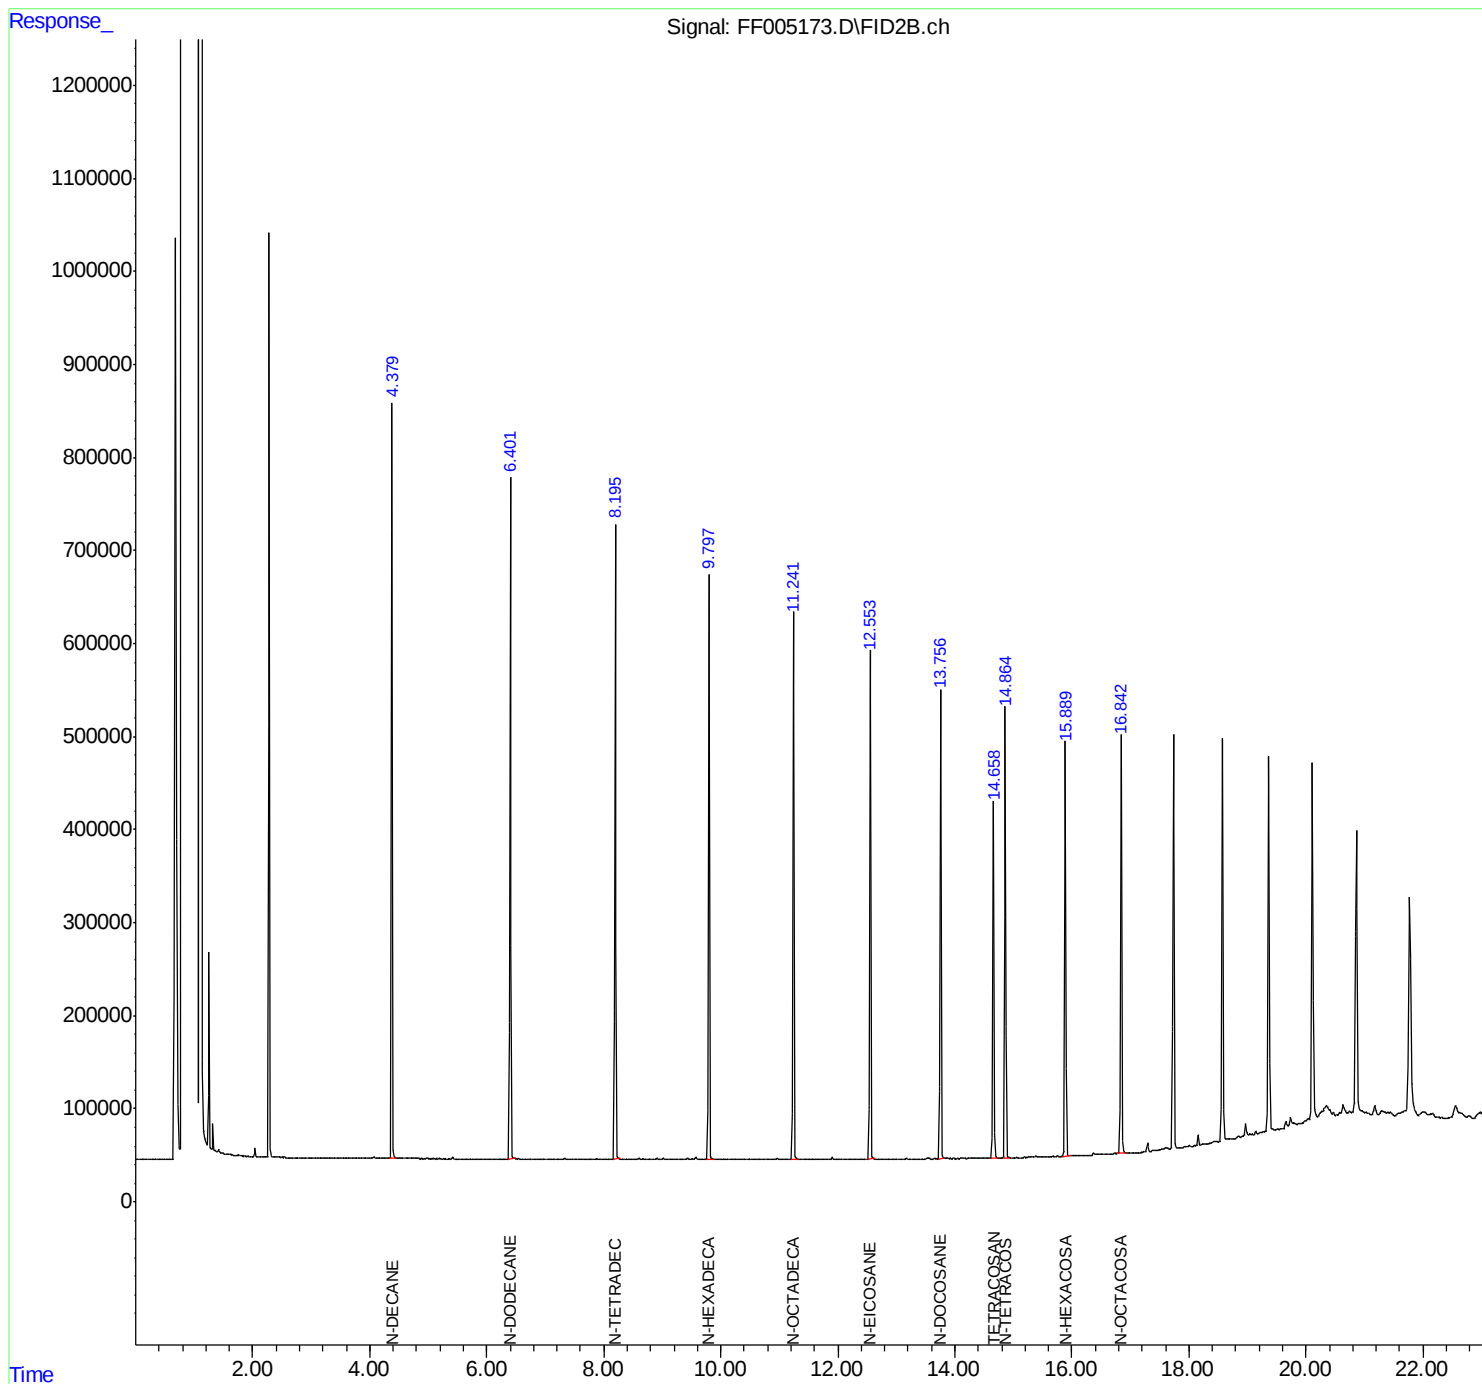

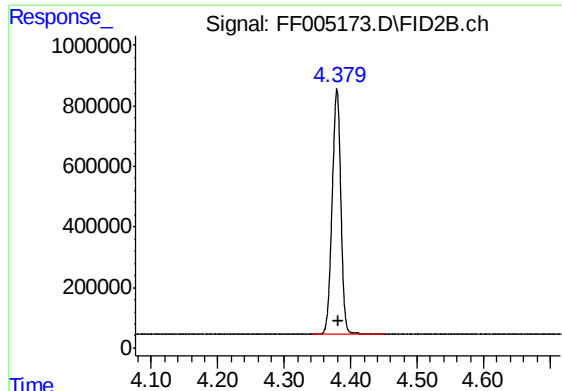


#2 N-DECANE

R.T.: 4.379 min
Delta R.T.: -0.001 min
Response: 7314585
Conc: 50.77 ug/ml

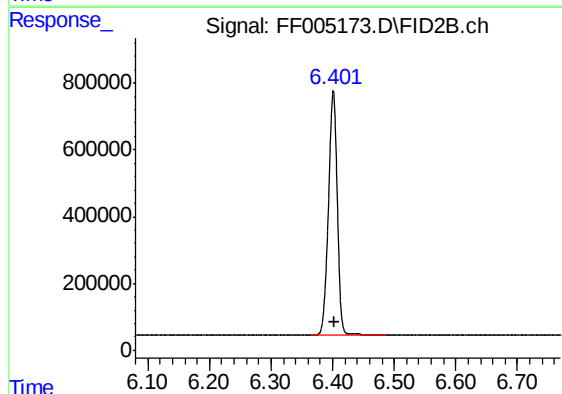


#3 N-DODECANE

R.T.: 6.401 min
Delta R.T.: -0.001 min
Response: 7247243
Conc: 49.67 ug/ml

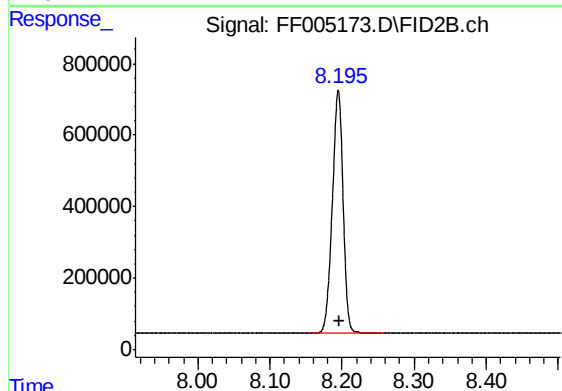


#4 N-TETRADECANE

R.T.: 8.195 min
Delta R.T.: -0.001 min
Response: 7039941
Conc: 48.91 ug/ml

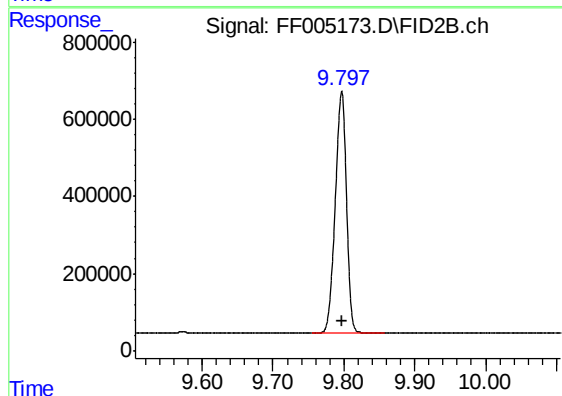


#5 N-HEXADECANE

R.T.: 9.797 min
Delta R.T.: 0.000 min
Response: 6900058
Conc: 48.66 ug/ml

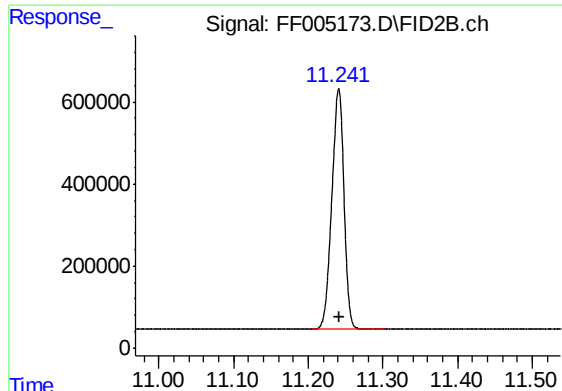


#6 N-OCTADECANE

R.T.: 11.241 min
Delta R.T.: 0.000 min
Response: 6649685
Conc: 48.56 ug/ml

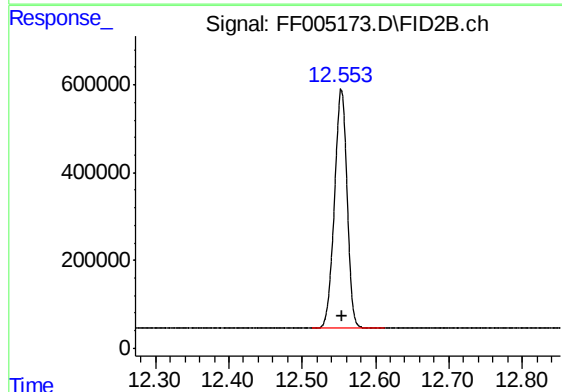


#7 N-EICOSANE

R.T.: 12.554 min
Delta R.T.: 0.000 min
Response: 6501358
Conc: 48.45 ug/ml

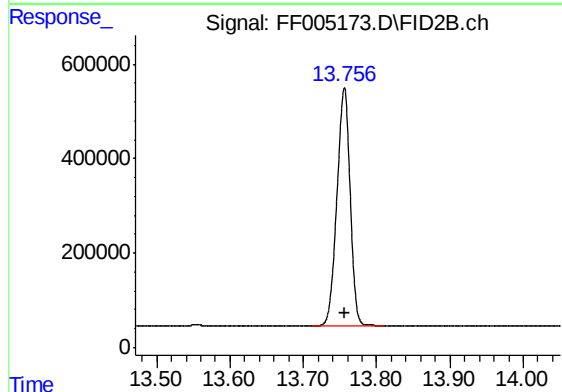


#8 N-DOCOSANE

R.T.: 13.756 min
Delta R.T.: 0.000 min
Response: 6269310
Conc: 48.46 ug/ml

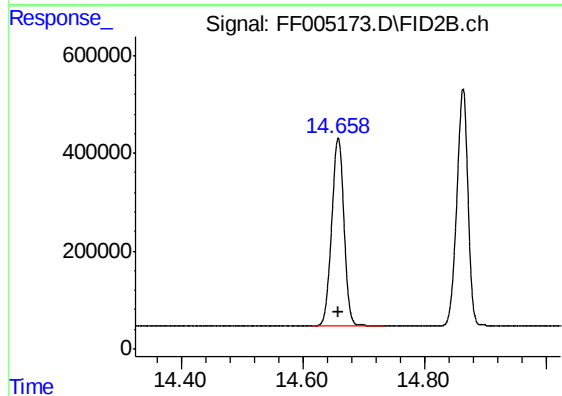


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.658 min
Delta R.T.: 0.000 min
Response: 5376929
Conc: 48.82 ug/ml

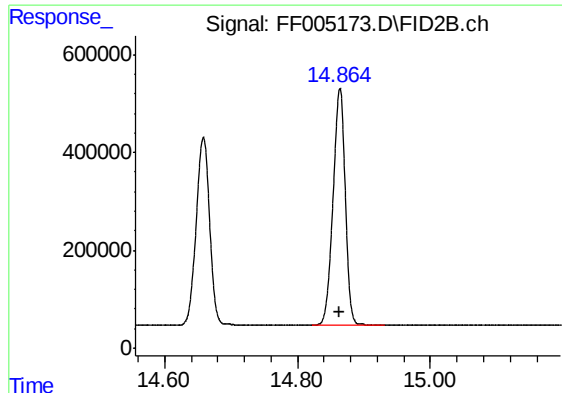


#10 N-TETRACOSANE

R.T.: 14.864 min
Delta R.T.: 0.000 min
Response: 6141357
Conc: 48.75 ug/ml

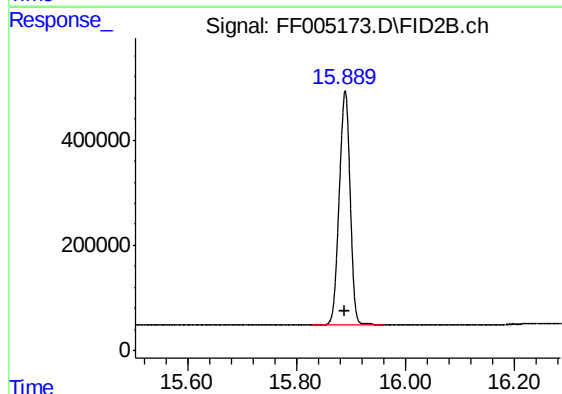

#11 N-HEXACOSANE

R.T.: 15.889 min
Delta R.T.: 0.000 min
Response: 6118573
Conc: 49.52 ug/ml

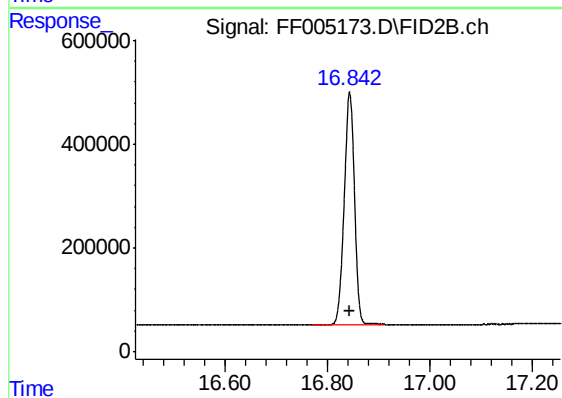

#12 N-OCTACOSANE

R.T.: 16.843 min
Delta R.T.: -0.001 min
Response: 6201841
Conc: 49.65 ug/ml