

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080522\
Data File : FF011175.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2022 08:34
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 07:01:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.962	70196	0.564 ug/ml
14)	N-DOTRIACONTANE	18.703	120093	1.017 ug/ml
16)	N-HEXATRIACONTANE	20.250	199042	1.958 ug/ml
18)	N-TETRACONTANE	21.768	304817	2.782 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080522\
Data File : FF011175.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2022 08:34
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 07:01:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

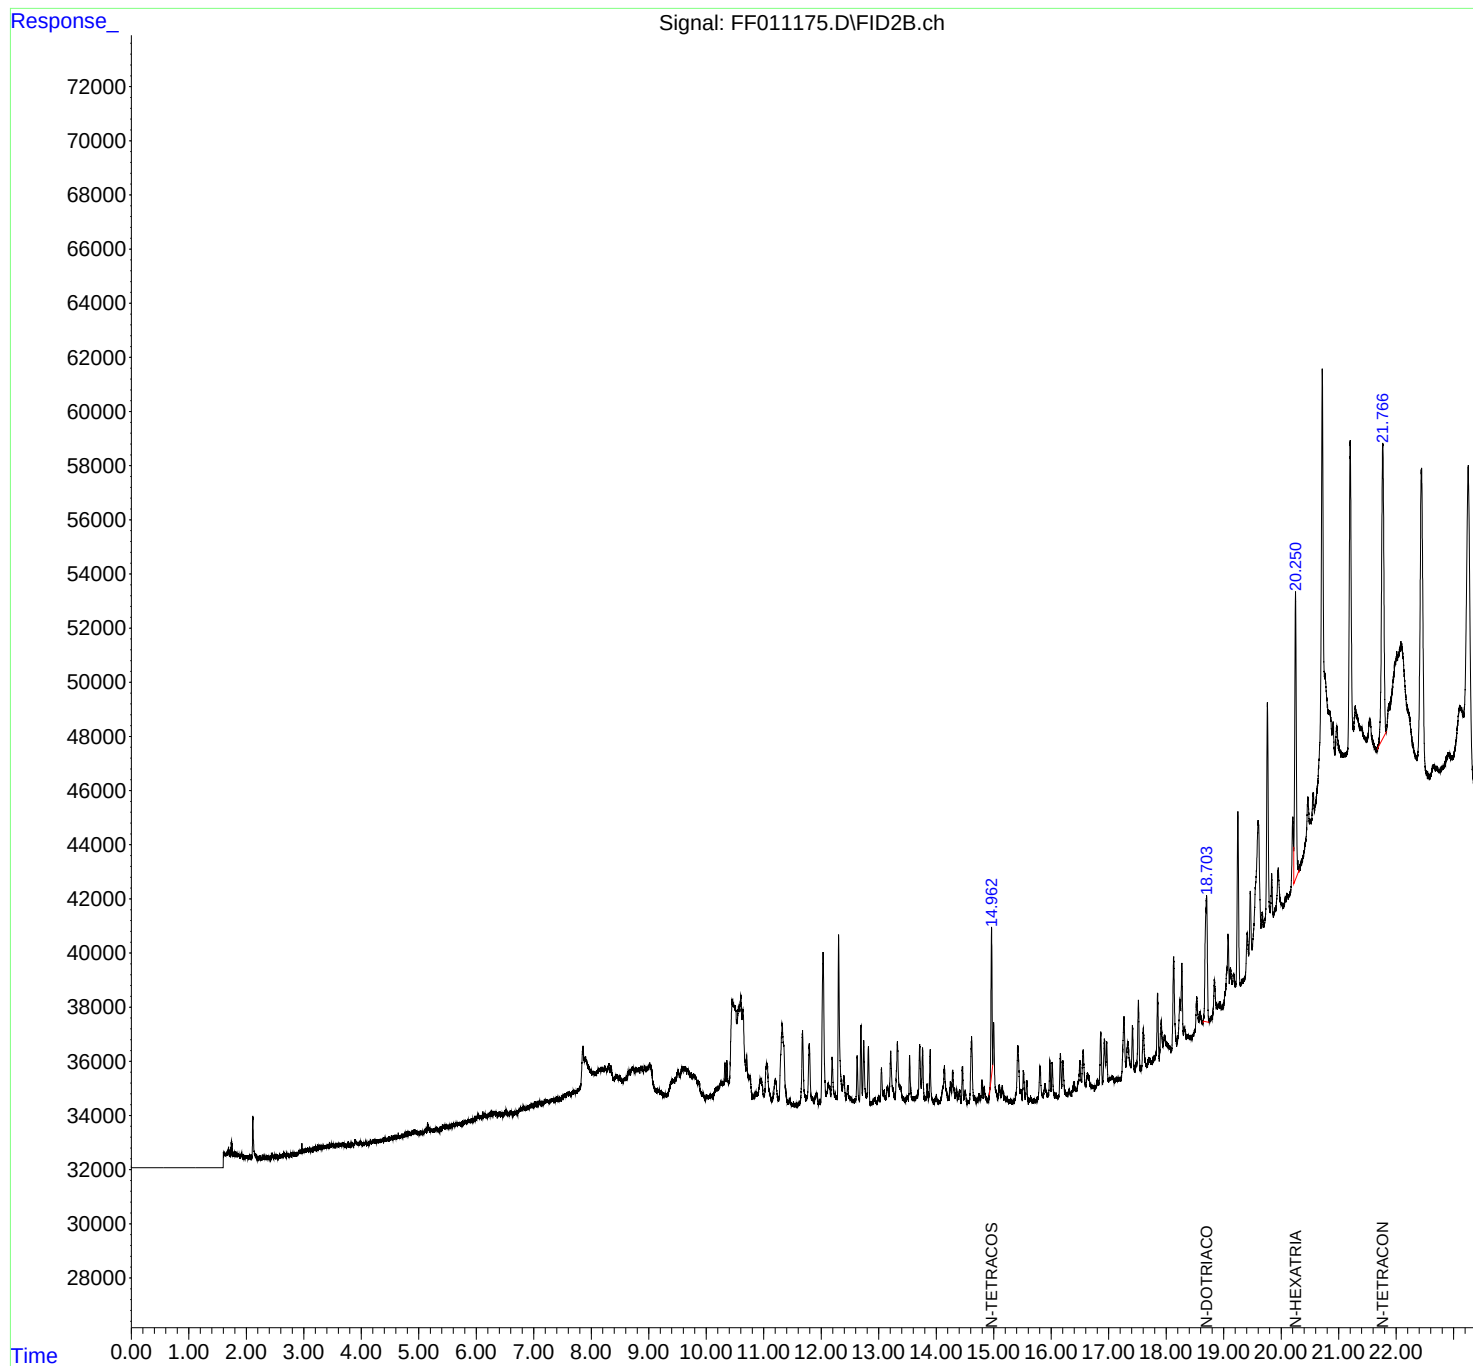


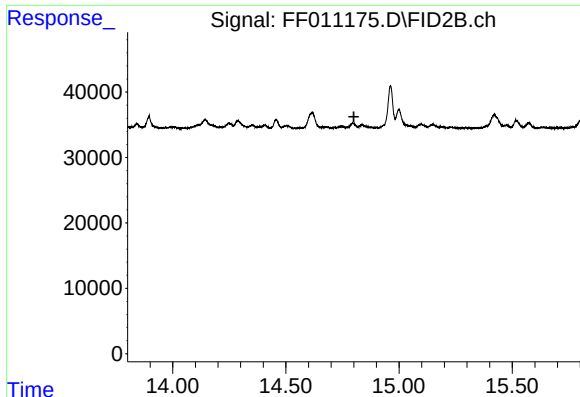

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.801 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

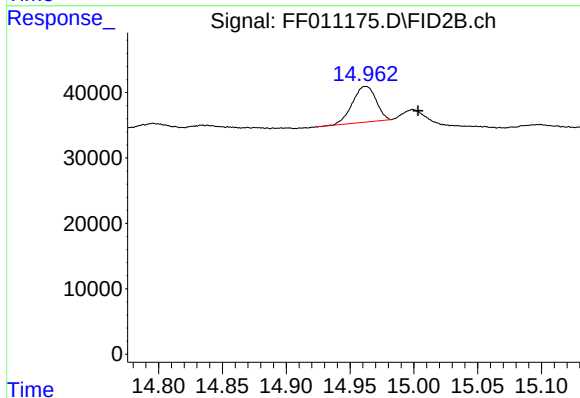


#10 N-TETRACOSANE

R.T.: 14.962 min
Delta R.T.: -0.041 min
Response: 70196
Conc: 0.56 ug/ml

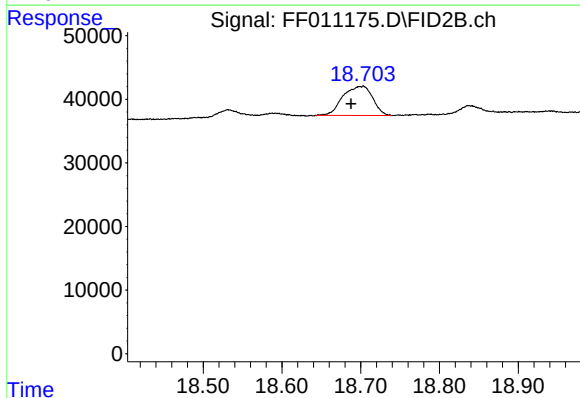


#14 N-DOTRIACONTANE

R.T.: 18.703 min
Delta R.T.: 0.016 min
Response: 120093
Conc: 1.02 ug/ml

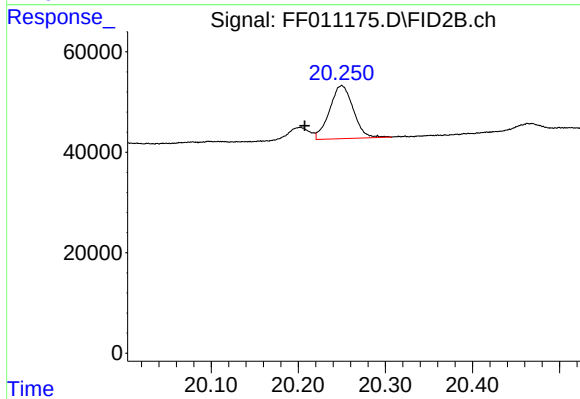

#16 N-HEXATRIACONTANE

R.T.: 20.250 min
Delta R.T.: 0.043 min
Response: 199042
Conc: 1.96 ug/ml

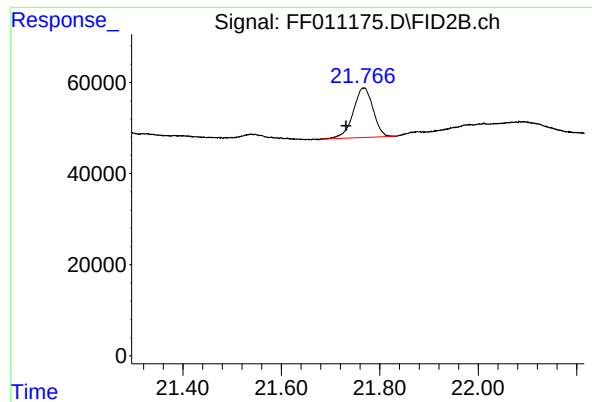

#18 N-TETRACONTANE

R.T.: 21.768 min
Delta R.T.: 0.036 min
Response: 304817
Conc: 2.78 ug/ml

Instrument :
FID_F
ClientSampleId :