

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080522\
Data File : FF011179.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2022 10:45
Operator : YP\AJ
Sample : PB146675BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 07:01:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.800	2693840	24.785 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.854	75255	0.630 ug/ml
14) N-DOTRIACONTANE	18.684	99378	0.841 ug/ml
15) N-TETRATRIACONTANE	19.463	74071	0.664 ug/ml
16) N-HEXATRIACONTANE	20.203	43576	0.429 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080522\
Data File : FF011179.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2022 10:45
Operator : YP\AJ
Sample : PB146675BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 07:01:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

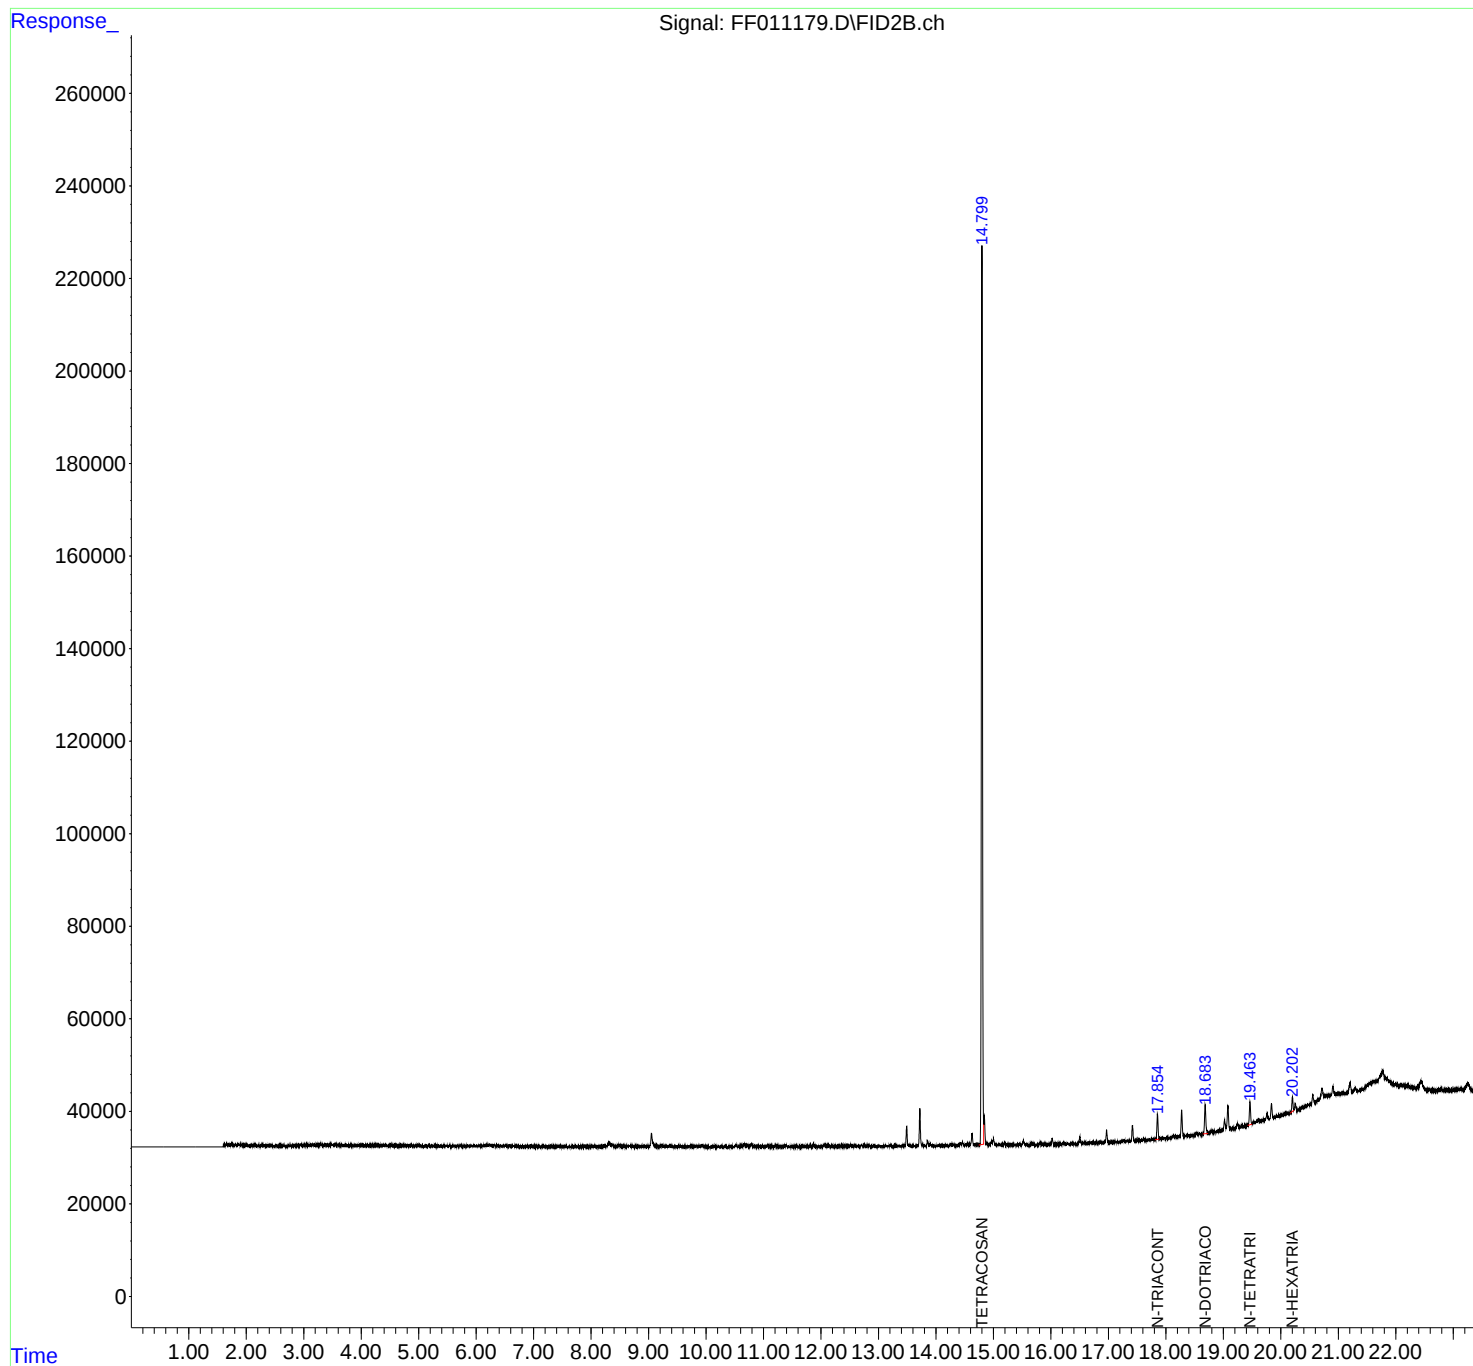


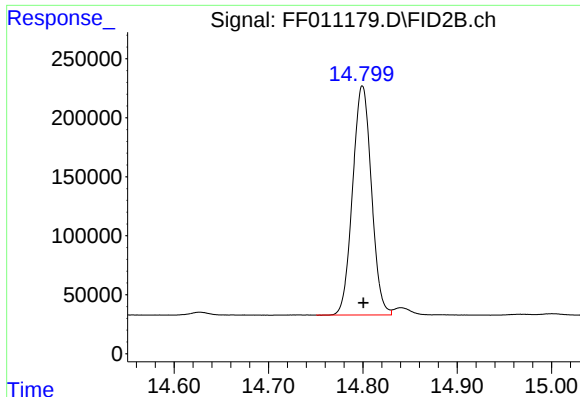

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.800 min
Delta R.T.: -0.001 min
Response: 2693840
Conc: 24.79 ug/ml

Instrument :
FID_F
ClientSampleId :

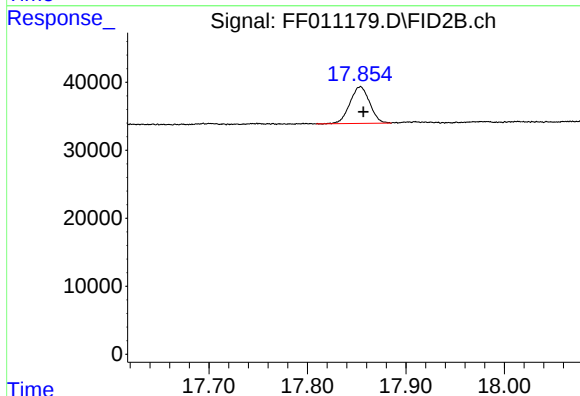


#13 N-TRIACONTANE

R.T.: 17.854 min
Delta R.T.: -0.003 min
Response: 75255
Conc: 0.63 ug/ml

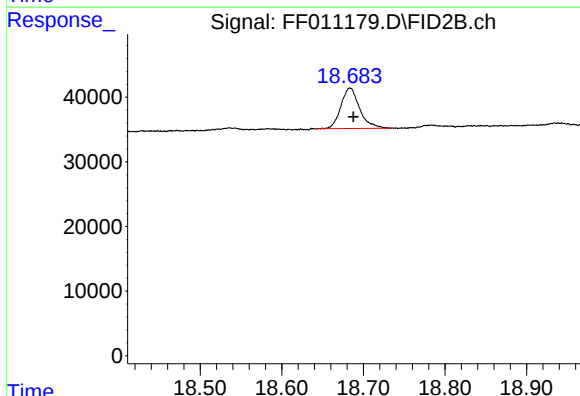


#14 N-DOTRIACONTANE

R.T.: 18.684 min
Delta R.T.: -0.004 min
Response: 99378
Conc: 0.84 ug/ml

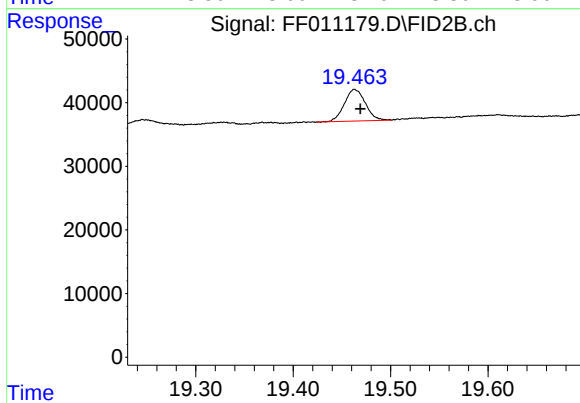

#15 N-TETRATRIACONTANE

R.T.: 19.463 min
Delta R.T.: -0.006 min
Response: 74071
Conc: 0.66 ug/ml

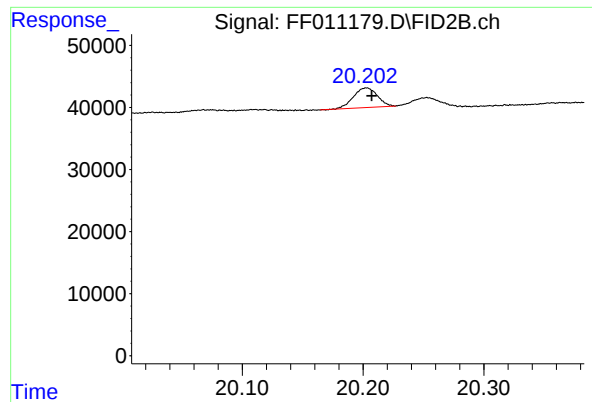

#16 N-HEXATRIACONTANE

R.T.: 20.203 min
Delta R.T.: -0.004 min
Response: 43576
Conc: 0.43 ug/ml

Instrument :

FID_F

ClientSampleId :