

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080522\
Data File : FF011187.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2022 14:54
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Aug 08 07:02:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.528	1337025	10.621 ug/ml
12)	N-OCTACOSANE	16.966	1372506	11.370 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080522\
Data File : FF011187.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2022 14:54
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Aug 08 07:02:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

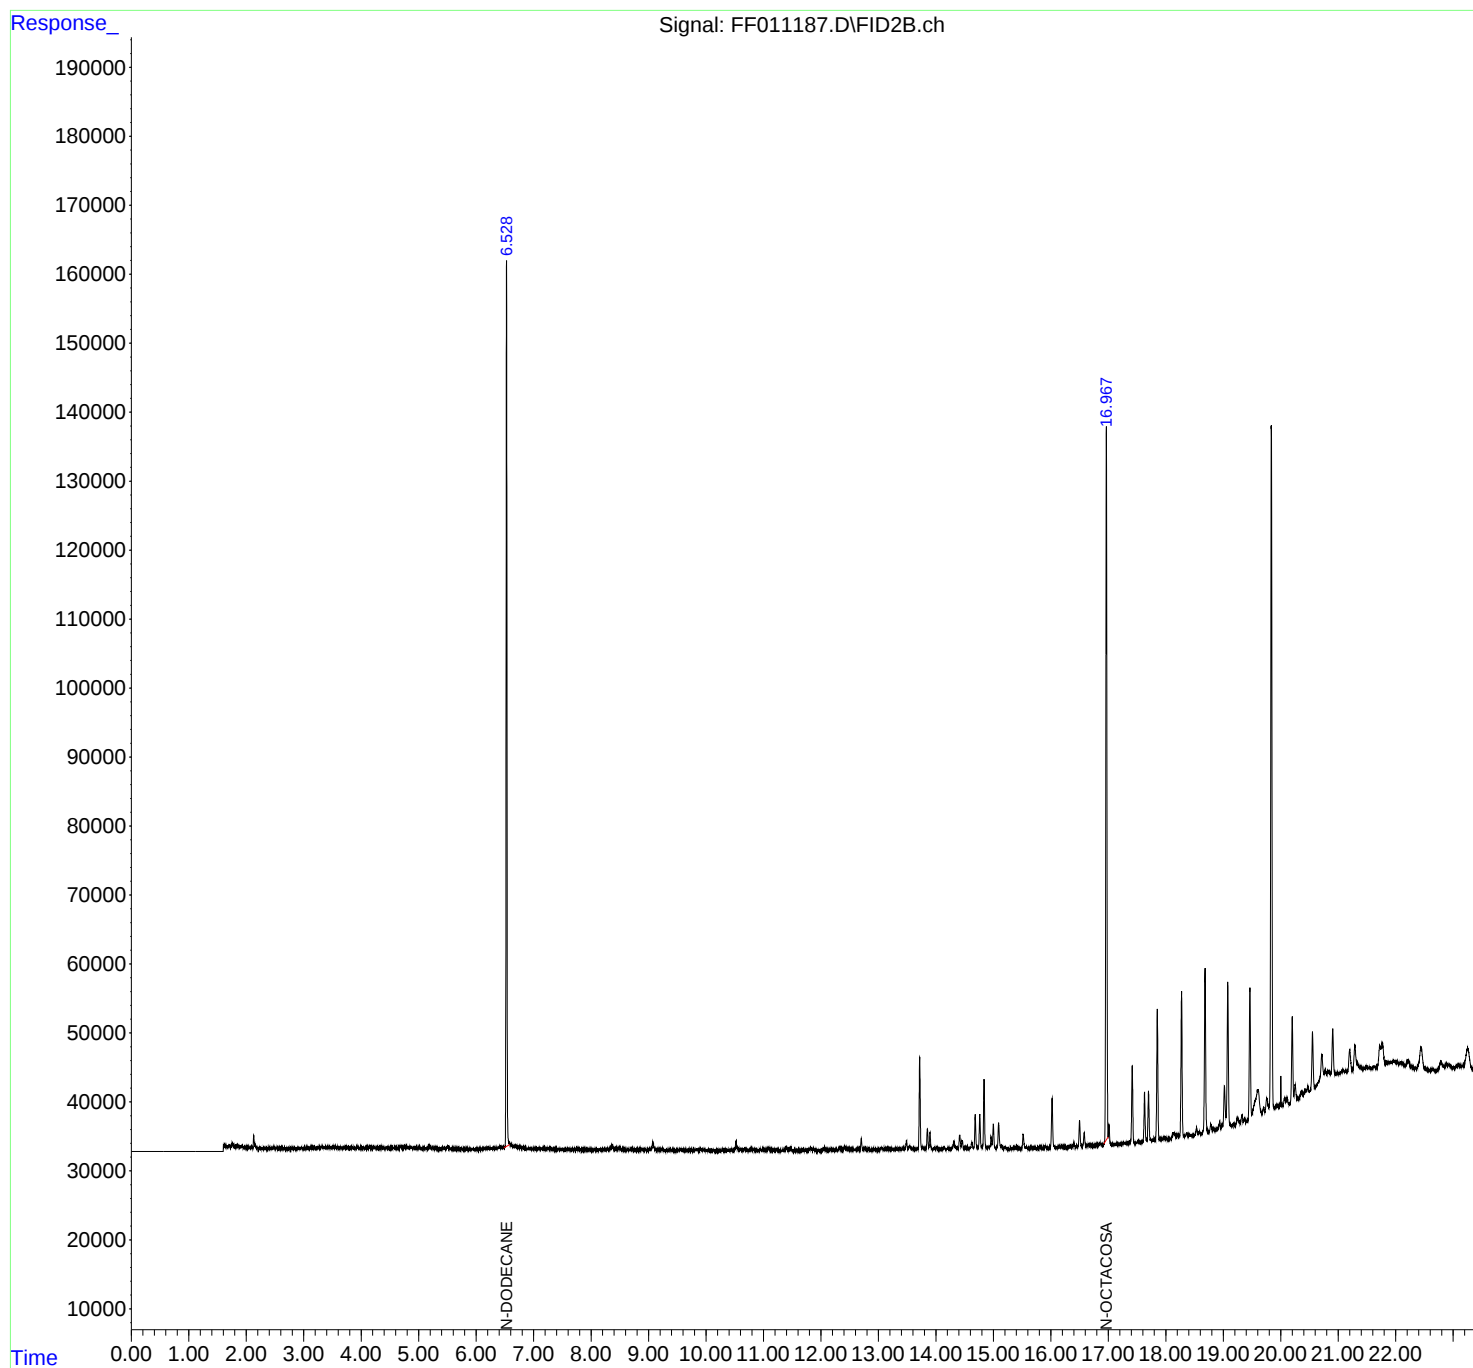


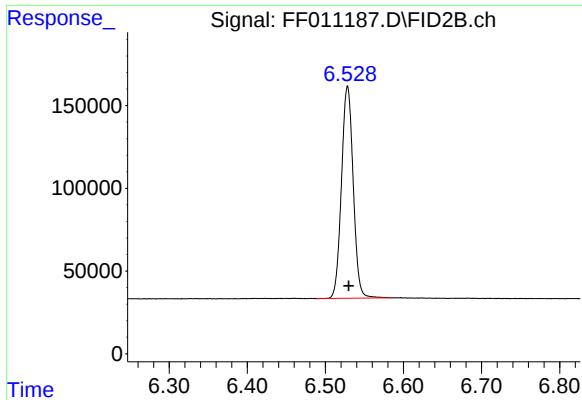

#3 N-DODECANE


R.T.: 6.528 min
Delta R.T.: -0.001 min
Response: 1337025
Conc: 10.62 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

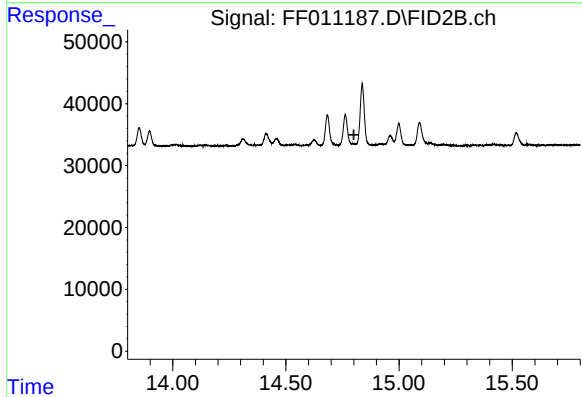

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.801 min
Response: 0
Conc: N.D.

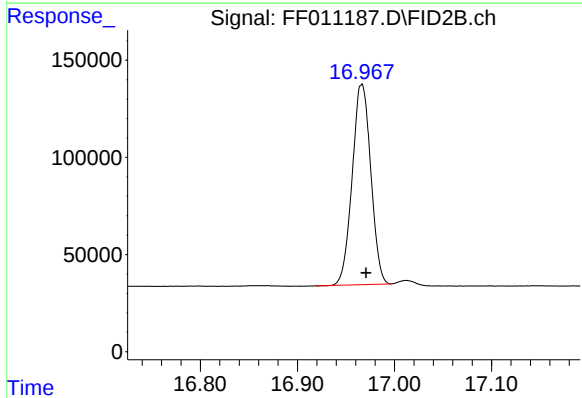

#12 N-OCTACOSANE

R.T.: 16.966 min
Delta R.T.: -0.005 min
Response: 1372506
Conc: 11.37 ug/ml