

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080522\
Data File : FF011191.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2022 17:04
Operator : YP\AJ
Sample : N4060-01 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
JERSEY-CITY-SP

Integration File: Sample.e
Quant Time: Aug 08 07:03:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.799	228619	2.103 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080522\
Data File : FF011191.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2022 17:04
Operator : YP\AJ
Sample : N4060-01 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
JERSEY-CITY-SP

Integration File: Sample.e
Quant Time: Aug 08 07:03:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

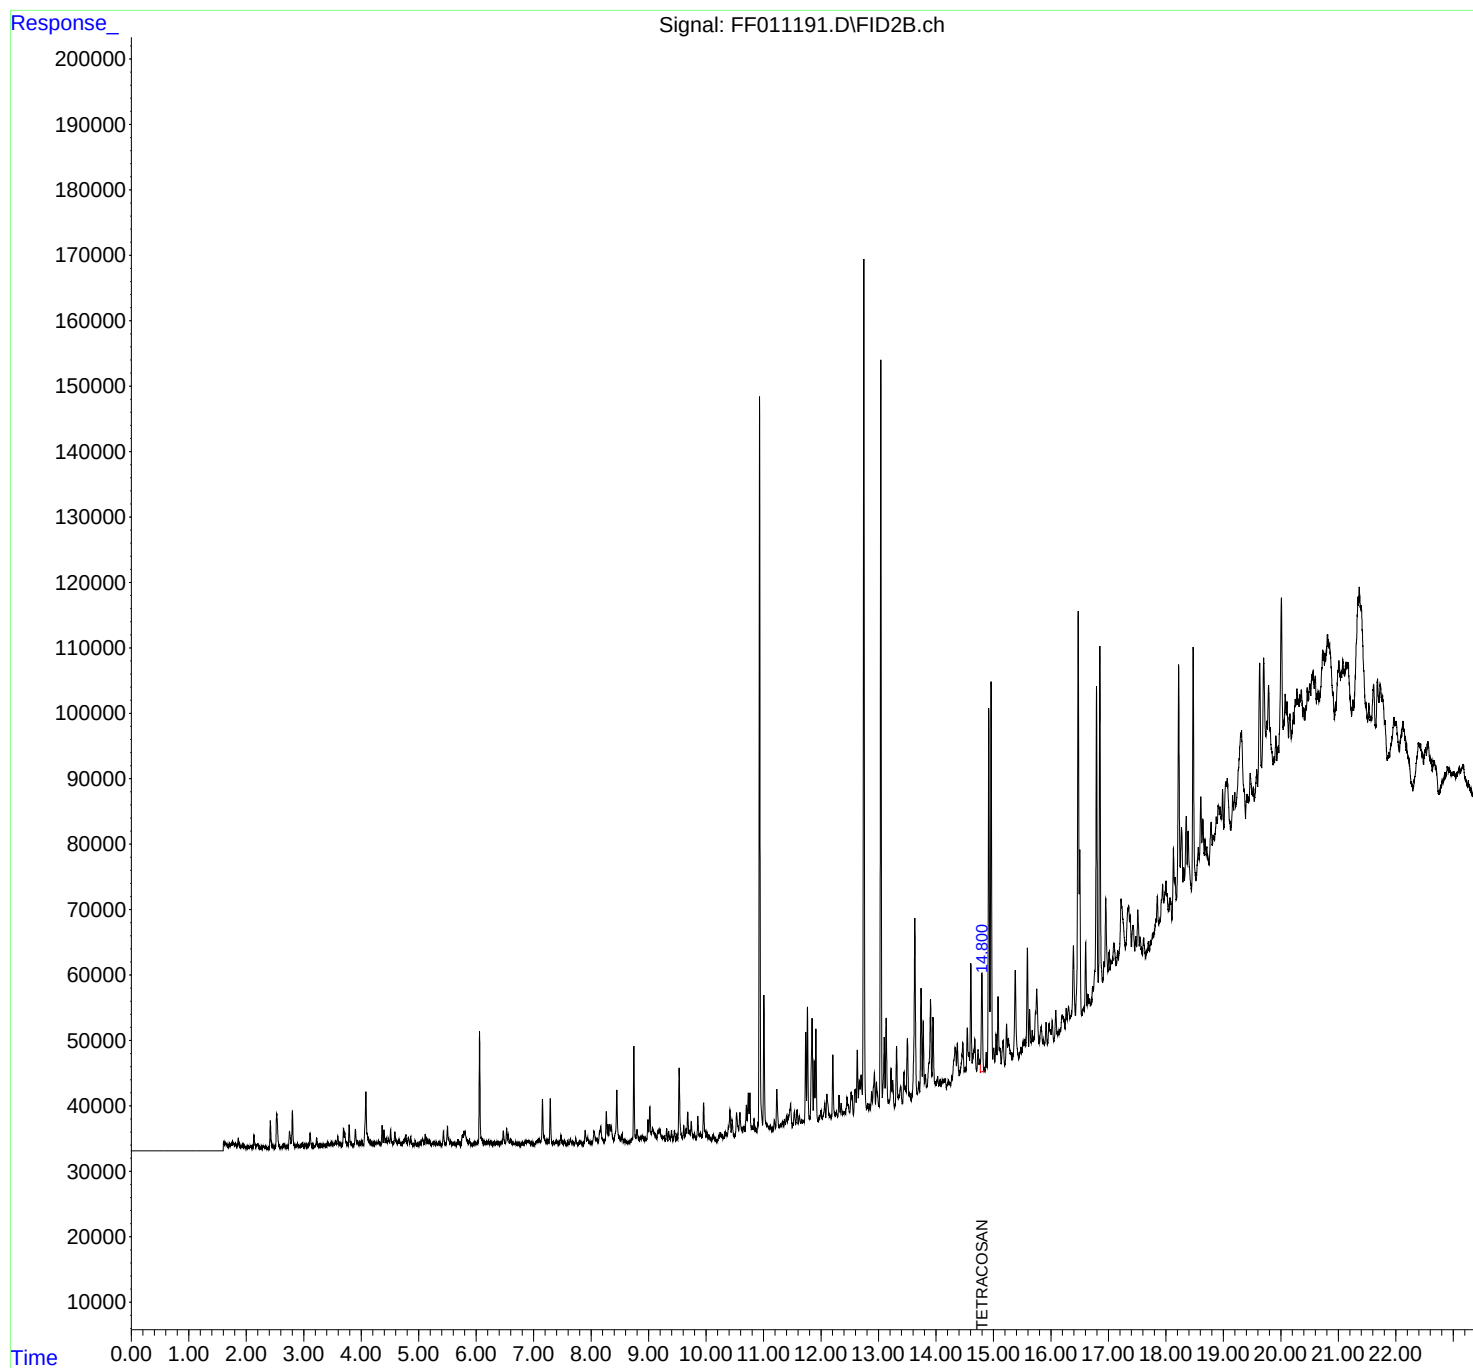

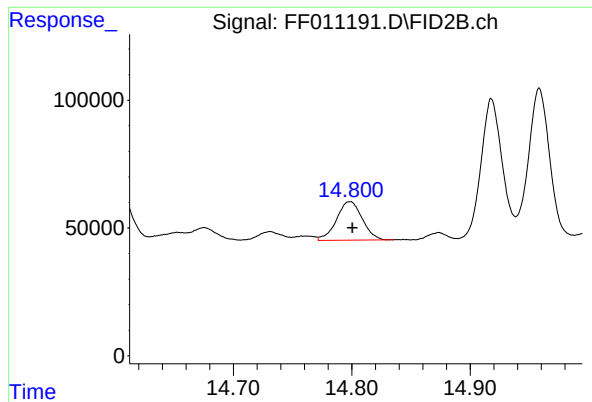

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.799 min
Delta R.T.: -0.002 min
Response: 228619
Conc: 2.10 ug/ml

Instrument :
FID_F
ClientSampleId :
JERSEY-CITY-SP