

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080524AL\
Data File : FF014393.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2024 15:04
Operator : YP\AJ
Sample : I.BLK
Misc : 4 PPM WATER LOD
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 06 06:25:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 072924.M
Quant Title : GC Extractables
QLast Update : Tue Jul 30 05:51:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.982	57418	0.514 ug/ml
18) T	n-Dotriacontane (C32)	18.813	100440	0.915 ug/ml
19) T	n-Tetratriacontane (C34)	19.596	88627	0.863 ug/ml
20) T	n-Hexatriacontane (C36)	20.339	72999	0.818 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080524AL\
Data File : FF014393.D
Signal(s) : FID2B.ch
Acq On : 05 Aug 2024 15:04
Operator : YP\AJ
Sample : I.BLK
Misc : 4 PPM WATER LOD
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 06 06:25:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 072924.M
Quant Title : GC Extractables
QLast Update : Tue Jul 30 05:51:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

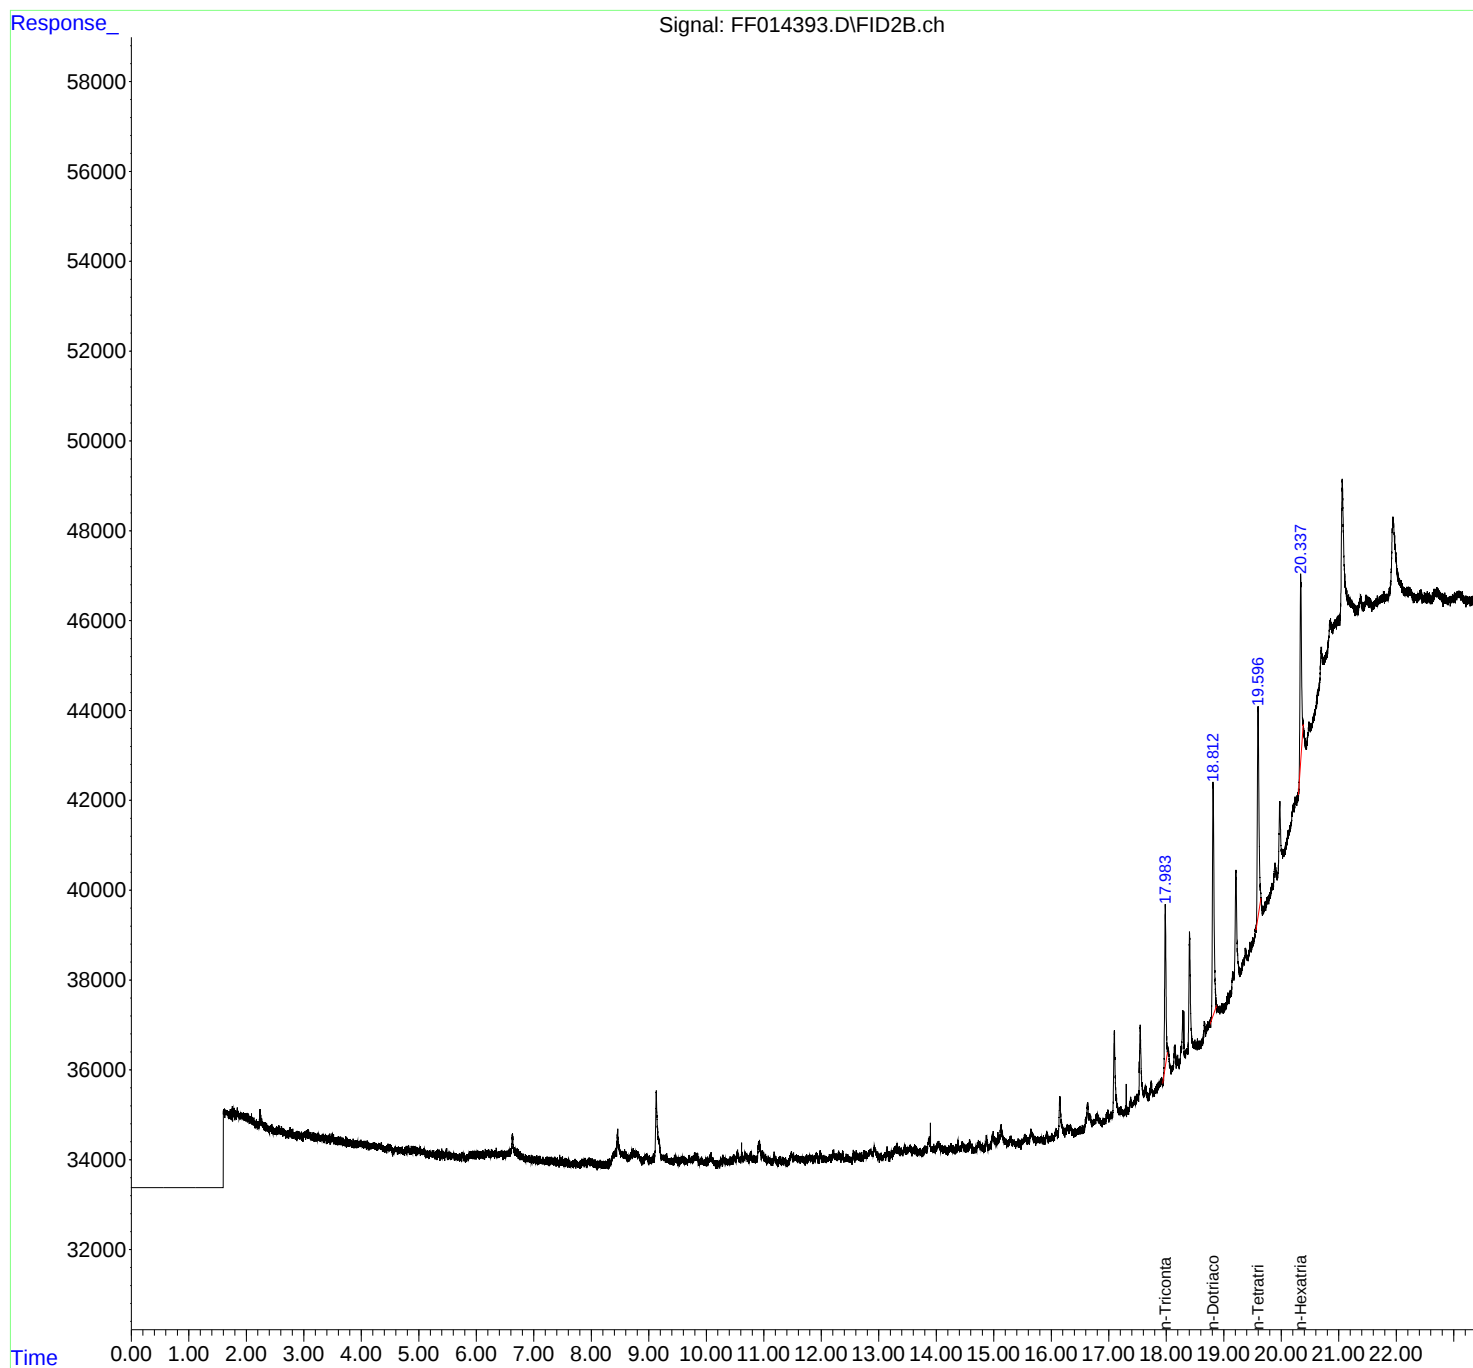


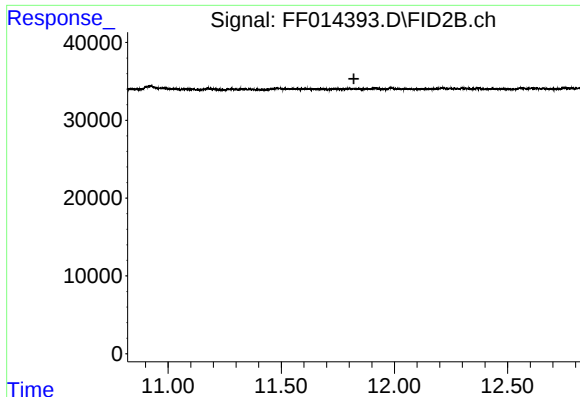

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.821 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

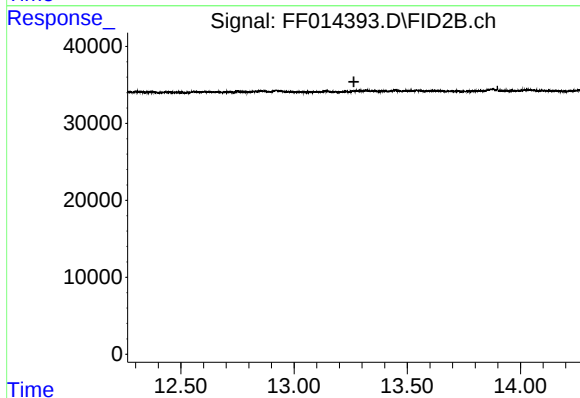


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.264 min
Response: 0
Conc: N.D.

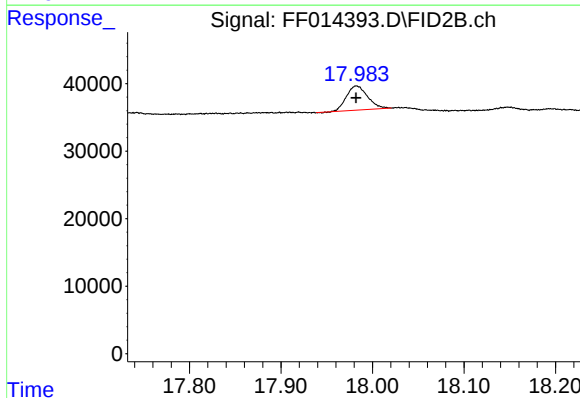


#17 n-Tricontane (C30)

R.T.: 17.982 min
Delta R.T.: 0.000 min
Response: 57418
Conc: 0.51 ug/ml

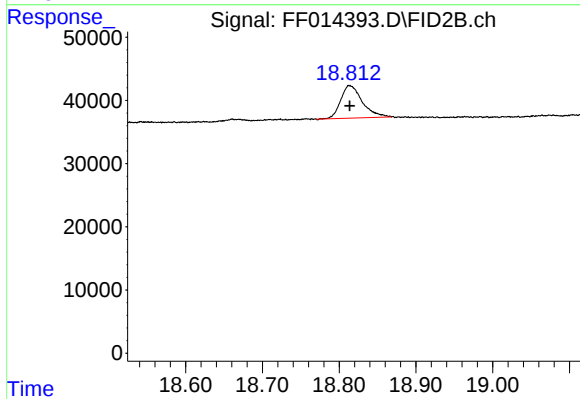

#18 n-Dotriacontane (C32)


R.T.: 18.813 min
Delta R.T.: 0.000 min
Response: 100440
Conc: 0.92 ug/ml

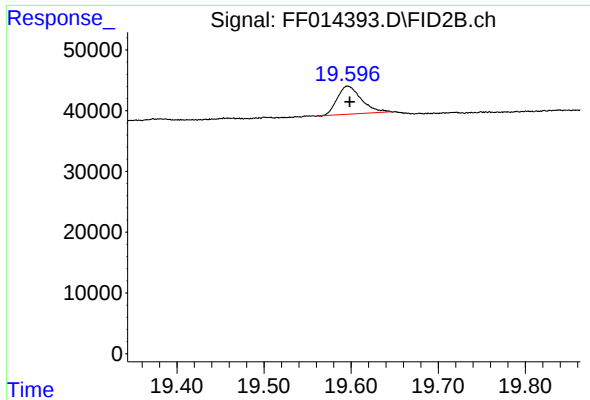

#19 n-Tetratriacontane (C34)

R.T.: 19.596 min
Delta R.T.: -0.003 min
Response: 88627
Conc: 0.86 ug/ml

Instrument :
FID_F
ClientSampleId :

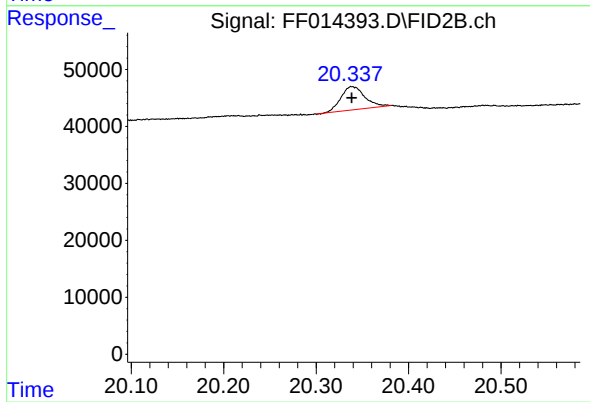

#20 n-Hexatriacontane (C36)

R.T.: 20.339 min
Delta R.T.: 0.000 min
Response: 72999
Conc: 0.82 ug/ml