

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
 Data File : FF001678.D
 Signal(s) : FID2B.ch
 Acq On : 06 Aug 2018 13:14
 Operator : AJ\SJ
 Sample : J4307-14
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 07 01:43:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.338	8704447	21.594 ug/ml
Target Compounds			
6) N-TETRADECANE	7.972	2208716	7.078 ug/ml
8) N-OCTADECANE	11.018	270948	0.859 ug/ml
9) N-EICOSANE	12.240	429800	1.362 ug/ml
10) N-TETRACOSANE	14.504	5374049	16.917 ug/ml
11) N-OCTACOSANE	16.508	1255635	3.902 ug/ml
12) N-DOTRIACONTANE	18.184	2866090	8.784 ug/ml
14) N-HEXATRIACONTANE	19.733	670079	2.272 ug/ml
15) N-TETRACONTANE	21.208	596490	2.477 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
Data File : FF001678.D
Signal(s) : FID2B.ch
Acq On : 06 Aug 2018 13:14
Operator : AJ\SJ
Sample : J4307-14
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 07 01:43:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

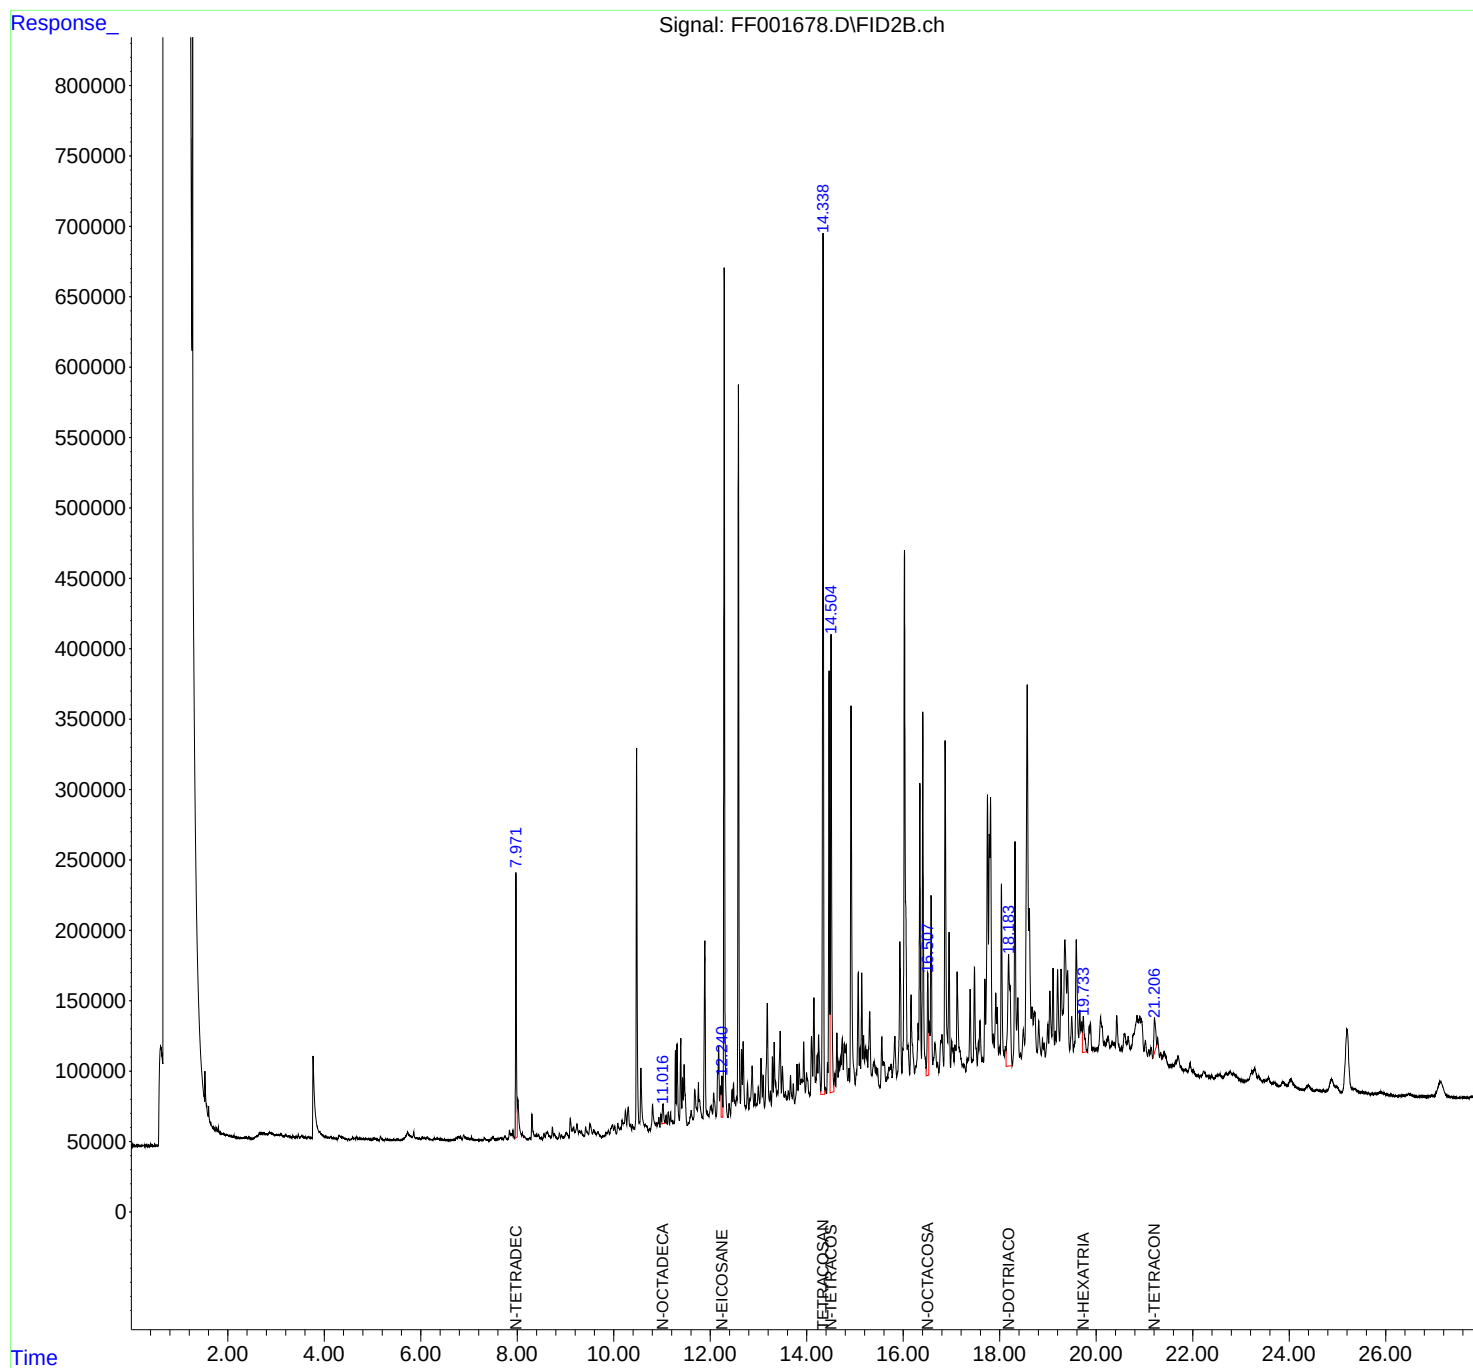

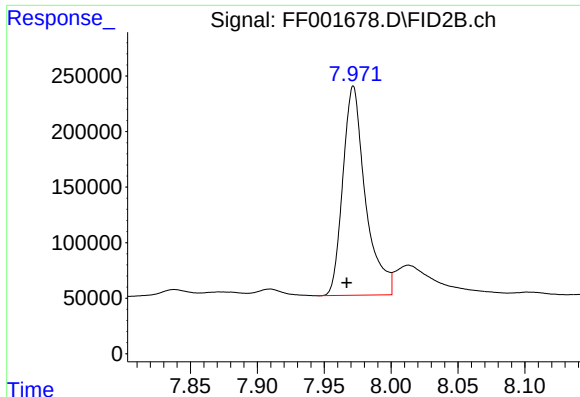


#6 N-TETRADECANE

R.T.: 7.972 min
Delta R.T.: 0.005 min
Response: 2208716
Conc: 7.08 ug/ml

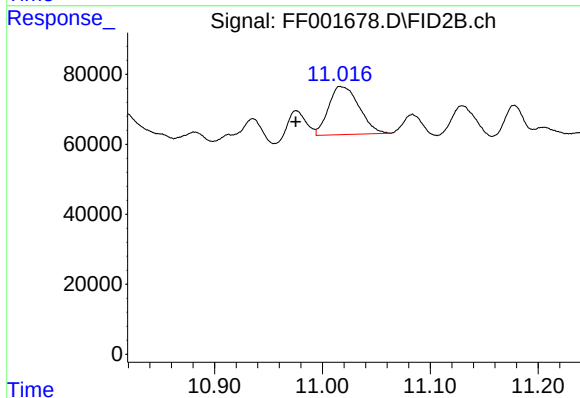


#8 N-OCTADECANE

R.T.: 11.018 min
Delta R.T.: 0.043 min
Response: 270948
Conc: 0.86 ug/ml

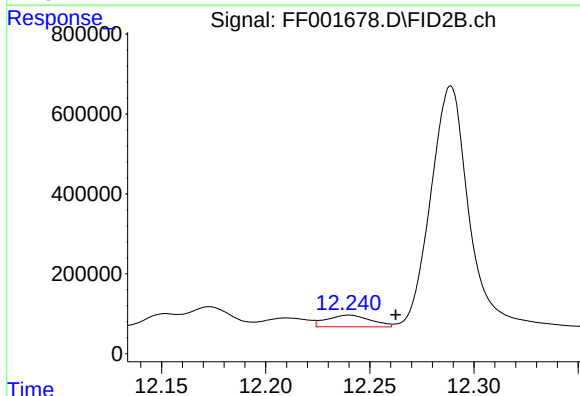


#9 N-EICOSANE

R.T.: 12.240 min
Delta R.T.: -0.023 min
Response: 429800
Conc: 1.36 ug/ml

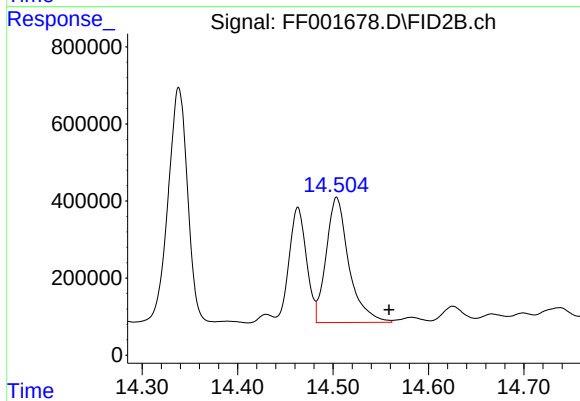


#10 N-TETRACOSANE

R.T.: 14.504 min
Delta R.T.: -0.055 min
Response: 5374049
Conc: 16.92 ug/ml

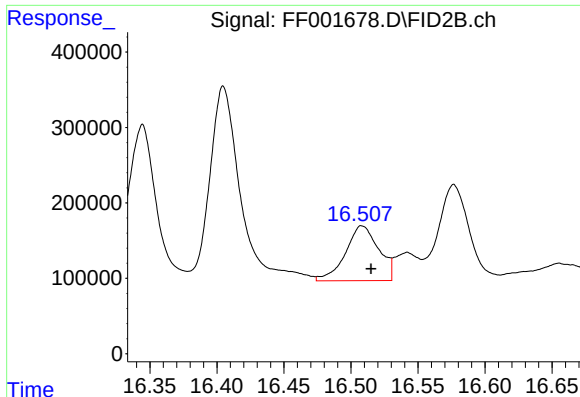


#11 N-OCTACOSANE

R.T.: 16.508 min
Delta R.T.: -0.007 min
Response: 1255635
Conc: 3.90 ug/ml

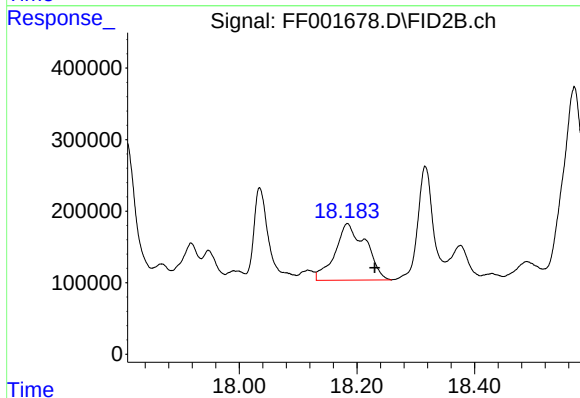


#12 N-DOTRIACONTANE

R.T.: 18.184 min
Delta R.T.: -0.047 min
Response: 2866090
Conc: 8.78 ug/ml

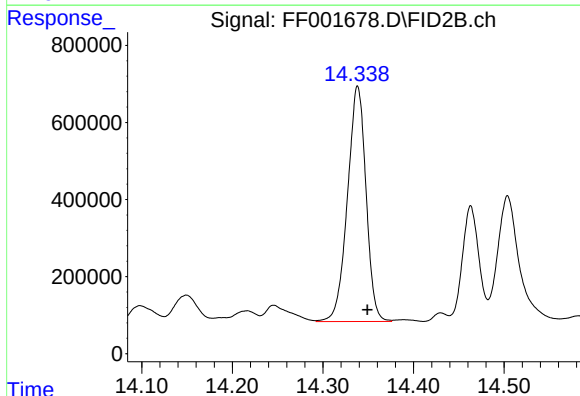


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.338 min
Delta R.T.: -0.011 min
Response: 8704447
Conc: 21.59 ug/ml

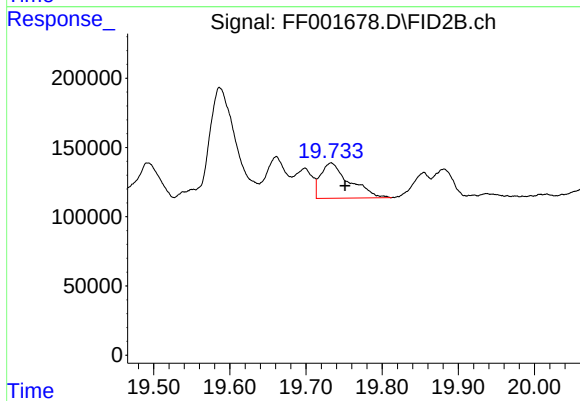

#14 N-HEXATRIACONTANE

R.T.: 19.733 min
Delta R.T.: -0.018 min
Response: 670079
Conc: 2.27 ug/ml

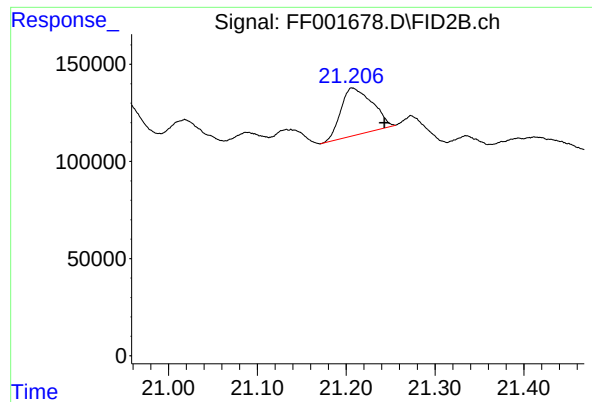

#15 N-TETRACONTANE

R.T.: 21.208 min
Delta R.T.: -0.036 min
Response: 596490
Conc: 2.48 ug/ml