

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
Data File : FF001679.D
Signal(s) : FID2B.ch
Acq On : 06 Aug 2018 13:50
Operator : AJ\SJ
Sample : J4307-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 07 01:43:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.335	4960991	12.307 ug/ml
Target Compounds			
6) N-TETRADECANE	7.972	1148136	3.679 ug/ml
9) N-EICOSANE	12.288	1560526	4.947 ug/ml
10) N-TETRACOSANE	14.506	1366655	4.302 ug/ml
11) N-OCTACOSANE	16.501	266122	0.827 ug/ml
12) N-DOTRIACONTANE	18.212	856690	2.626 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
Data File : FF001679.D
Signal(s) : FID2B.ch
Acq On : 06 Aug 2018 13:50
Operator : AJ\SJ
Sample : J4307-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 07 01:43:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

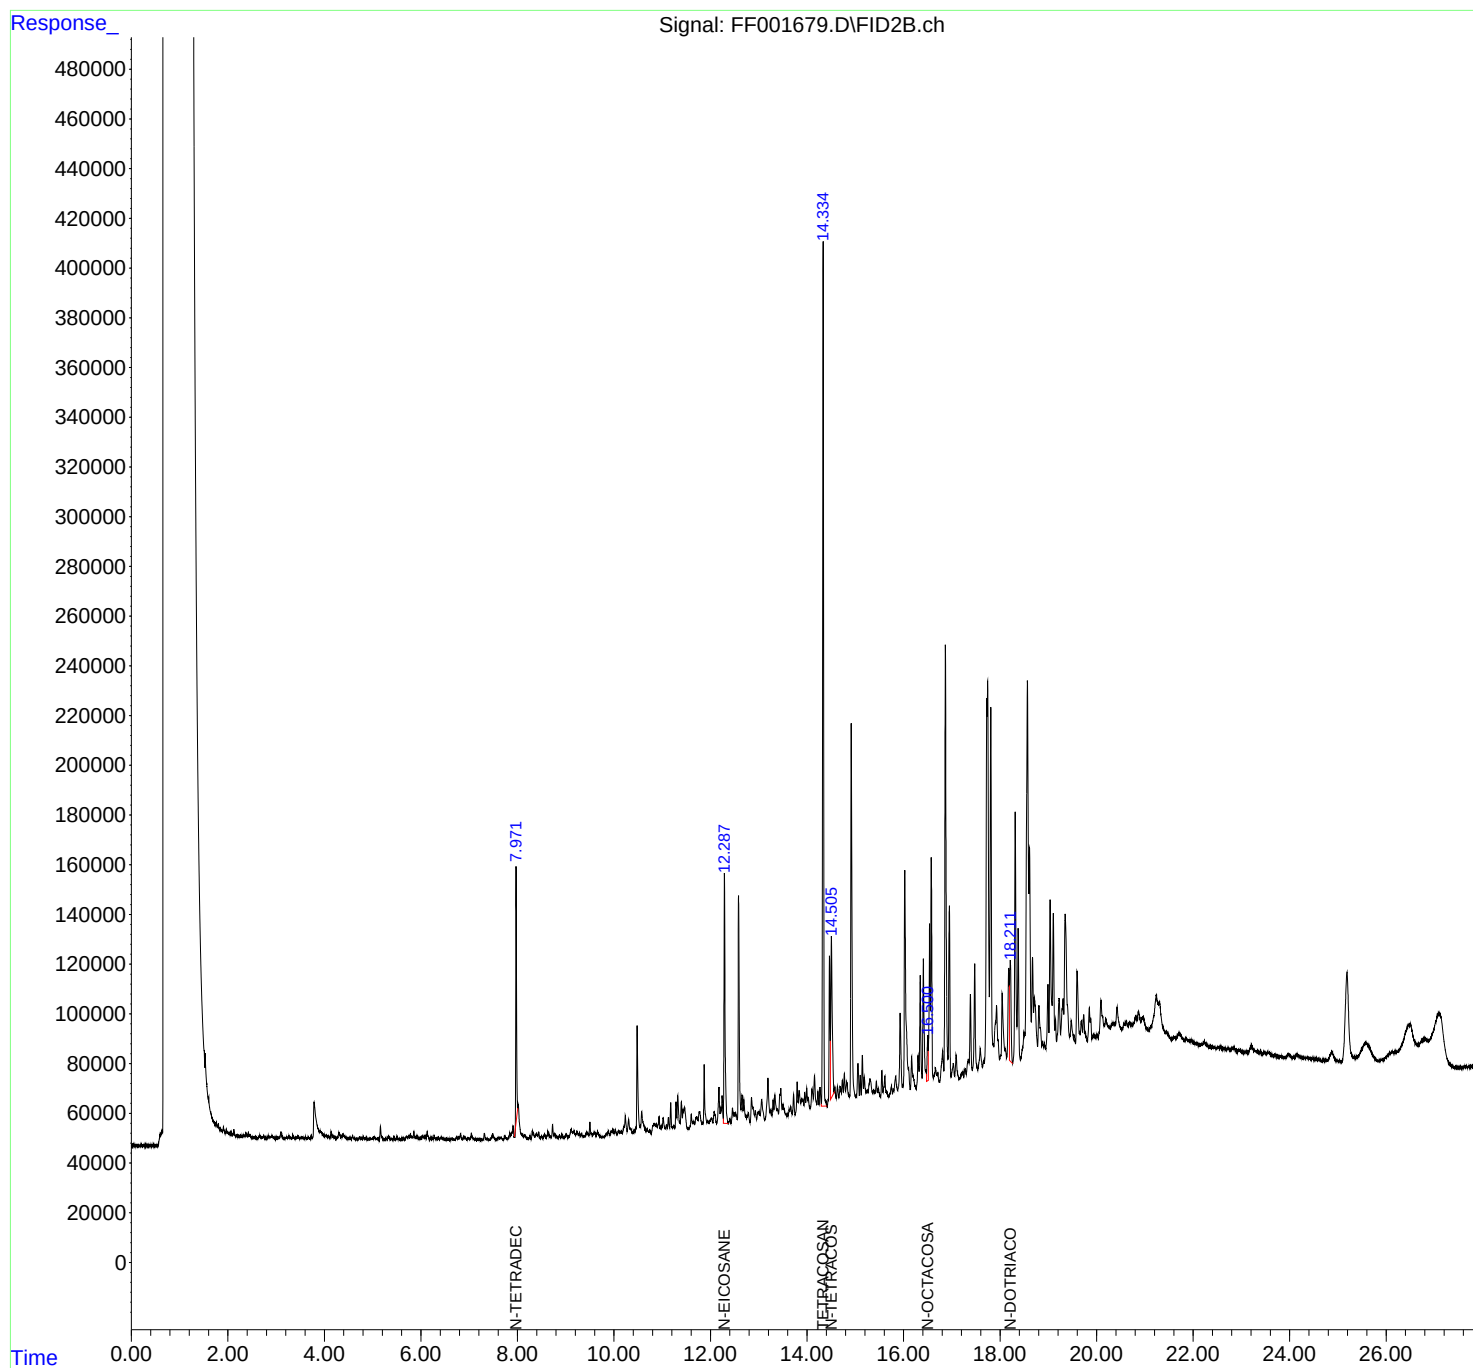

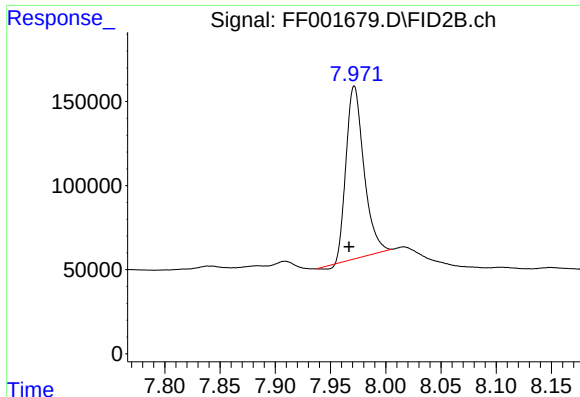


#6 N-TETRADECANE

R.T.: 7.972 min
Delta R.T.: 0.005 min
Response: 1148136
Conc: 3.68 ug/ml

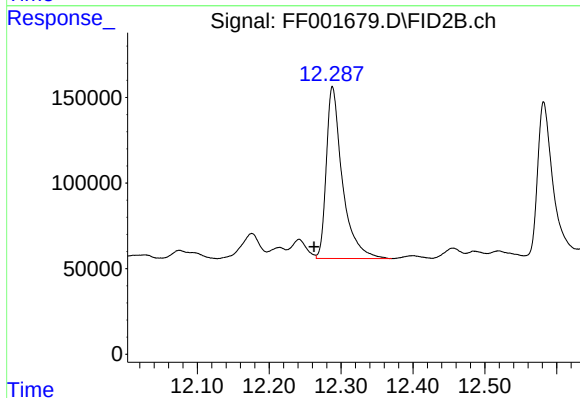


#9 N-EICOSANE

R.T.: 12.288 min
Delta R.T.: 0.026 min
Response: 1560526
Conc: 4.95 ug/ml

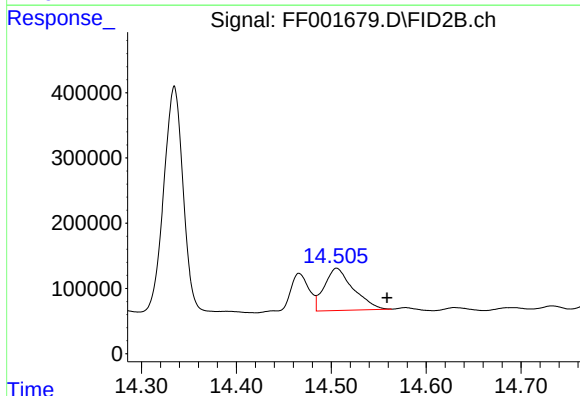


#10 N-TETRACOSANE

R.T.: 14.506 min
Delta R.T.: -0.053 min
Response: 1366655
Conc: 4.30 ug/ml

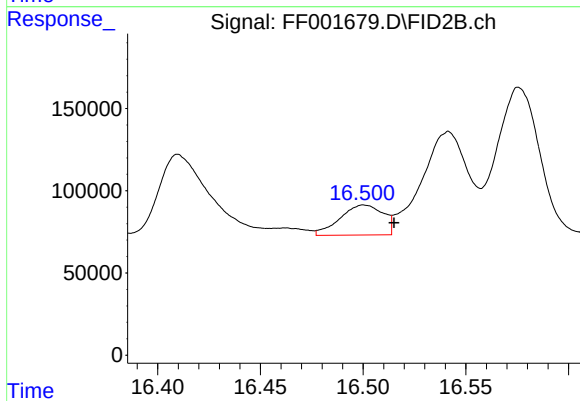


#11 N-OCTACOSANE

R.T.: 16.501 min
Delta R.T.: -0.015 min
Response: 266122
Conc: 0.83 ug/ml

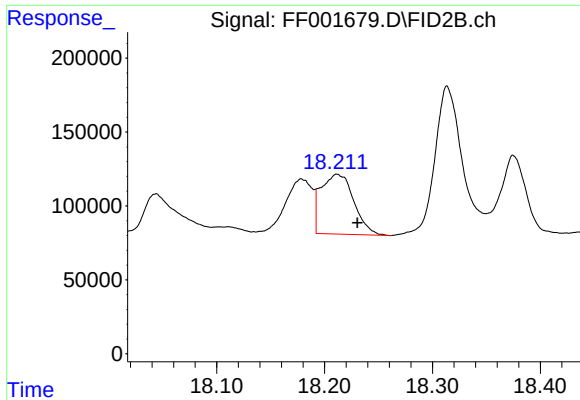

#12 N-DOTRIACONTANE

R.T.: 18.212 min
Delta R.T.: -0.019 min
Response: 856690
Conc: 2.63 ug/ml

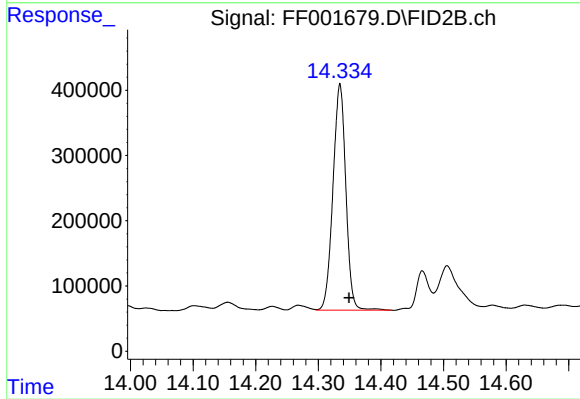

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.335 min
Delta R.T.: -0.014 min
Response: 4960991
Conc: 12.31 ug/ml