

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
 Data File : FF001691.D
 Signal(s) : FID2B.ch
 Acq On : 06 Aug 2018 21:05
 Operator : AJ\SJ
 Sample : J4307-08
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 07 01:46:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.334	5624889	13.954 ug/ml
Target Compounds			
6) N-TETRADECANE	7.969	1503211	4.817 ug/ml
9) N-EICOSANE	12.285	4929848	15.627 ug/ml
10) N-TETRACOSANE	14.499	4005717	12.610 ug/ml
11) N-OCTACOSANE	16.506	805398	2.503 ug/ml
12) N-DOTRIACONTANE	18.209	663511	2.034 ug/ml
15) N-TETRACONTANE	21.221	454036	1.886 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
Data File : FF001691.D
Signal(s) : FID2B.ch
Acq On : 06 Aug 2018 21:05
Operator : AJ\SJ
Sample : J4307-08
Misc :
ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 07 01:46:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

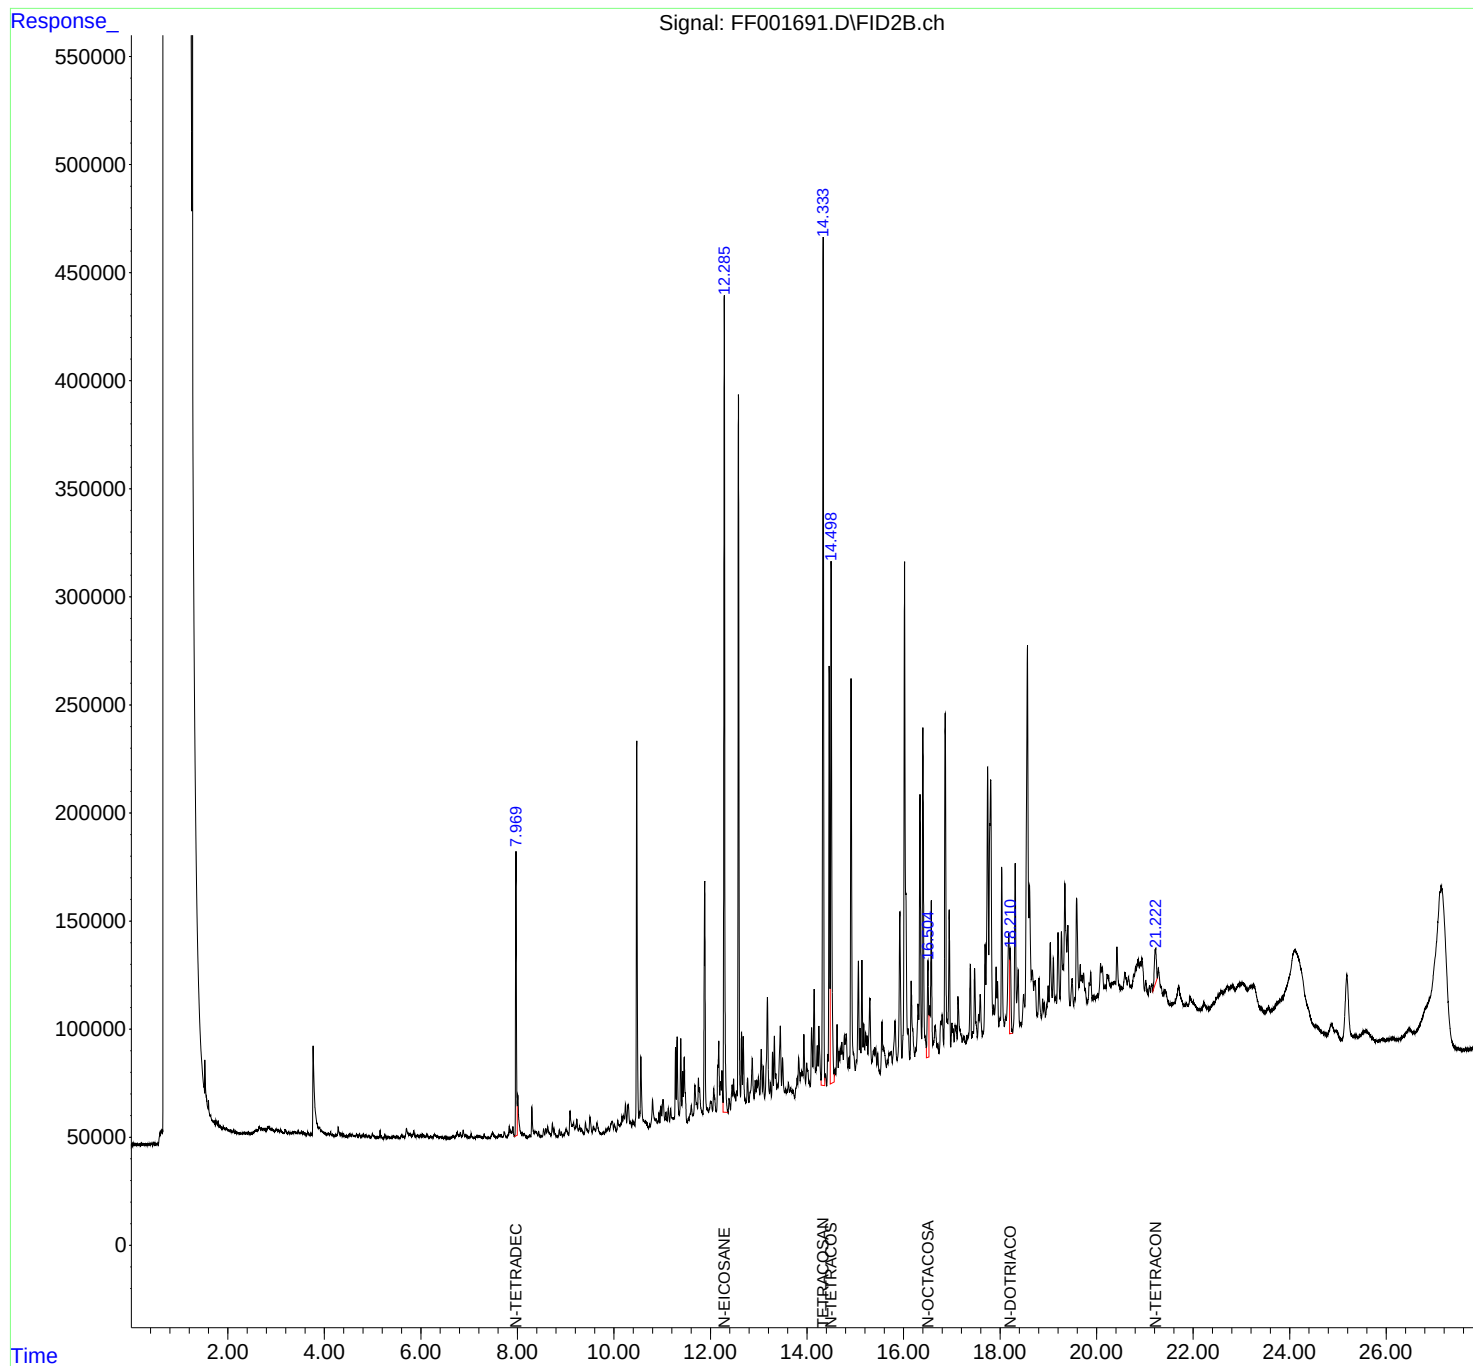

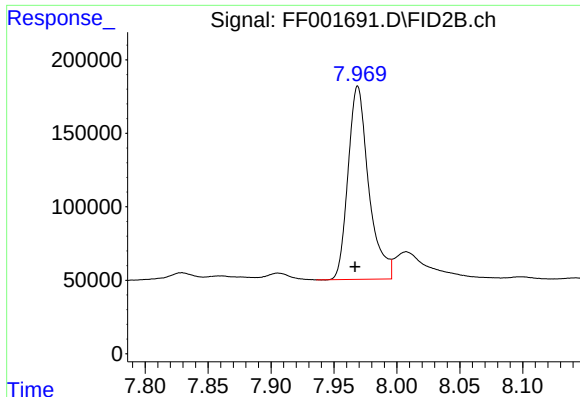


#6 N-TETRADECANE

R.T.: 7.969 min
Delta R.T.: 0.002 min
Response: 1503211
Conc: 4.82 ug/ml

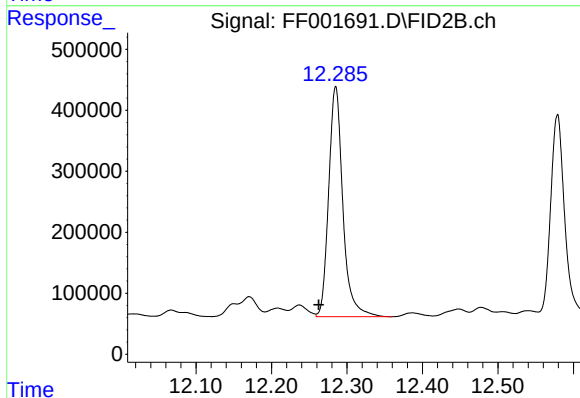


#9 N-EICOSANE

R.T.: 12.285 min
Delta R.T.: 0.023 min
Response: 4929848
Conc: 15.63 ug/ml

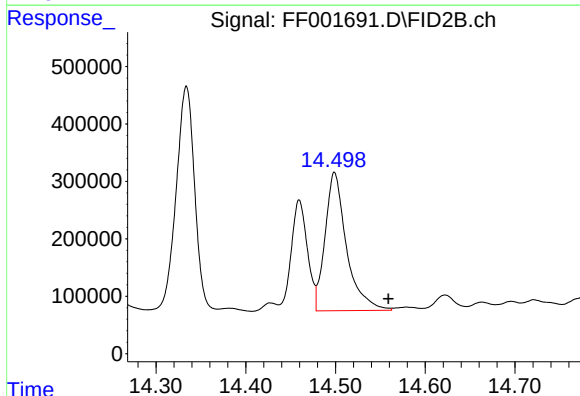


#10 N-TETRACOSANE

R.T.: 14.499 min
Delta R.T.: -0.060 min
Response: 4005717
Conc: 12.61 ug/ml

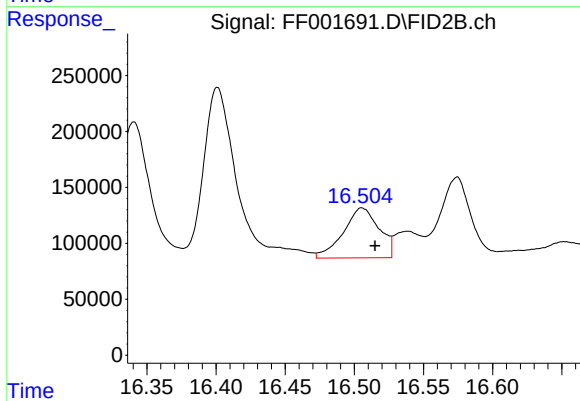


#11 N-OCTACOSANE

R.T.: 16.506 min
Delta R.T.: -0.009 min
Response: 805398
Conc: 2.50 ug/ml

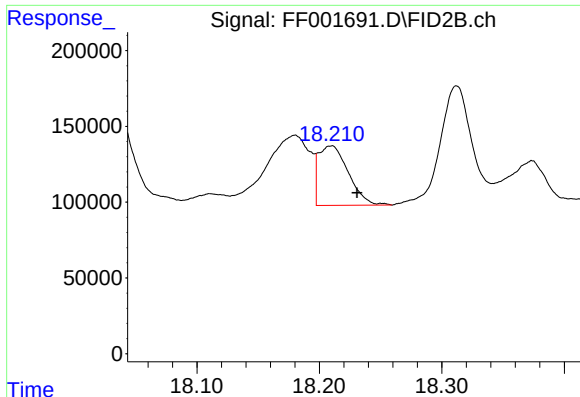


#12 N-DOTRIACONTANE

R.T.: 18.209 min
Delta R.T.: -0.021 min
Response: 663511
Conc: 2.03 ug/ml

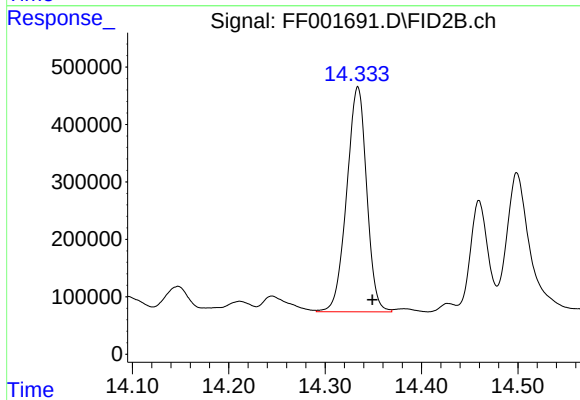

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.334 min
Delta R.T.: -0.015 min
Response: 5624889
Conc: 13.95 ug/ml

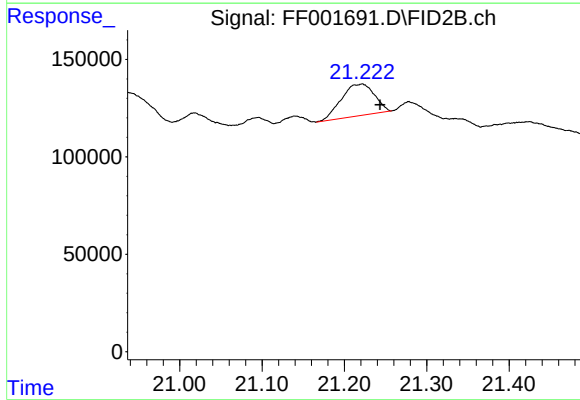

#15 N-TETRACONTANE

R.T.: 21.221 min
Delta R.T.: -0.022 min
Response: 454036
Conc: 1.89 ug/ml