

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
 Data File : FF001693.D
 Signal(s) : FID2B.ch
 Acq On : 06 Aug 2018 22:18
 Operator : AJ\SJ
 Sample : J4307-06
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 07 01:46:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.333	4064183	10.082 ug/ml
Target Compounds			
6) N-TETRADECANE	7.969	1257097	4.028 ug/ml
9) N-EICOSANE	12.284	3355509	10.637 ug/ml
10) N-TETRACOSANE	14.497	6639031	20.899 ug/ml
11) N-OCTACOSANE	16.508	678052	2.107 ug/ml
12) N-DOTRIACONTANE	18.210	682315	2.091 ug/ml
14) N-HEXATRIACONTANE	19.692	372869	1.264 ug/ml
15) N-TETRACONTANE	21.227	1235258	5.130 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
Data File : FF001693.D
Signal(s) : FID2B.ch
Acq On : 06 Aug 2018 22:18
Operator : AJ\SJ
Sample : J4307-06
Misc :
ALS Vial : 68 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 07 01:46:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

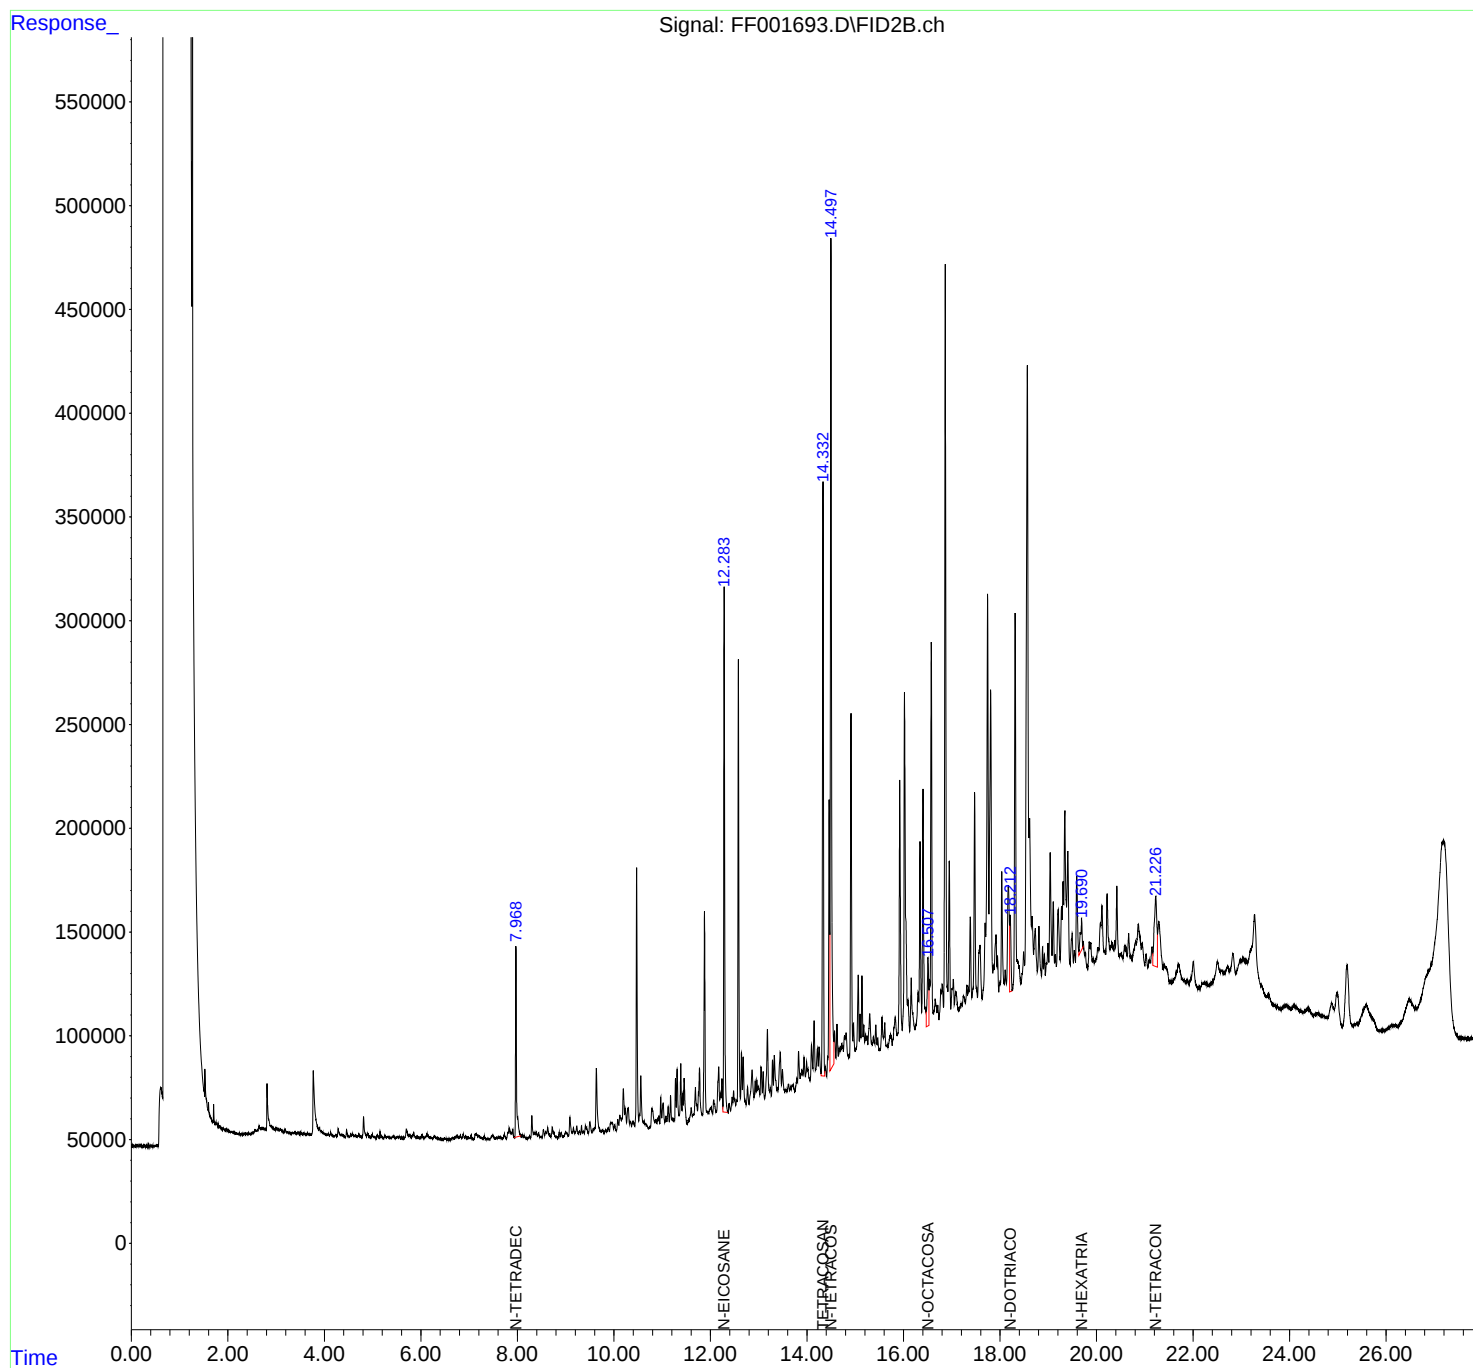

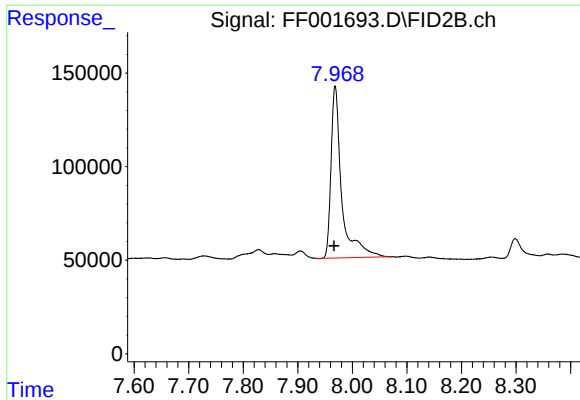


#6 N-TETRADECANE

R.T.: 7.969 min
Delta R.T.: 0.002 min
Response: 1257097
Conc: 4.03 ug/ml

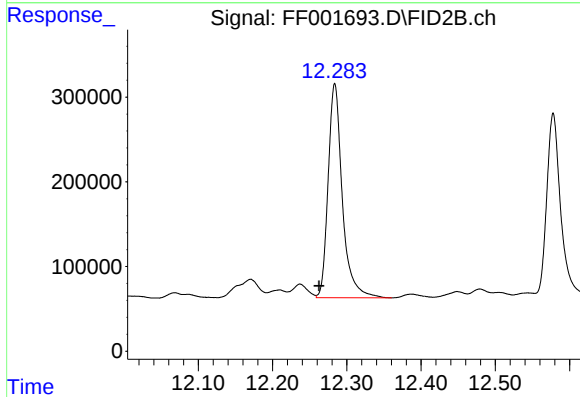


#9 N-EICOSANE

R.T.: 12.284 min
Delta R.T.: 0.021 min
Response: 3355509
Conc: 10.64 ug/ml

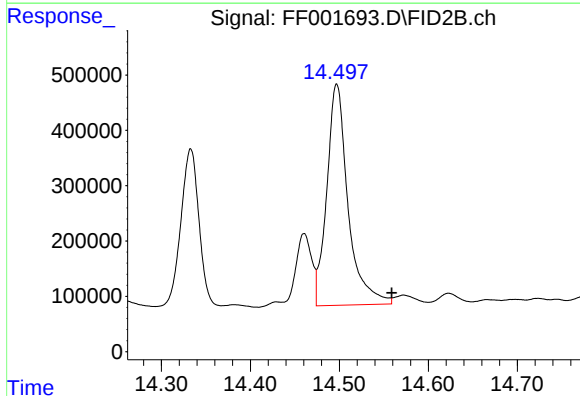


#10 N-TETRACOSANE

R.T.: 14.497 min
Delta R.T.: -0.062 min
Response: 6639031
Conc: 20.90 ug/ml

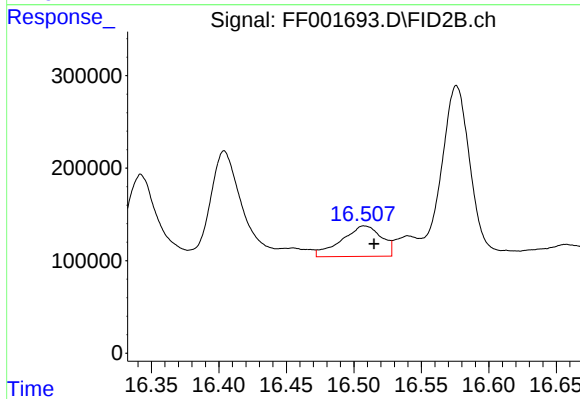


#11 N-OCTACOSANE

R.T.: 16.508 min
Delta R.T.: -0.007 min
Response: 678052
Conc: 2.11 ug/ml

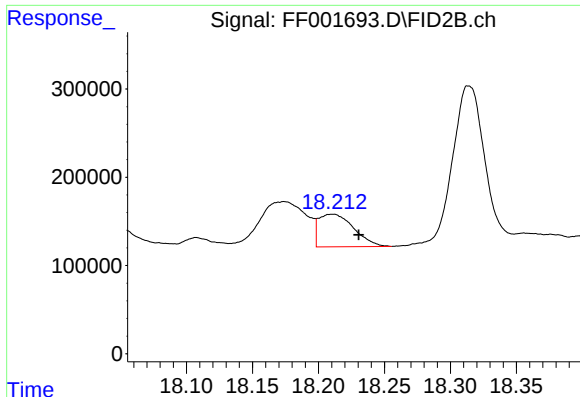


#12 N-DOTRIACONTANE

R.T.: 18.210 min
Delta R.T.: -0.020 min
Response: 682315
Conc: 2.09 ug/ml

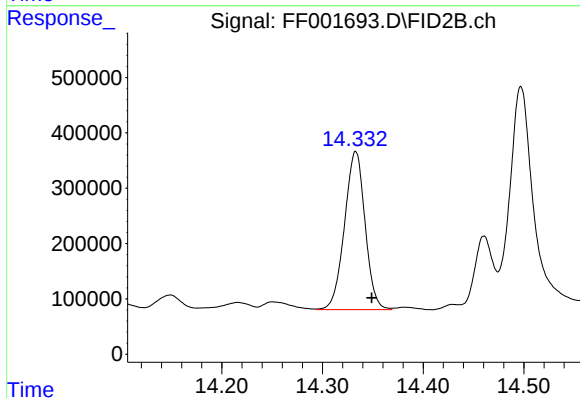


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.333 min
Delta R.T.: -0.016 min
Response: 4064183
Conc: 10.08 ug/ml

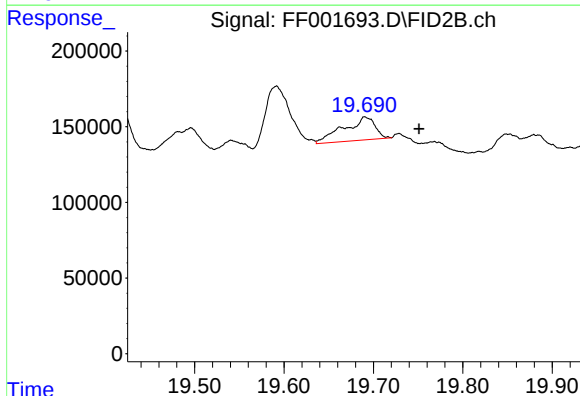

#14 N-HEXATRIACONTANE

R.T.: 19.692 min
Delta R.T.: -0.059 min
Response: 372869
Conc: 1.26 ug/ml

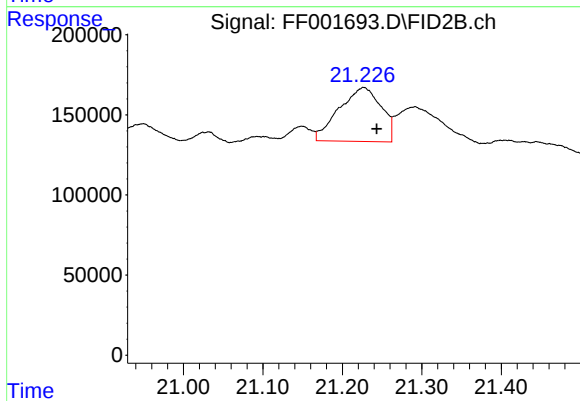

#15 N-TETRACONTANE

R.T.: 21.227 min
Delta R.T.: -0.016 min
Response: 1235258
Conc: 5.13 ug/ml