

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
 Data File : FF001698.D
 Signal(s) : FID2B.ch
 Acq On : 07 Aug 2018 01:18
 Operator : AJ\SJ
 Sample : J4307-09
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 07 04:35:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.352	20199149	50.109 ug/ml
Target Compounds			
6) N-TETRADECANE	7.970	2342436	7.506 ug/ml
7) N-HEXADECANE	9.500	1913116	6.076 ug/ml
8) N-OCTADECANE	11.002	6801512	21.563 ug/ml
9) N-EICOSANE	12.253	8209744	26.024 ug/ml
10) N-TETRACOSANE	14.562	45387834	142.878 ug/ml
11) N-OCTACOSANE	16.545	9273582	28.817 ug/ml
12) N-DOTRIACONTANE	18.216	12035146	36.886 ug/ml
14) N-HEXATRIACONTANE	19.760	6340087	21.493 ug/ml
15) N-TETRACONTANE	21.254	3725187	15.472 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
Data File : FF001698.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2018 01:18
Operator : AJ\SJ
Sample : J4307-09
Misc :
ALS Vial : 73 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 07 04:35:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

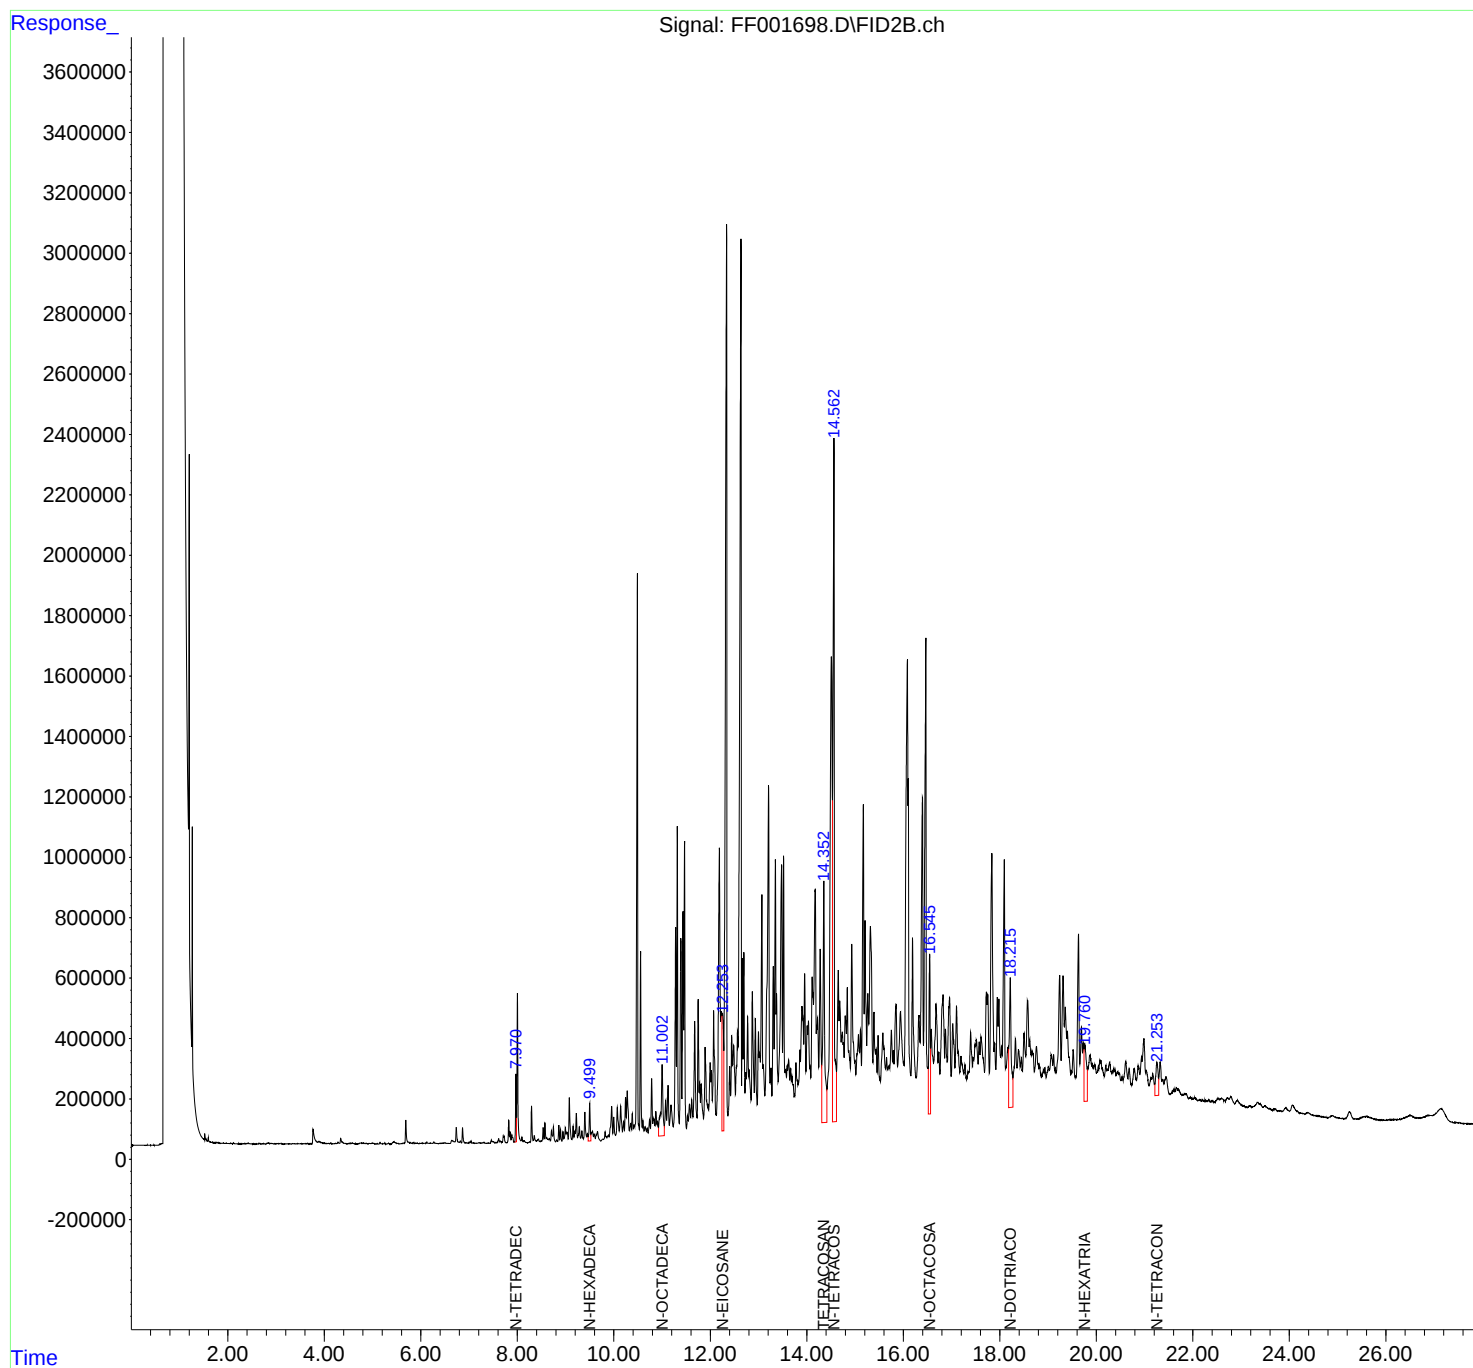

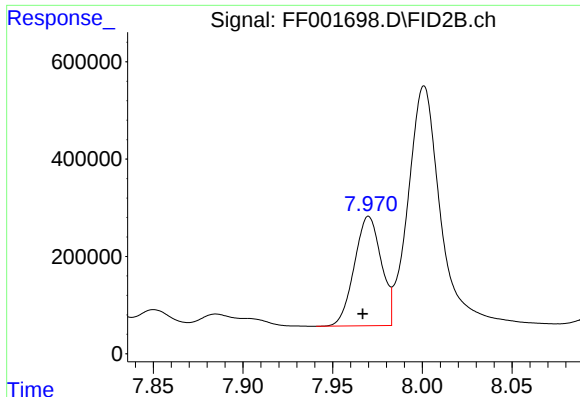


#6 N-TETRADECANE

R.T.: 7.970 min
Delta R.T.: 0.003 min
Response: 2342436
Conc: 7.51 ug/ml

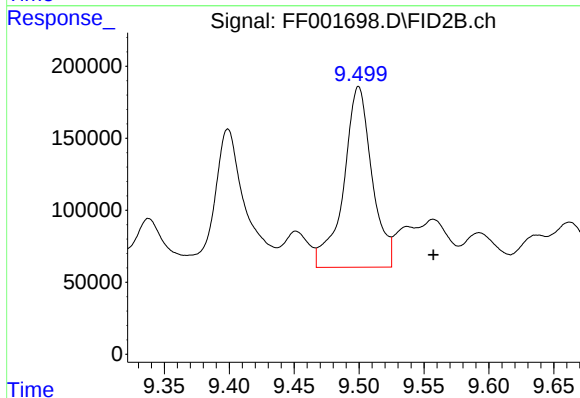


#7 N-HEXADECANE

R.T.: 9.500 min
Delta R.T.: -0.058 min
Response: 1913116
Conc: 6.08 ug/ml

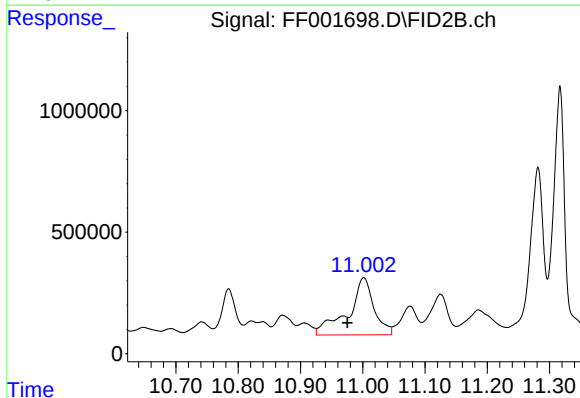


#8 N-OCTADECANE

R.T.: 11.002 min
Delta R.T.: 0.026 min
Response: 6801512
Conc: 21.56 ug/ml

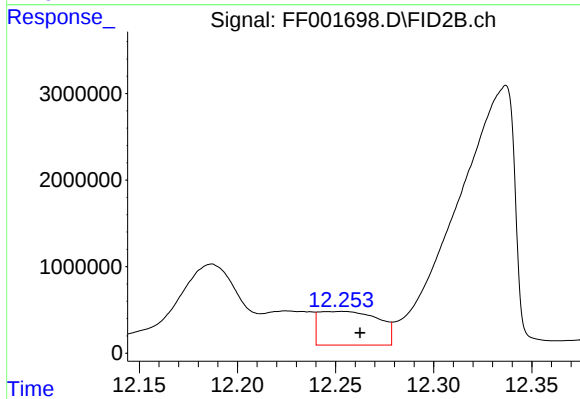


#9 N-EICOSANE

R.T.: 12.253 min
Delta R.T.: -0.010 min
Response: 8209744
Conc: 26.02 ug/ml

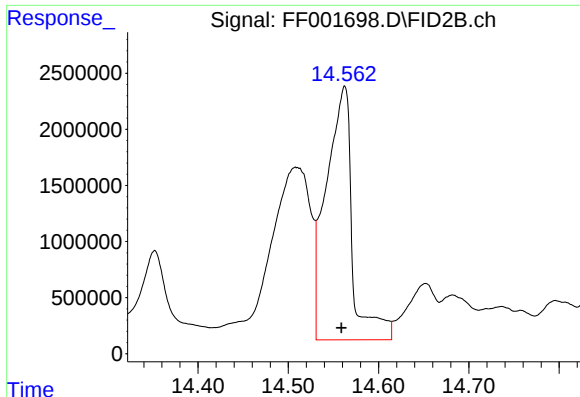


#10 N-TETRACOSANE

R.T.: 14.562 min
Delta R.T.: 0.003 min
Response: 45387834
Conc: 142.88 ug/ml

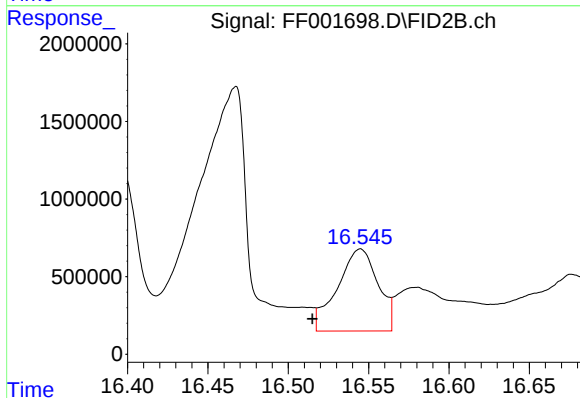


#11 N-OCTACOSANE

R.T.: 16.545 min
Delta R.T.: 0.030 min
Response: 9273582
Conc: 28.82 ug/ml

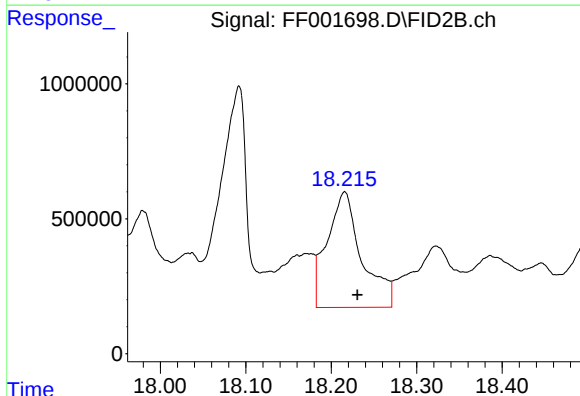


#12 N-DOTRIACONTANE

R.T.: 18.216 min
Delta R.T.: -0.015 min
Response: 12035146
Conc: 36.89 ug/ml

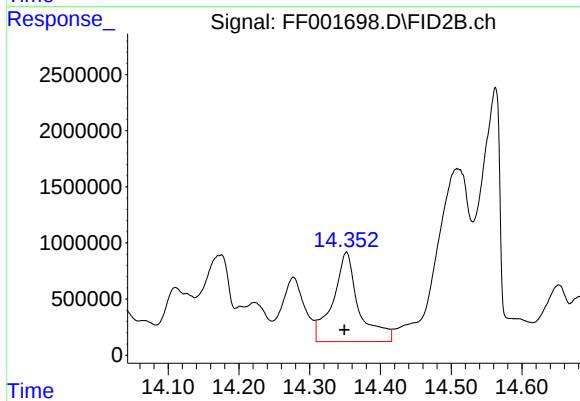


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.352 min
Delta R.T.: 0.003 min
Response: 20199149
Conc: 50.11 ug/ml

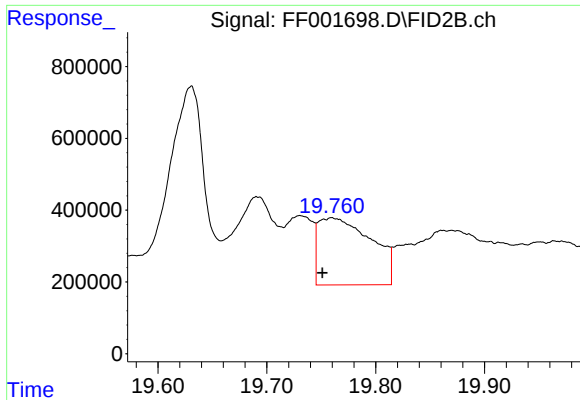

#14 N-HEXATRIACONTANE

R.T.: 19.760 min
Delta R.T.: 0.009 min
Response: 6340087
Conc: 21.49 ug/ml

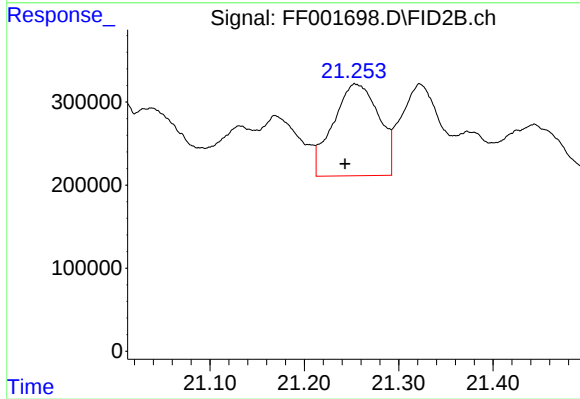

#15 N-TETRACONTANE

R.T.: 21.254 min
Delta R.T.: 0.011 min
Response: 3725187
Conc: 15.47 ug/ml