

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
 Data File : FF001700.D
 Signal(s) : FID2B.ch
 Acq On : 07 Aug 2018 02:30
 Operator : AJ\SJ
 Sample : J4307-19
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 07 04:36:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.334	7456850	18.499 ug/ml
Target Compounds			
6) N-TETRADECANE	7.969	1635300	5.240 ug/ml
8) N-OCTADECANE	10.973	201448	0.639 ug/ml
9) N-EICOSANE	12.283	3212786	10.184 ug/ml
10) N-TETRACOSANE	14.619	164331	0.517 ug/ml
11) N-OCTACOSANE	16.503	483408	1.502 ug/ml
12) N-DOTRIACONTANE	18.207	653626	2.003 ug/ml
15) N-TETRACONTANE	21.220	238054	0.989 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
Data File : FF001700.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2018 02:30
Operator : AJ\SJ
Sample : J4307-19
Misc :
ALS Vial : 75 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 07 04:36:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

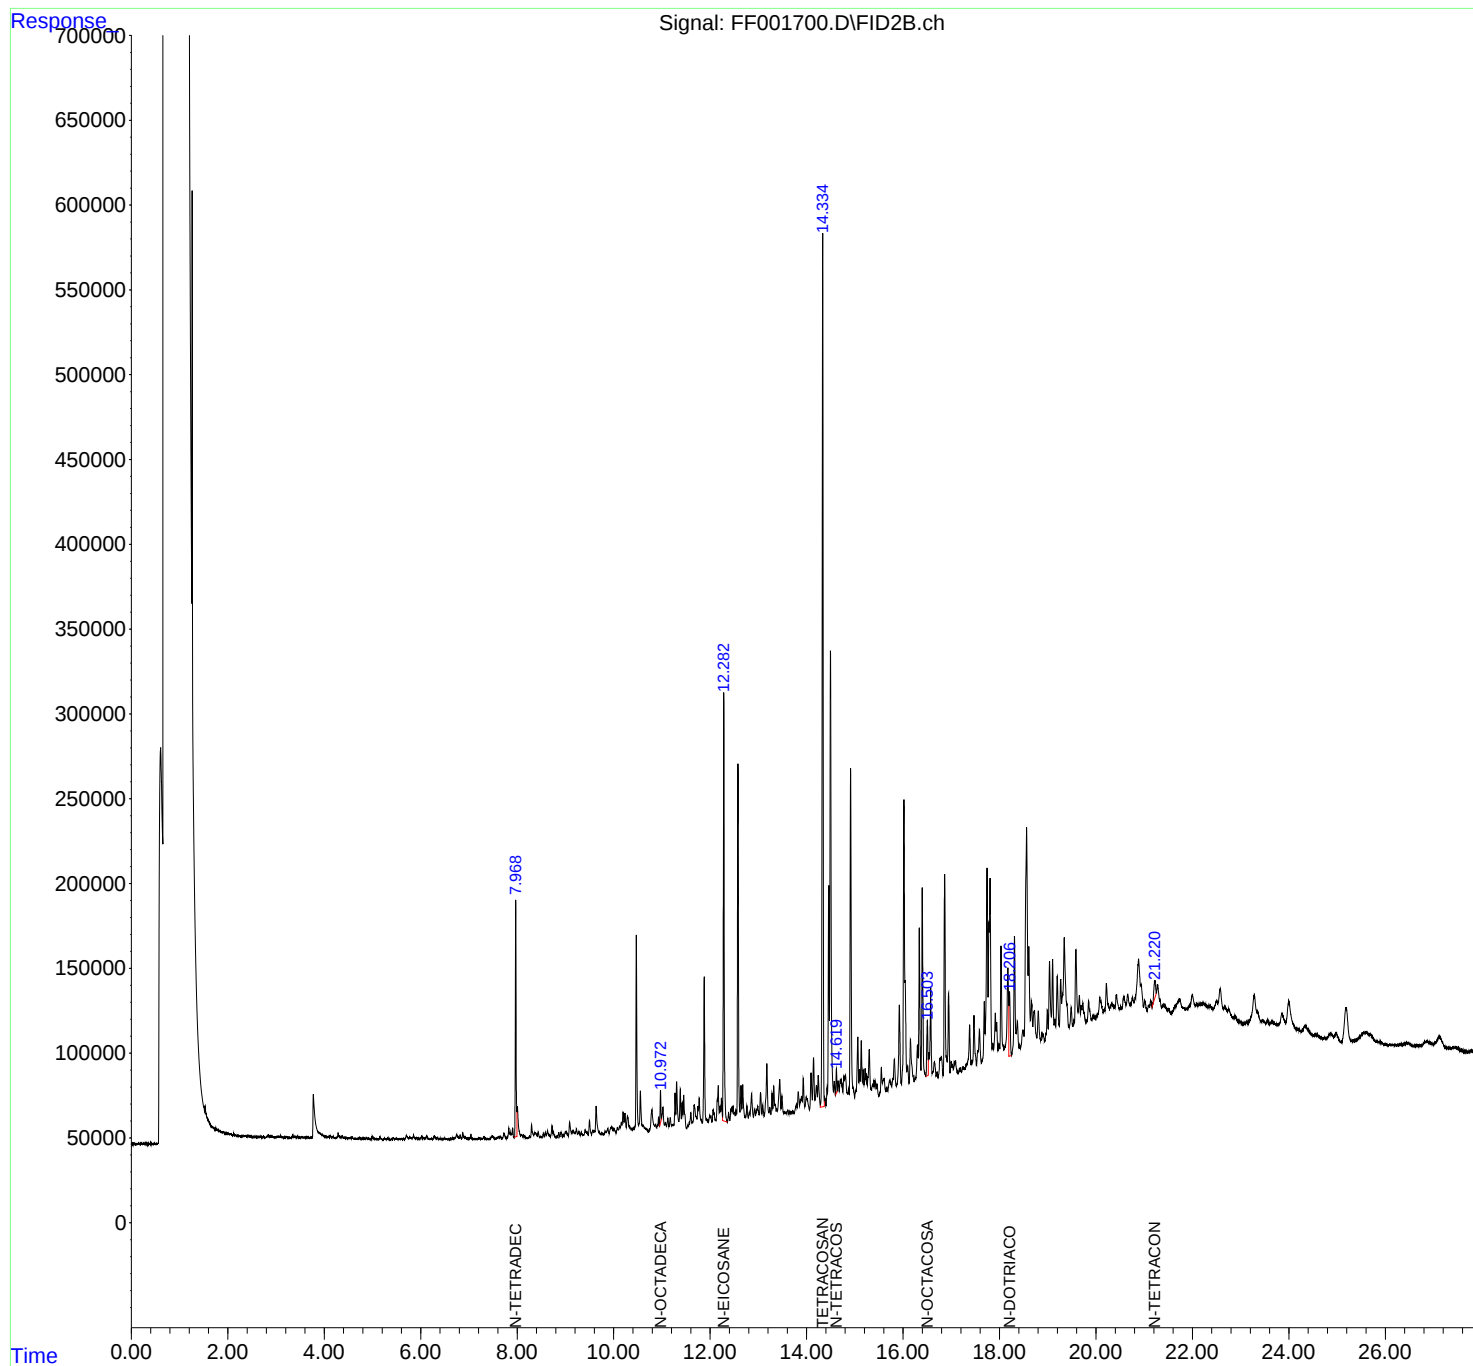

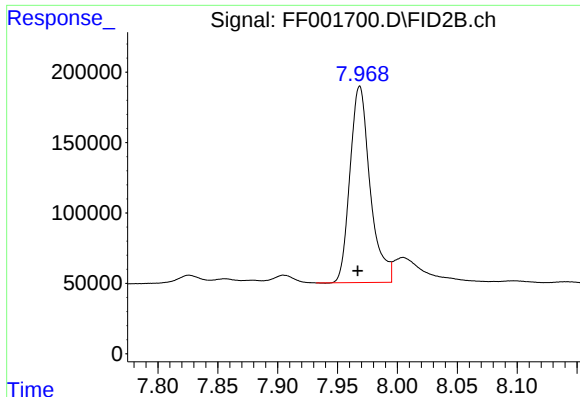


#6 N-TETRADECANE

R.T.: 7.969 min
Delta R.T.: 0.002 min
Response: 1635300
Conc: 5.24 ug/ml

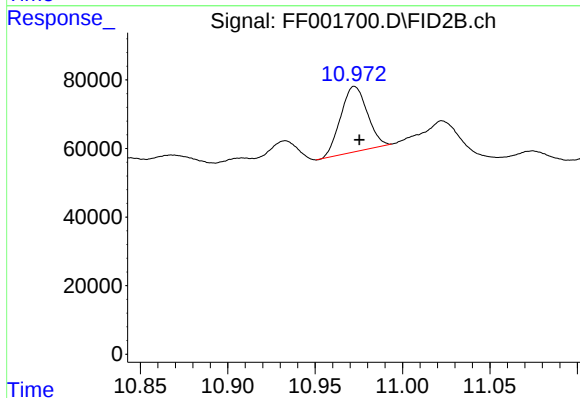


#8 N-OCTADECANE

R.T.: 10.973 min
Delta R.T.: -0.003 min
Response: 201448
Conc: 0.64 ug/ml

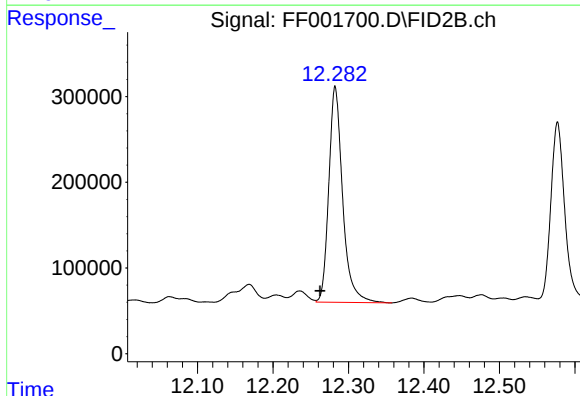


#9 N-EICOSANE

R.T.: 12.283 min
Delta R.T.: 0.020 min
Response: 3212786
Conc: 10.18 ug/ml

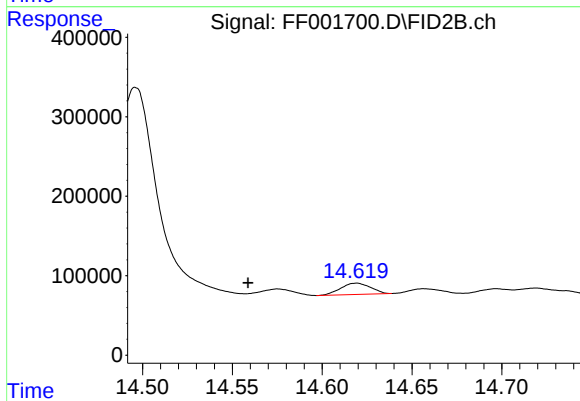


#10 N-TETRACOSANE

R.T.: 14.619 min
Delta R.T.: 0.060 min
Response: 164331
Conc: 0.52 ug/ml

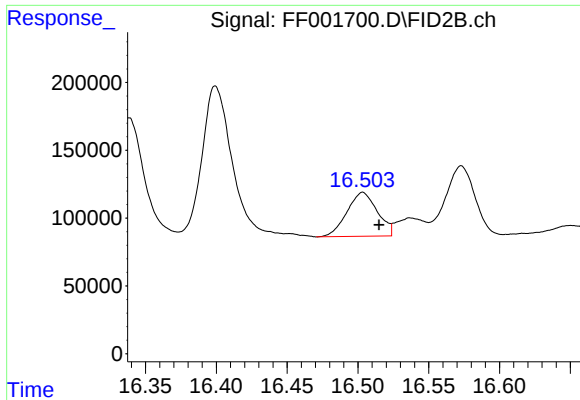


#11 N-OCTACOSANE

R.T.: 16.503 min
Delta R.T.: -0.012 min
Response: 483408
Conc: 1.50 ug/ml

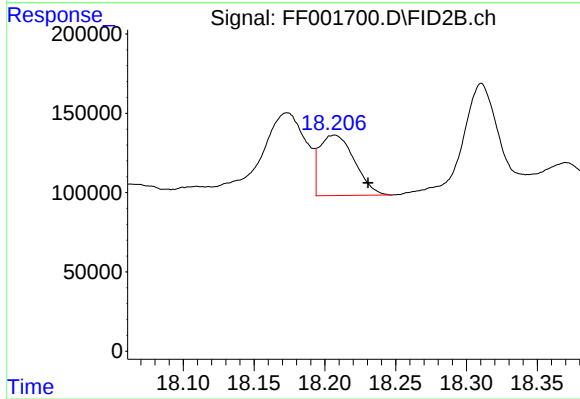


#12 N-DOTRIACONTANE

R.T.: 18.207 min
Delta R.T.: -0.024 min
Response: 653626
Conc: 2.00 ug/ml

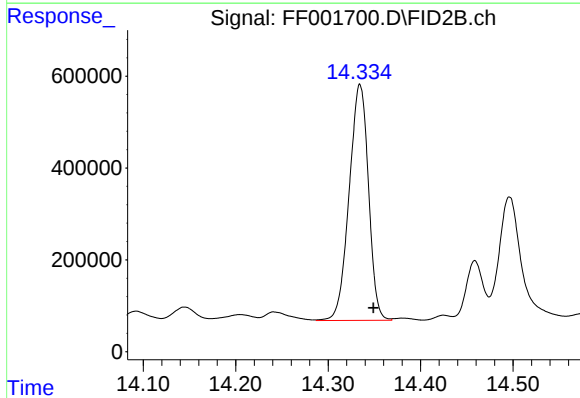

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.334 min
Delta R.T.: -0.015 min
Response: 7456850
Conc: 18.50 ug/ml

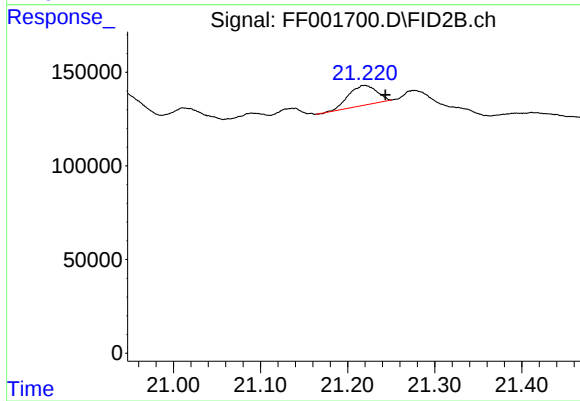

#15 N-TETRACONTANE

R.T.: 21.220 min
Delta R.T.: -0.023 min
Response: 238054
Conc: 0.99 ug/ml