

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
 Data File : FF001705.D
 Signal(s) : FID2B.ch
 Acq On : 07 Aug 2018 05:29
 Operator : AJ\SJ
 Sample : J4347-03 5X
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 07 10:24:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.329	939794	2.331 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.492	2184869	6.878 ug/ml
11)	N-OCTACOSANE	16.494	245277	0.762 ug/ml
12)	N-DOTRIACONTANE	18.212	620959	1.903 ug/ml
14)	N-HEXATRIACONTANE	19.737	338554	1.148 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080618\
Data File : FF001705.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2018 05:29
Operator : AJ\SJ
Sample : J4347-03 5X
Misc :
ALS Vial : 78 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 07 10:24:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

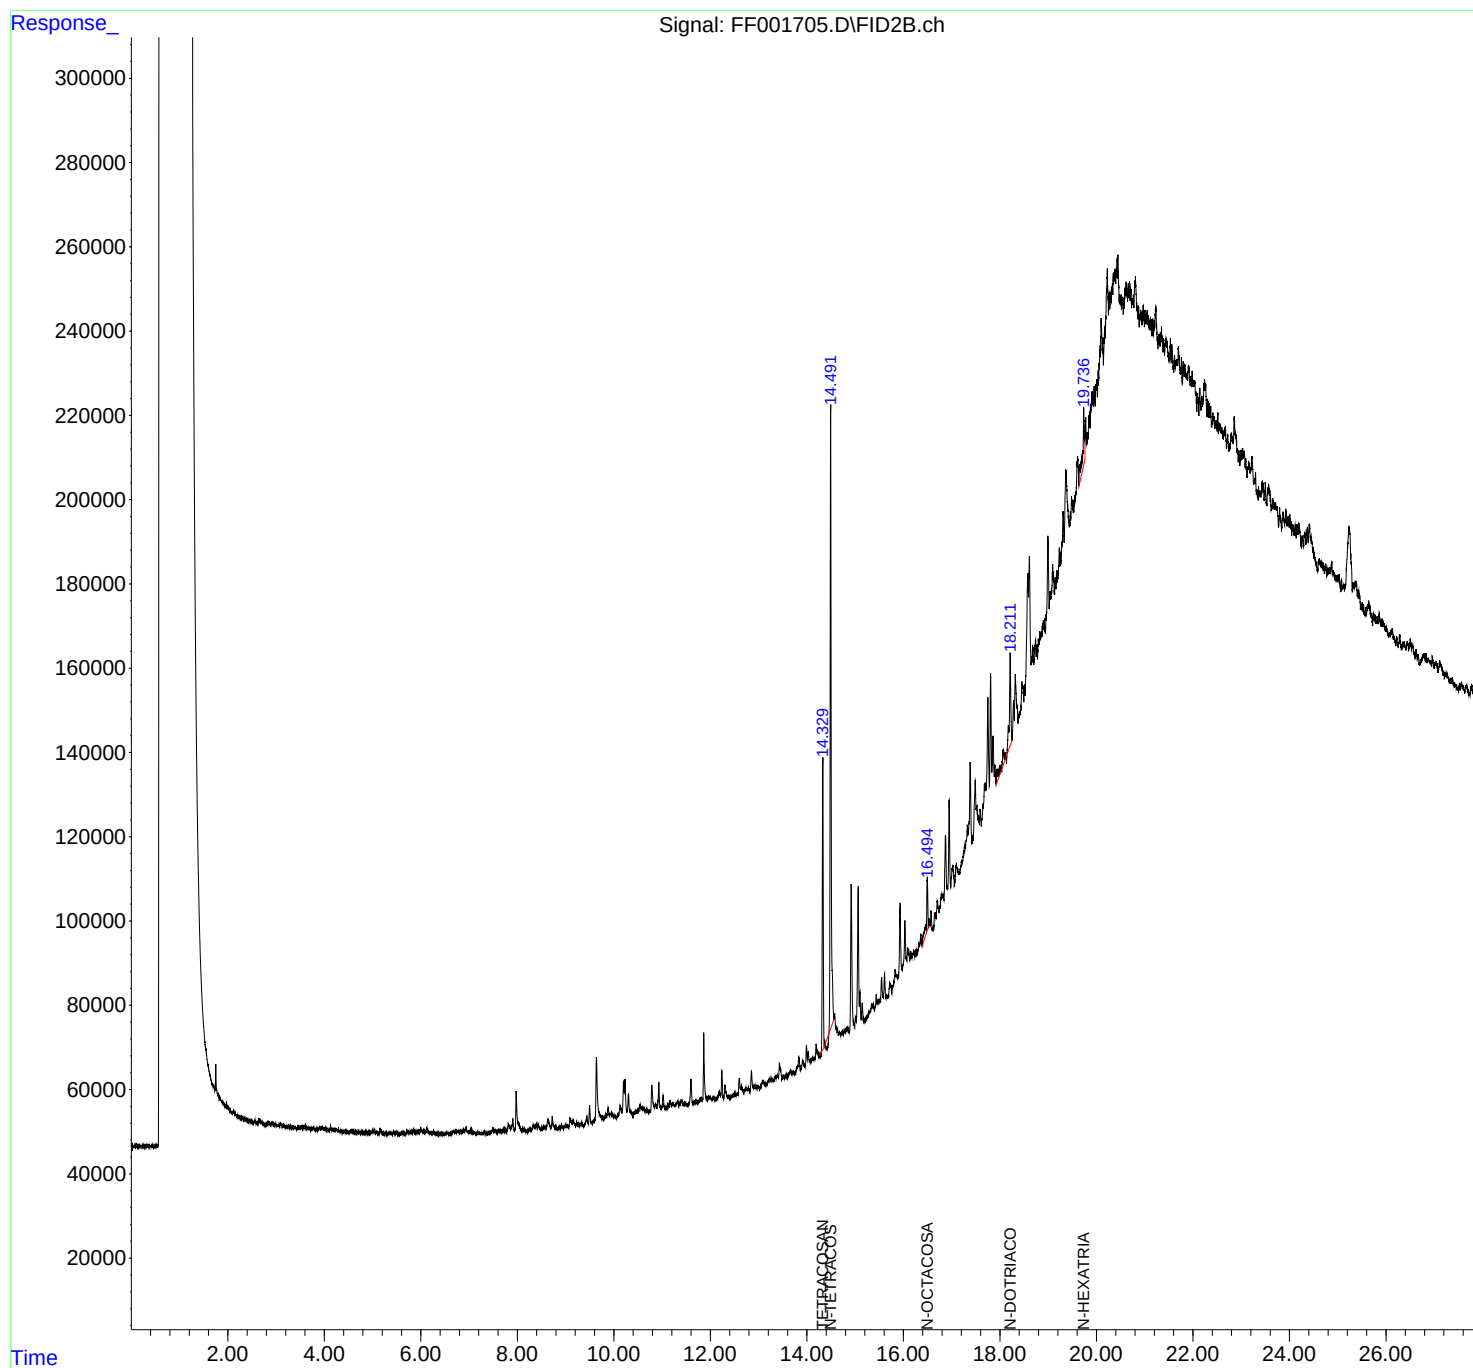

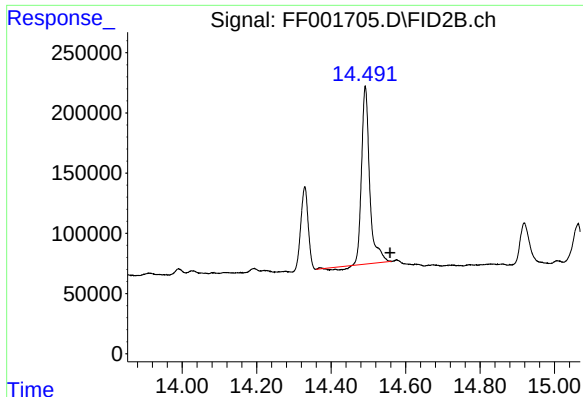


#10 N-TETRACOSANE

R.T.: 14.492 min
Delta R.T.: -0.067 min
Response: 2184869
Conc: 6.88 ug/ml

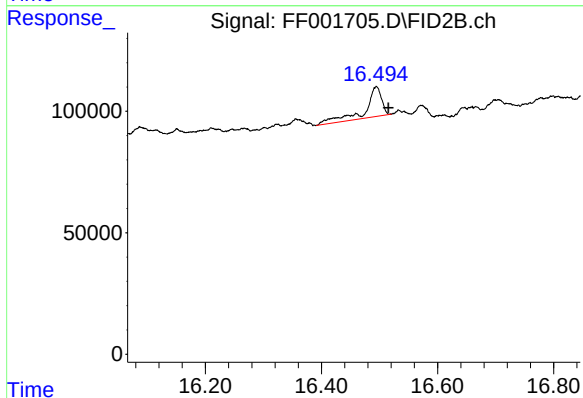


#11 N-OCTACOSANE

R.T.: 16.494 min
Delta R.T.: -0.021 min
Response: 245277
Conc: 0.76 ug/ml

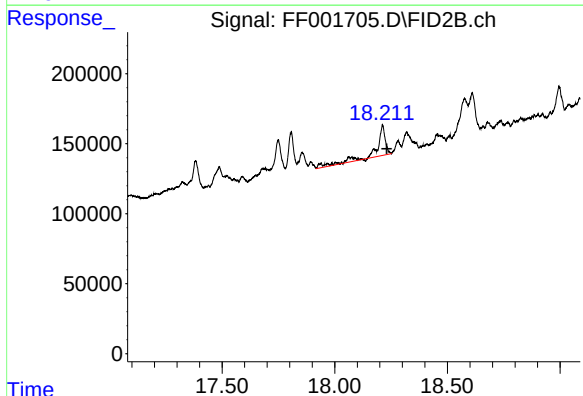


#12 N-DOTRIACONTANE

R.T.: 18.212 min
Delta R.T.: -0.018 min
Response: 620959
Conc: 1.90 ug/ml

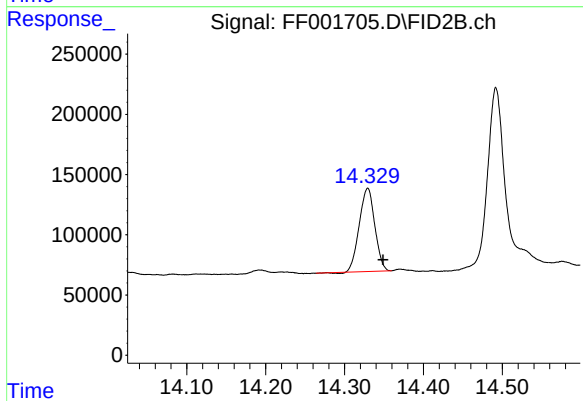

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.329 min
Delta R.T.: -0.020 min
Response: 939794
Conc: 2.33 ug/ml

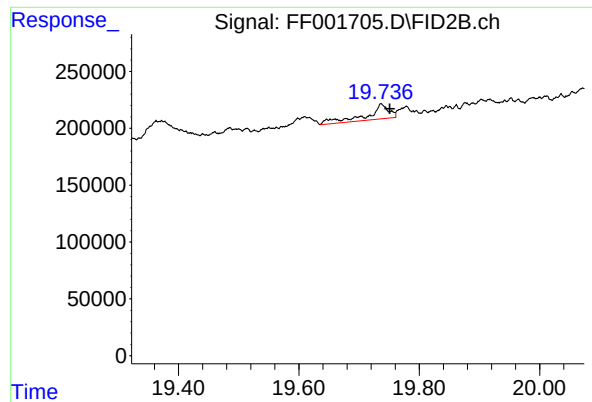

#14 N-HEXATRIACONTANE

R.T.: 19.737 min
Delta R.T.: -0.014 min
Response: 338554
Conc: 1.15 ug/ml