

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080620\
 Data File : FF007281.D
 Signal(s) : FID2B.ch
 Acq On : 06 Aug 2020 12:59
 Operator : DD\AJ
 Sample : L3553-02MS
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 06 13:49:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	2437787	17.859 ug/ml
Target Compounds			
2) N-DECANE	4.461	2330993	16.702 ug/ml
3) N-DODECANE	6.487	2461314	17.304 ug/ml
4) N-TETRADECANE	8.284	2532693	17.405 ug/ml
5) N-HEXADECANE	9.888	2603414	17.517 ug/ml
6) N-OCTADECANE	11.331	2512509	16.385 ug/mlm
7) N-EICOSANE	12.645	2739916	17.702 ug/ml
8) N-DOCOSANE	13.847	2627276	16.831 ug/ml
10) N-TETRACOSANE	14.951	3980857	25.205 ug/mlm
11) N-HEXACOSANE	15.979	2406880	15.352 ug/ml
12) N-OCTACOSANE	16.933	2944605	18.762 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080620\
Data File : FF007281.D
Signal(s) : FID2B.ch
Acq On : 06 Aug 2020 12:59
Operator : DD\AJ
Sample : L3553-02MS
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 06 13:49:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

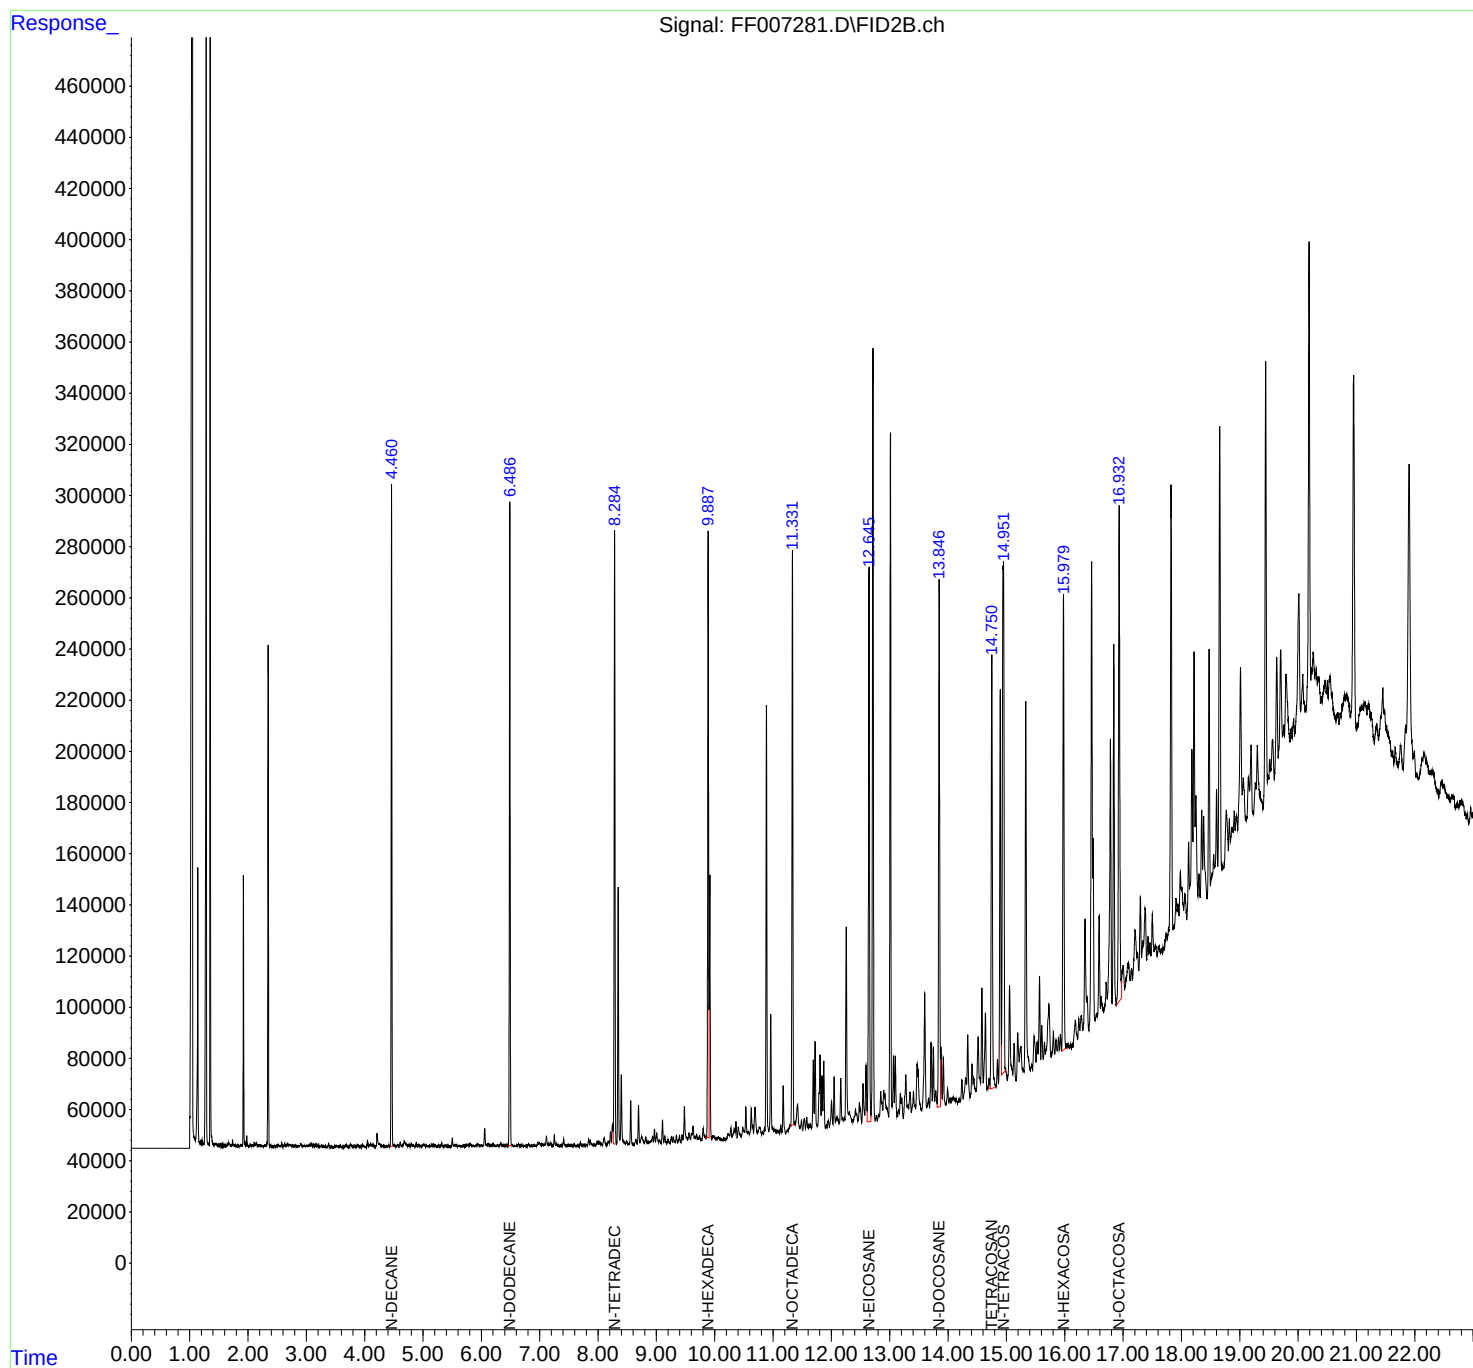

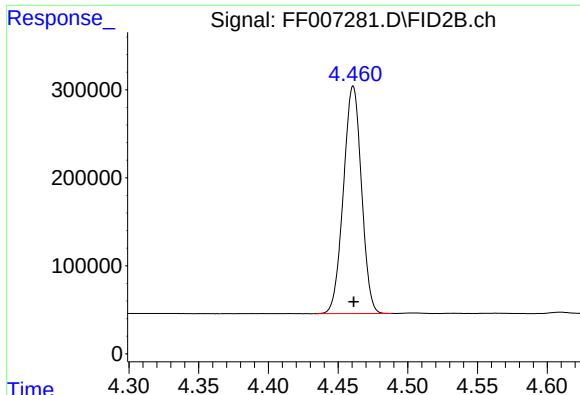


#2 N-DECANE

R.T.: 4.461 min
Delta R.T.: 0.000 min
Response: 2330993
Conc: 16.70 ug/ml

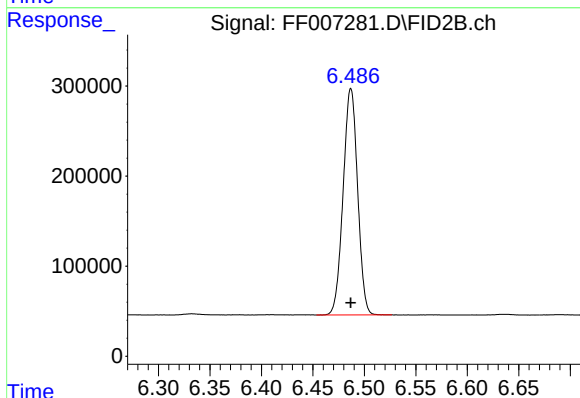


#3 N-DODECANE

R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 2461314
Conc: 17.30 ug/ml

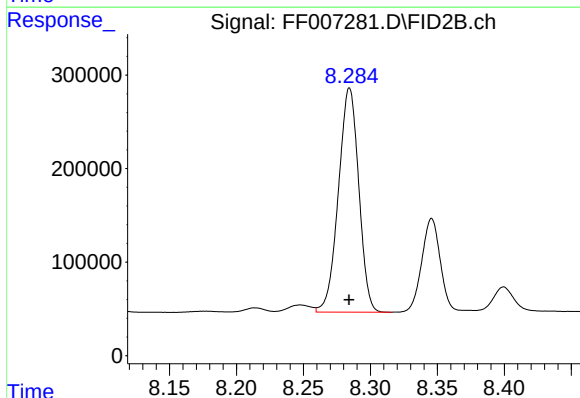


#4 N-TETRADECANE

R.T.: 8.284 min
Delta R.T.: 0.000 min
Response: 2532693
Conc: 17.40 ug/ml

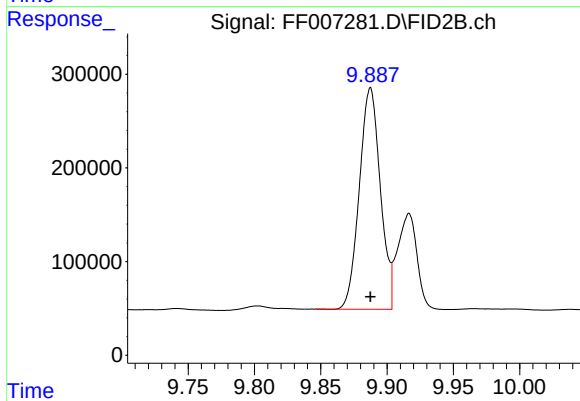


#5 N-HEXADECANE

R.T.: 9.888 min
Delta R.T.: 0.000 min
Response: 2603414
Conc: 17.52 ug/ml

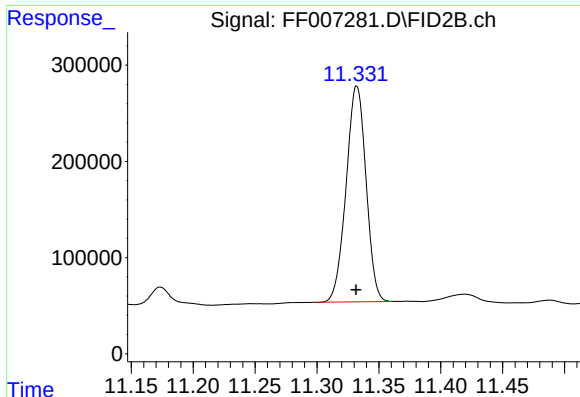


#6 N-OCTADECANE

R.T.: 11.331 min
Delta R.T.: 0.000 min
Response: 2512509
Conc: 16.39 ug/ml m

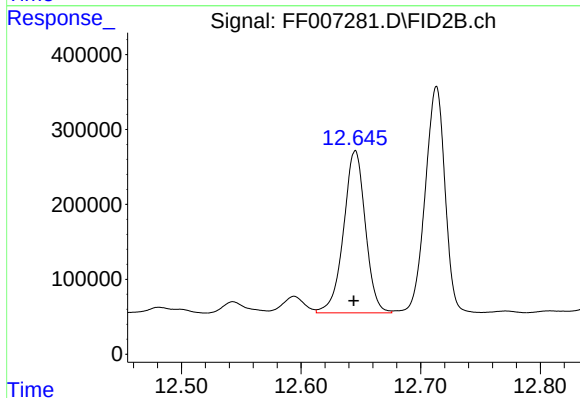


#7 N-EICOSANE

R.T.: 12.645 min
Delta R.T.: 0.001 min
Response: 2739916
Conc: 17.70 ug/ml

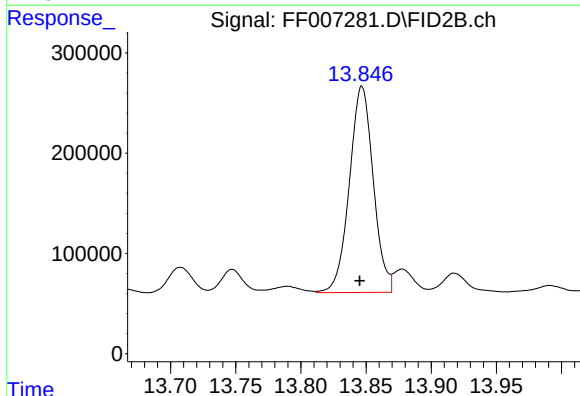


#8 N-DOCOSANE

R.T.: 13.847 min
Delta R.T.: 0.002 min
Response: 2627276
Conc: 16.83 ug/ml

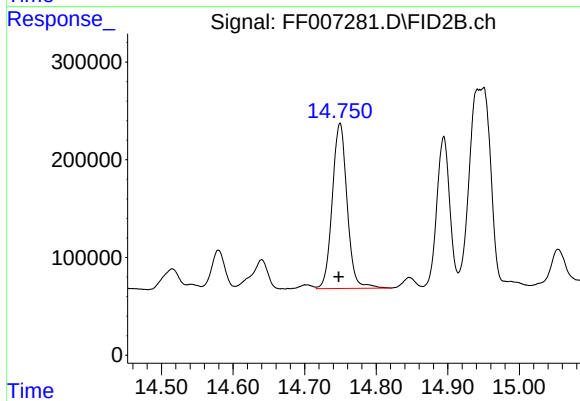


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: 0.002 min
Response: 2437787
Conc: 17.86 ug/ml

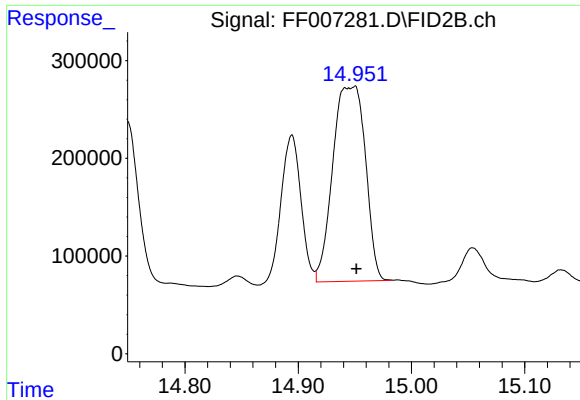


#10 N-TETRACOSANE

R.T.: 14.951 min
Delta R.T.: 0.000 min
Response: 3980857
Conc: 25.20 ug/ml m

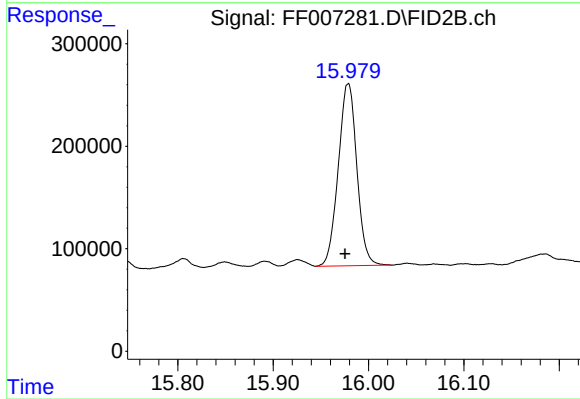

#11 N-HEXACOSANE

R.T.: 15.979 min
Delta R.T.: 0.003 min
Response: 2406880
Conc: 15.35 ug/ml

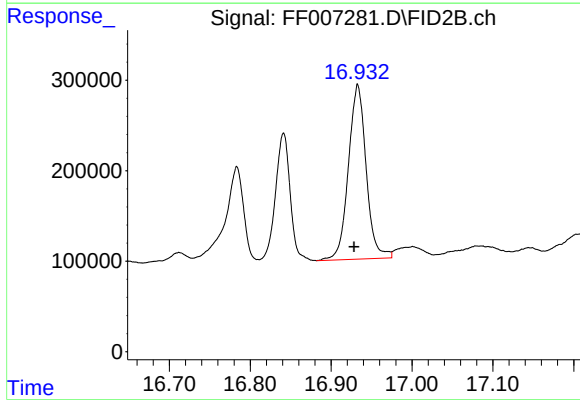

#12 N-OCTACOSANE

R.T.: 16.933 min
Delta R.T.: 0.005 min
Response: 2944605
Conc: 18.76 ug/ml