

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080720\
Data File : FF007286.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2020 09:59
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 08 00:04:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.748	2434264	17.833 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.817	123611	0.788 ug/ml
14)	N-DOTRIACONTANE	18.653	148523	1.002 ug/ml
15)	N-TETRATRIACONTANE	19.442	109475	0.905 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080720\
Data File : FF007286.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2020 09:59
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 08 00:04:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rx1-1ms
Signal Info : 20mx0.18mmx0.18um

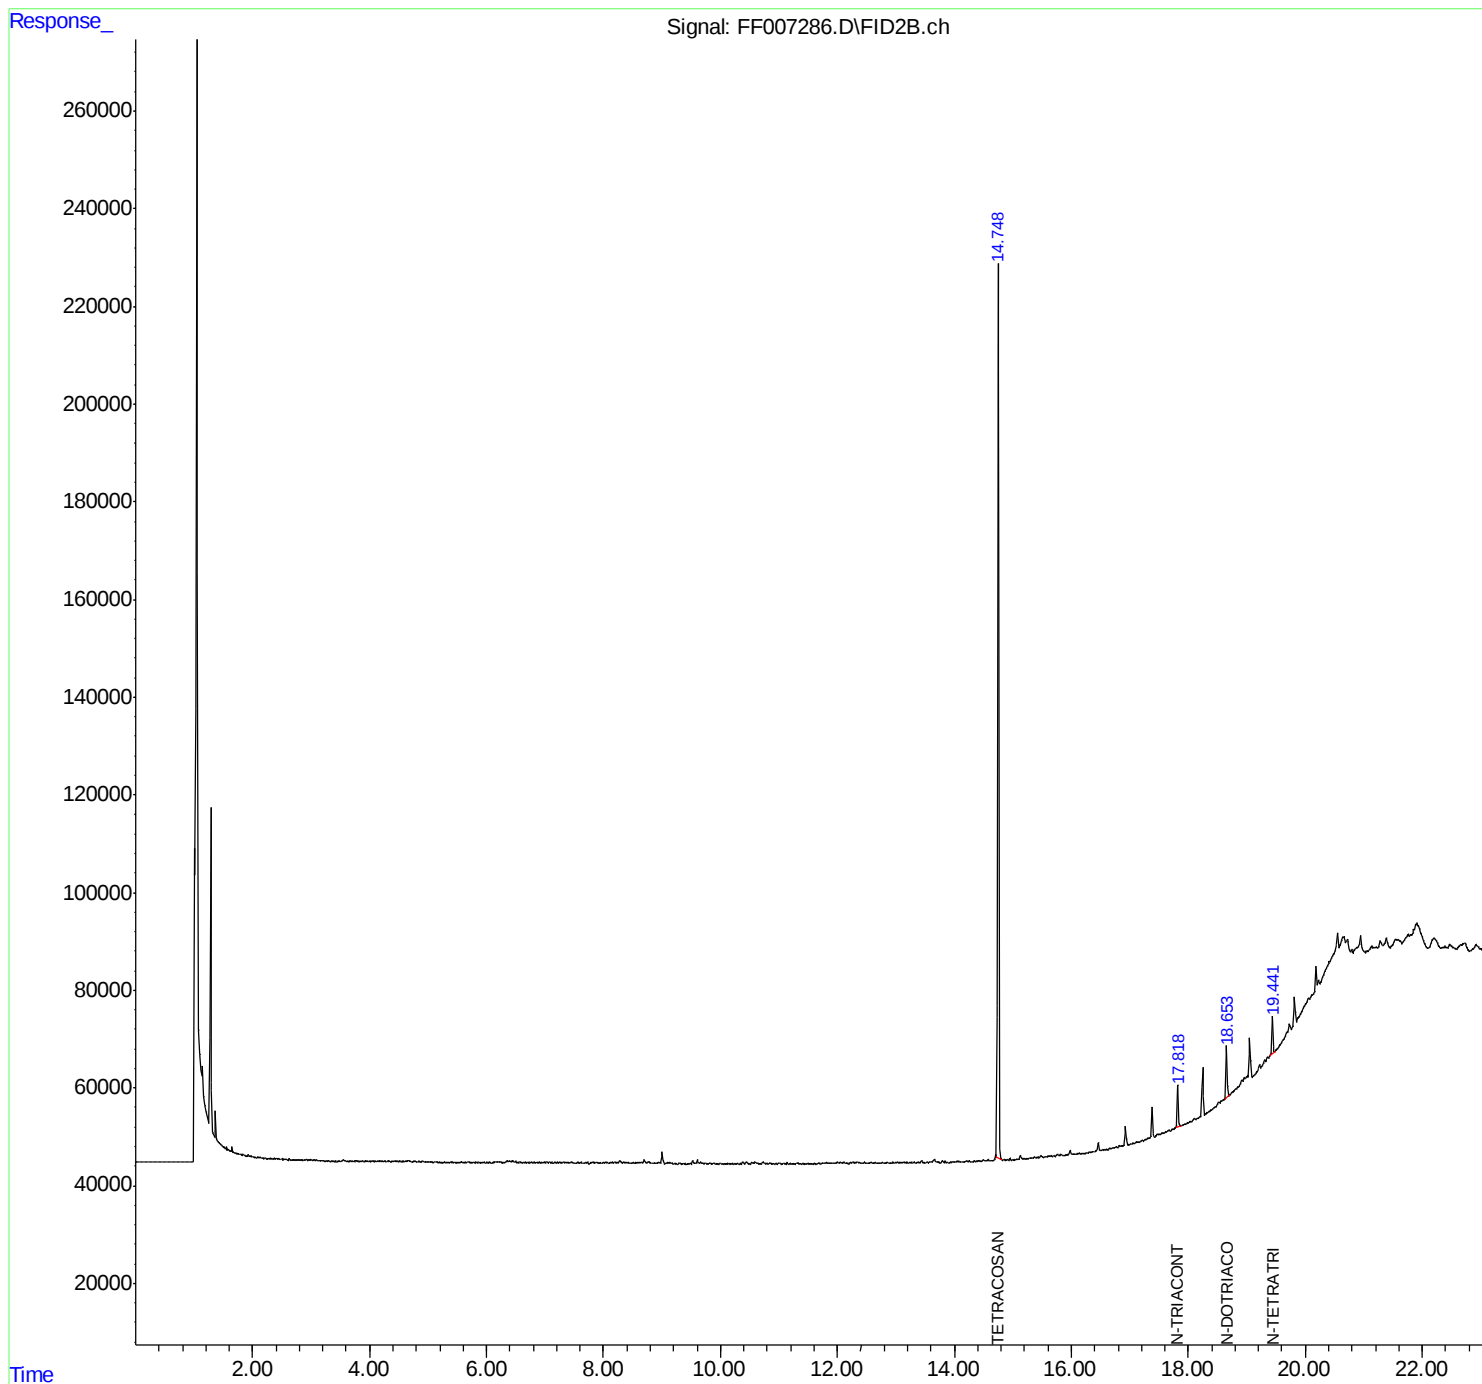


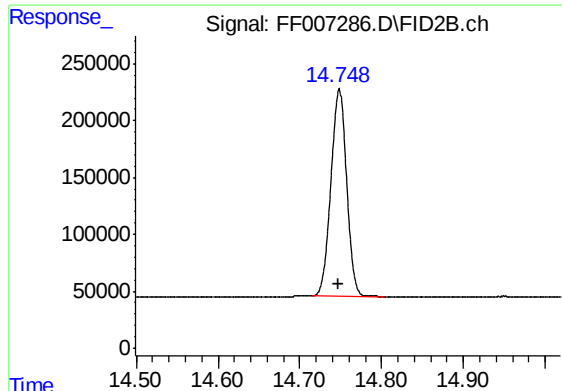

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.748 min
Delta R.T.: 0.000 min
Response: 2434264
Conc: 17.83 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

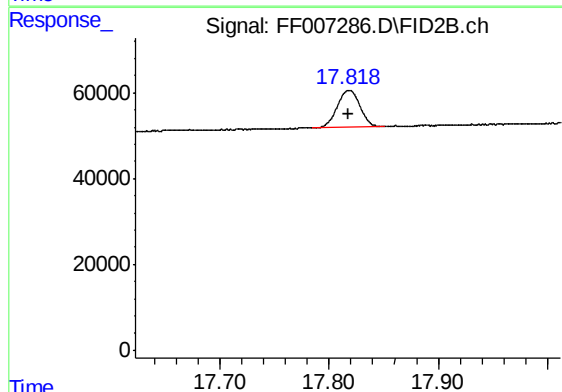


#13 N-TRIACONTANE

R.T.: 17.817 min
Delta R.T.: 0.000 min
Response: 123611
Conc: 0.79 ug/ml

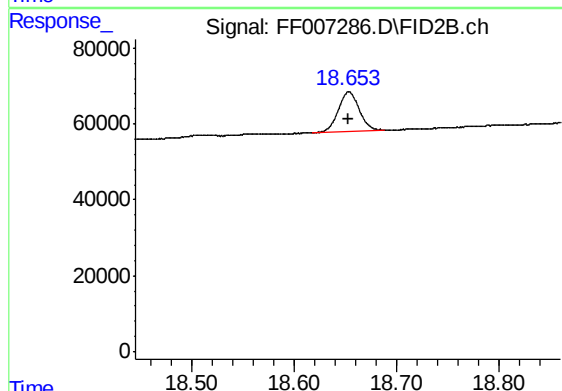

#14 N-DOTRIACONTANE

R.T.: 18.653 min
Delta R.T.: 0.000 min
Response: 148523
Conc: 1.00 ug/ml

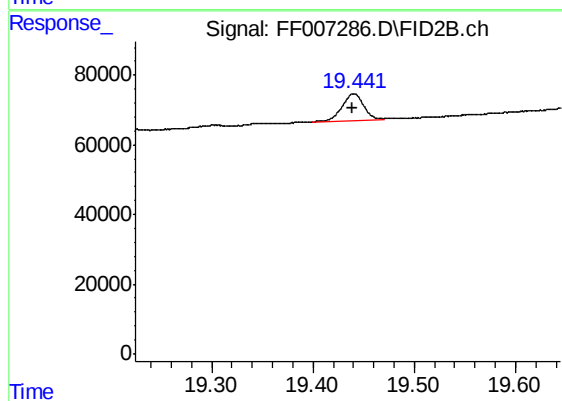

#15 N-TETRATRIACONTANE

R.T.: 19.442 min
Delta R.T.: 0.003 min
Response: 109475
Conc: 0.91 ug/ml