

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080720\
Data File : FF007288.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2020 11:01
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Aug 08 00:05:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.487	3152207	22.161 ug/ml
12)	N-OCTACOSANE	16.929	2967410	18.907 ug/ml
13)	N-TRIACONTANE	17.817	100381	0.640 ug/ml
14)	N-DOTRIACONTANE	18.652	113750	0.768 ug/ml
15)	N-TETRATRIACONTANE	19.439	87871	0.727 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080720\
Data File : FF007288.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2020 11:01
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Aug 08 00:05:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

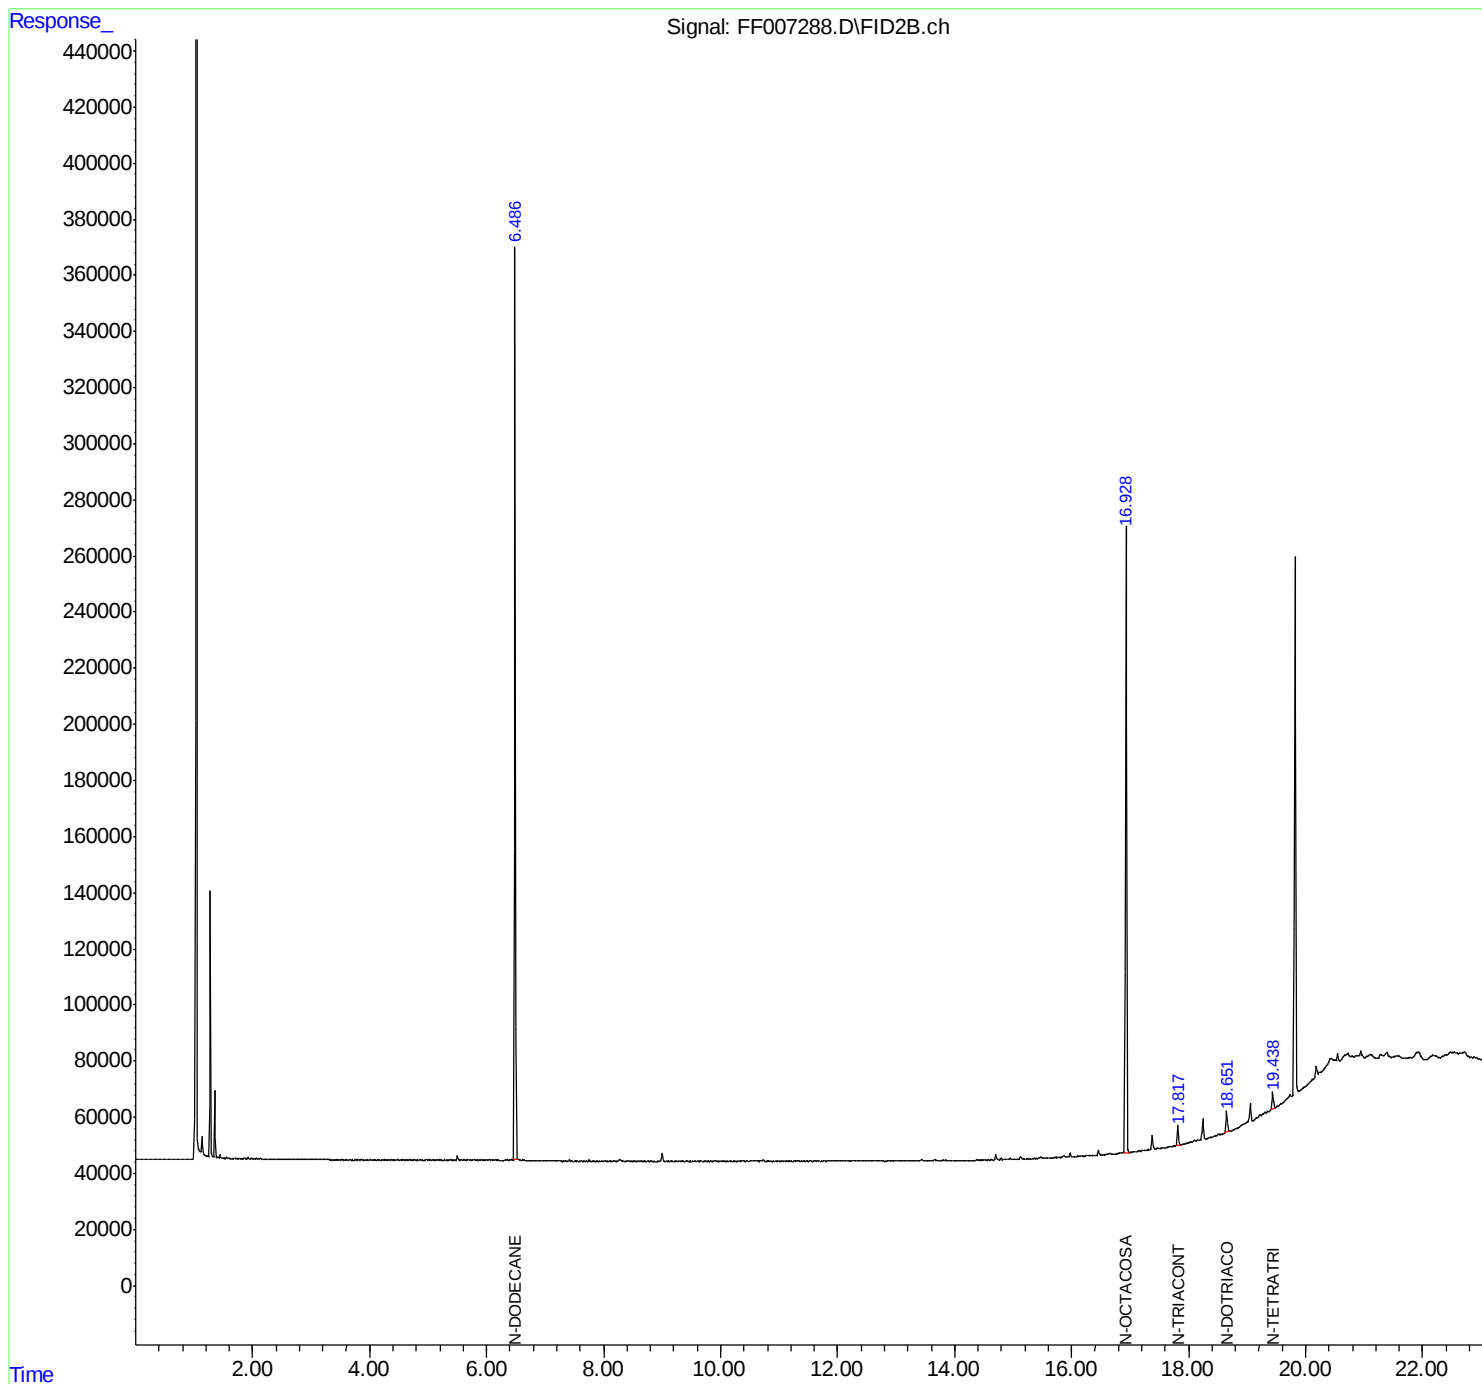


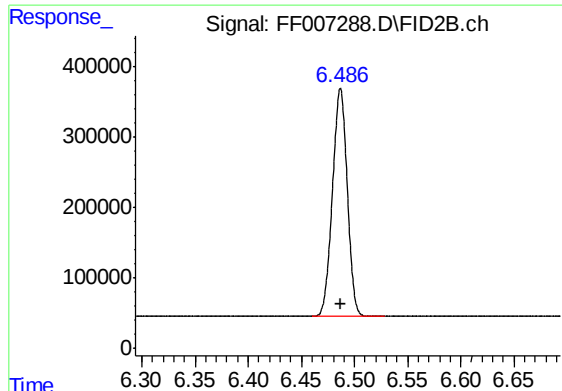

#3 N-DODECANE


R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 3152207
Conc: 22.16 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

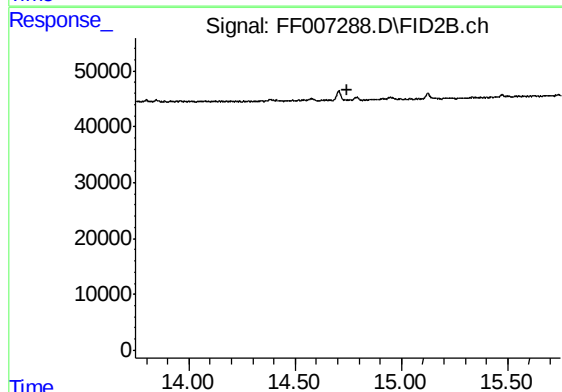


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.748 min
Response: 0
Conc: N.D.

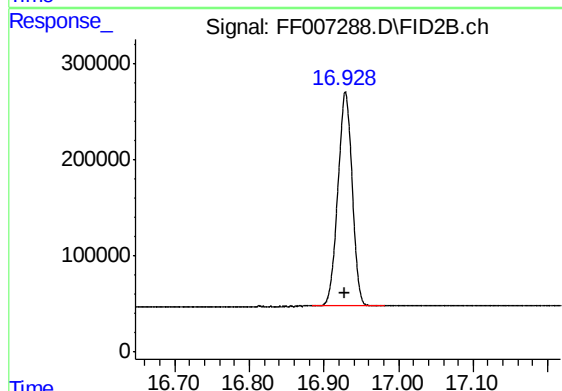


#12 N-OCTACOSANE

R.T.: 16.929 min
Delta R.T.: 0.000 min
Response: 2967410
Conc: 18.91 ug/ml

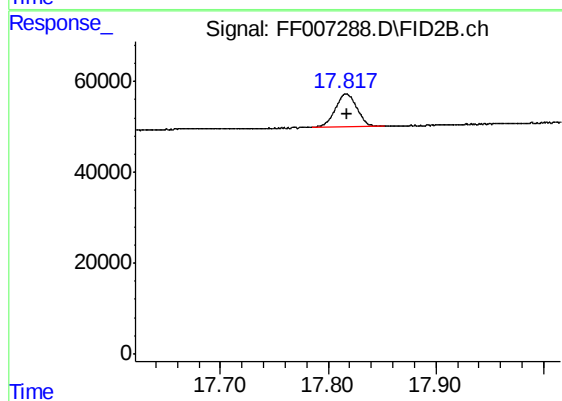

#13 N-TRIACONTANE


R.T.: 17.817 min
Delta R.T.: -0.001 min
Response: 100381
Conc: 0.64 ug/ml

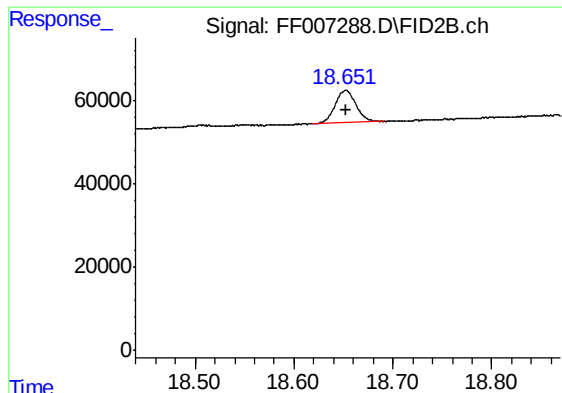

#14 N-DOTRIACONTANE

R.T.: 18.652 min
Delta R.T.: 0.000 min
Response: 113750
Conc: 0.77 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

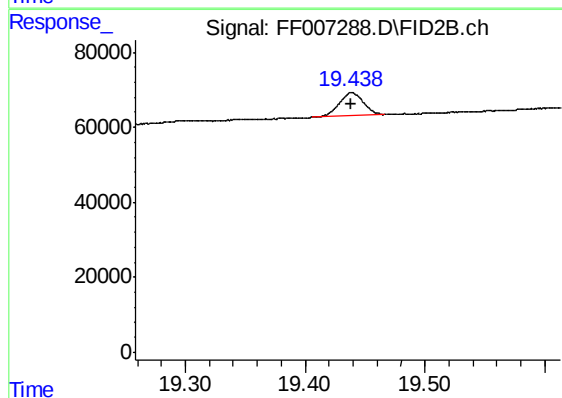

#15 N-TETRATRIACONTANE

R.T.: 19.439 min
Delta R.T.: 0.000 min
Response: 87871
Conc: 0.73 ug/ml