

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080720\
 Data File : FF007291.D
 Signal(s) : FID2B.ch
 Acq On : 07 Aug 2020 12:50
 Operator : DD\AJ
 Sample : L3592-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WASTE

Integration File: autoint1.e
 Quant Time: Aug 08 00:06:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.748	2277146	16.682 ug/ml
Target Compounds			
4) N-TETRADECANE	8.250	394061	2.708 ug/ml
10) N-TETRACOSANE	14.918	141782	0.898 ug/ml
11) N-HEXACOSANE	15.975	104015	0.663 ug/ml
12) N-OCTACOSANE	16.927	146523	0.934 ug/ml
13) N-TRIACONTANE	17.817	160168	1.021 ug/ml
14) N-DOTRIACONTANE	18.649	215475	1.454 ug/ml
16) N-HEXATRIACONTANE	20.224	190423	2.059 ug/ml
18) N-TETRACONTANE	21.937	355035	5.308 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080720\
Data File : FF07291.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2020 12:50
Operator : DD\AJ
Sample : L3592-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WASTE

Integration File: autoint1.e
Quant Time: Aug 08 00:06:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

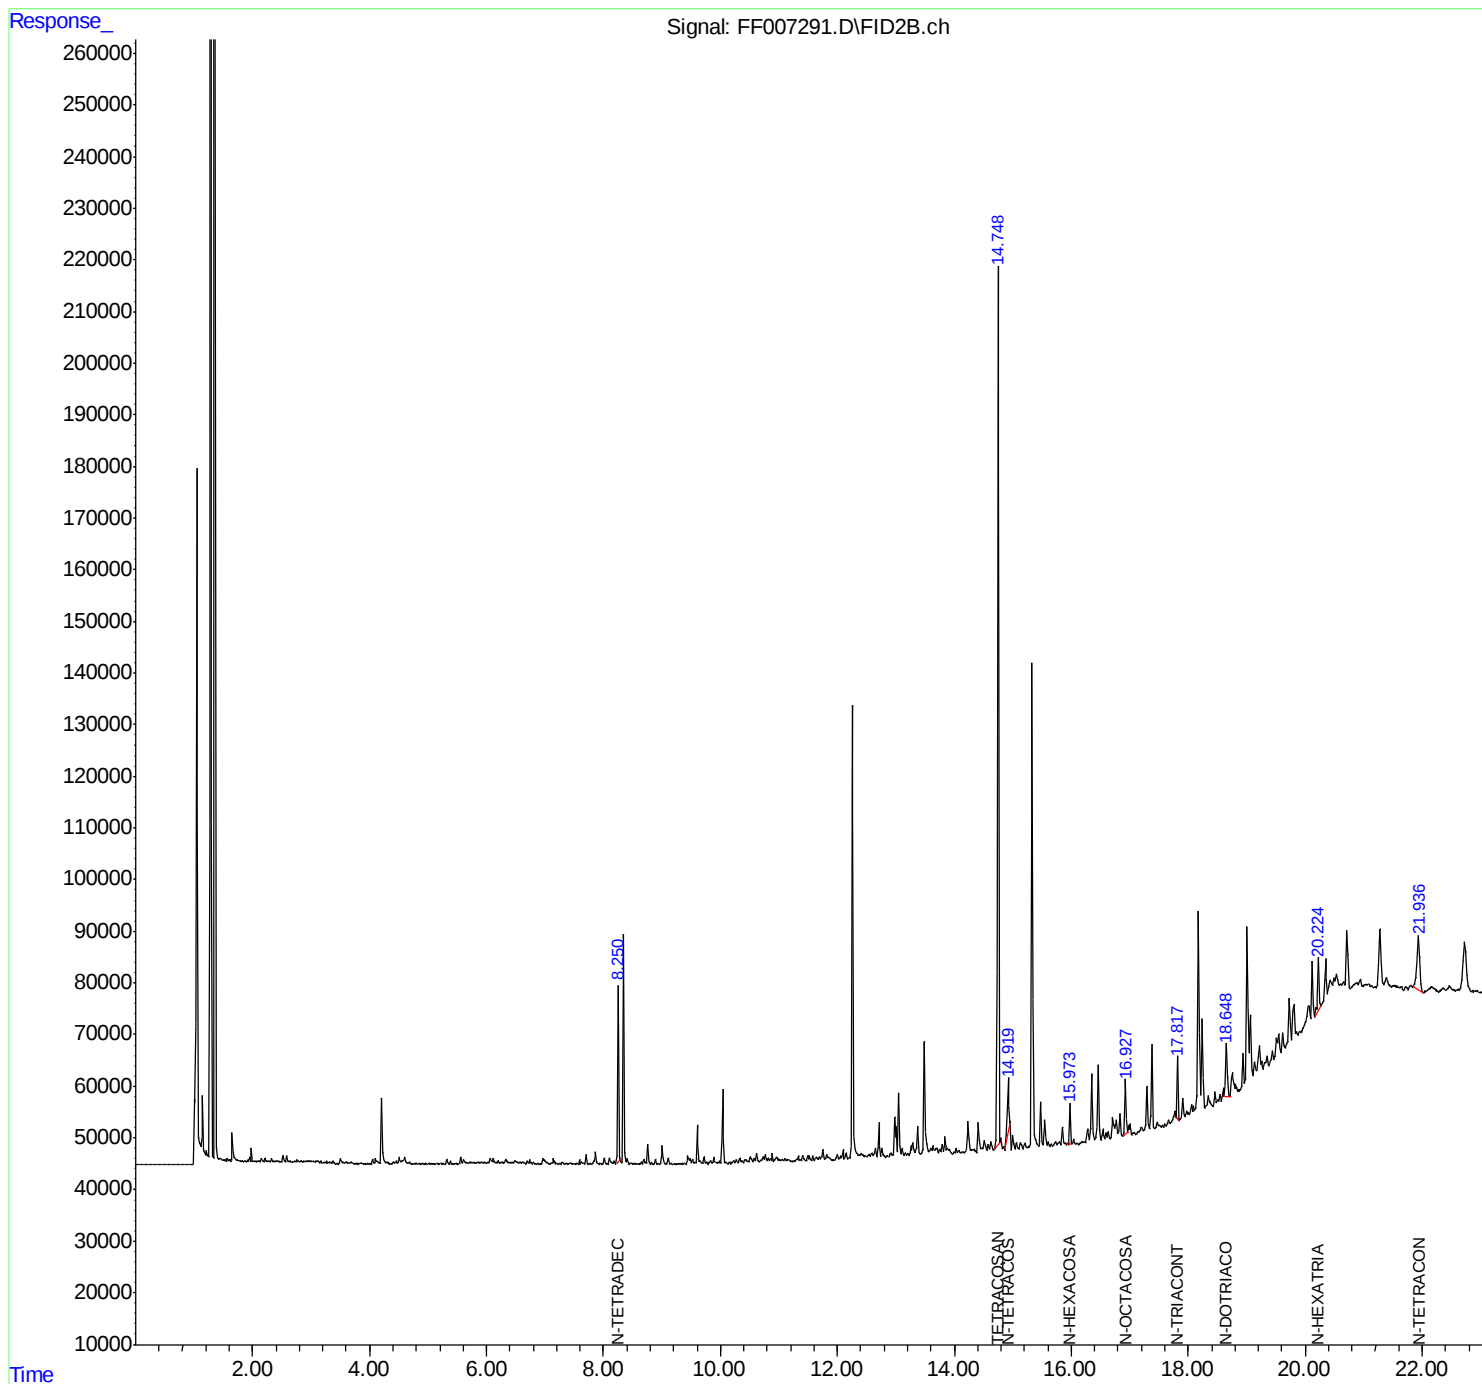


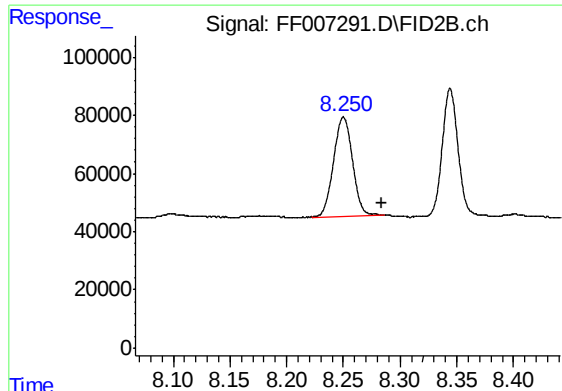

#4 N-TETRADECANE


R.T.: 8.250 min
Delta R.T.: -0.034 min
Response: 394061
Conc: 2.71 ug/ml

Instrument :
FID_F
ClientSampleId :
WASTE

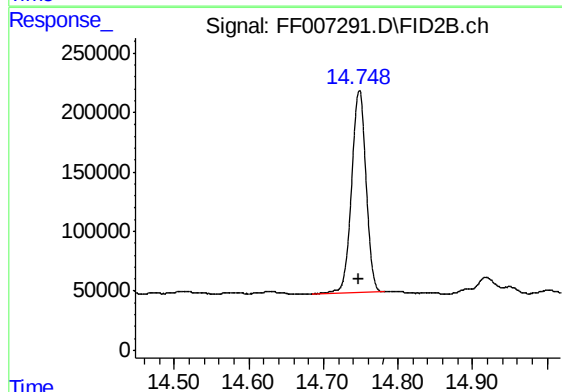


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.748 min
Delta R.T.: 0.000 min
Response: 2277146
Conc: 16.68 ug/ml

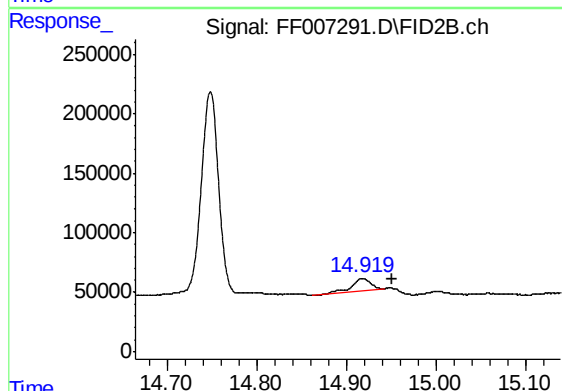


#10 N-TETRACOSANE

R.T.: 14.918 min
Delta R.T.: -0.033 min
Response: 141782
Conc: 0.90 ug/ml

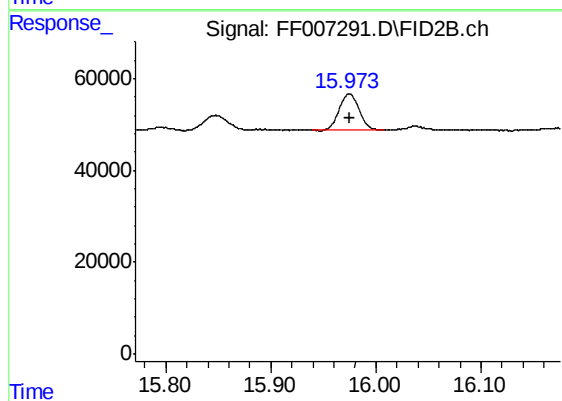

#11 N-HEXACOSANE


R.T.: 15.975 min
Delta R.T.: 0.000 min
Response: 104015
Conc: 0.66 ug/ml

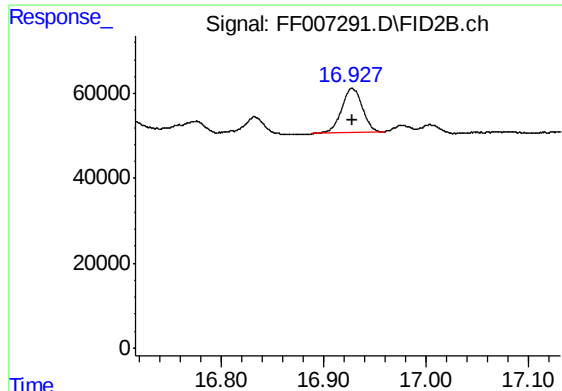

#12 N-OCTACOSANE


R.T.: 16.927 min
Delta R.T.: -0.001 min
Response: 146523
Conc: 0.93 ug/ml

Instrument :
FID_F
ClientSampleId :
WASTE

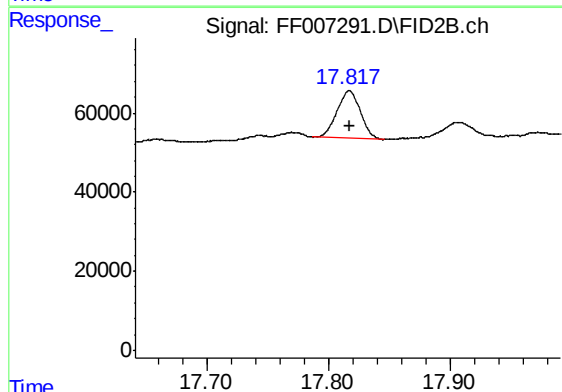


#13 N-TRIACONTANE

R.T.: 17.817 min
Delta R.T.: 0.000 min
Response: 160168
Conc: 1.02 ug/ml

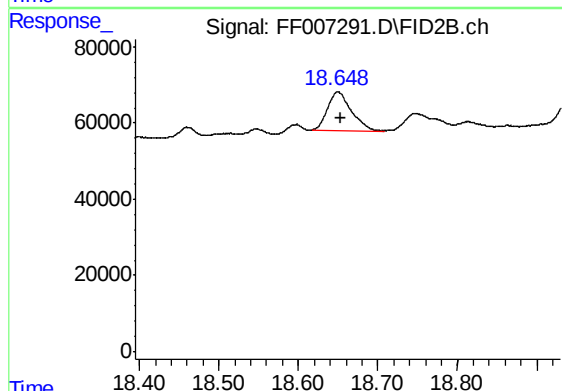


#14 N-DOTRIACONTANE

R.T.: 18.649 min
Delta R.T.: -0.004 min
Response: 215475
Conc: 1.45 ug/ml

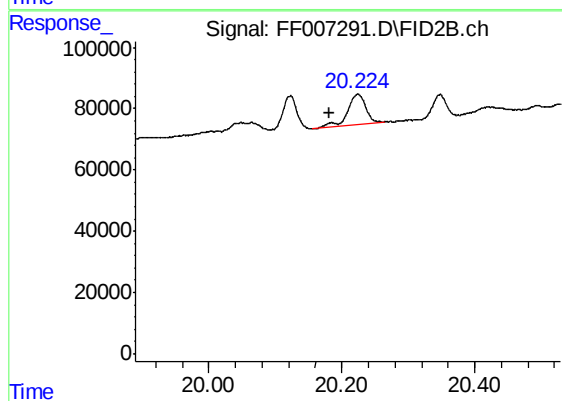

#16 N-HEXATRIACONTANE

R.T.: 20.224 min
Delta R.T.: 0.044 min
Response: 190423
Conc: 2.06 ug/ml

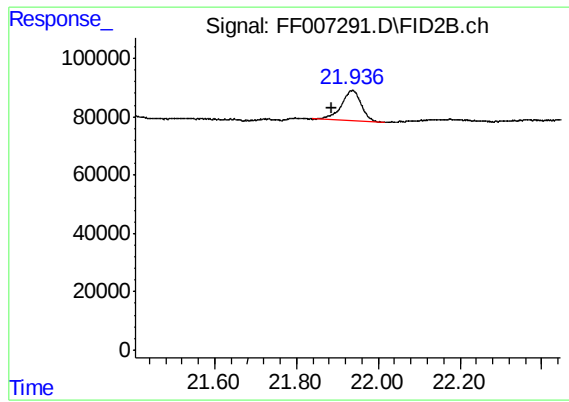

#18 N-TETRACONTANE

R.T.: 21.937 min
Delta R.T.: 0.050 min
Response: 355035
Conc: 5.31 ug/ml

Instrument :
FID_F
ClientSampleId :
WASTE