

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080720\
Data File : FF007298.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2020 16:27
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Aug 08 00:11:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.486	3177720	22.341 ug/ml
12) N-OCTACOSANE	16.928	2975241	18.957 ug/ml
13) N-TRIACONTANE	17.815	147094	0.938 ug/ml
14) N-DOTRIACONTANE	18.651	170986	1.154 ug/ml
15) N-TETRATRIACONTANE	19.438	131293	1.086 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080720\
Data File : FF007298.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2020 16:27
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Aug 08 00:11:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

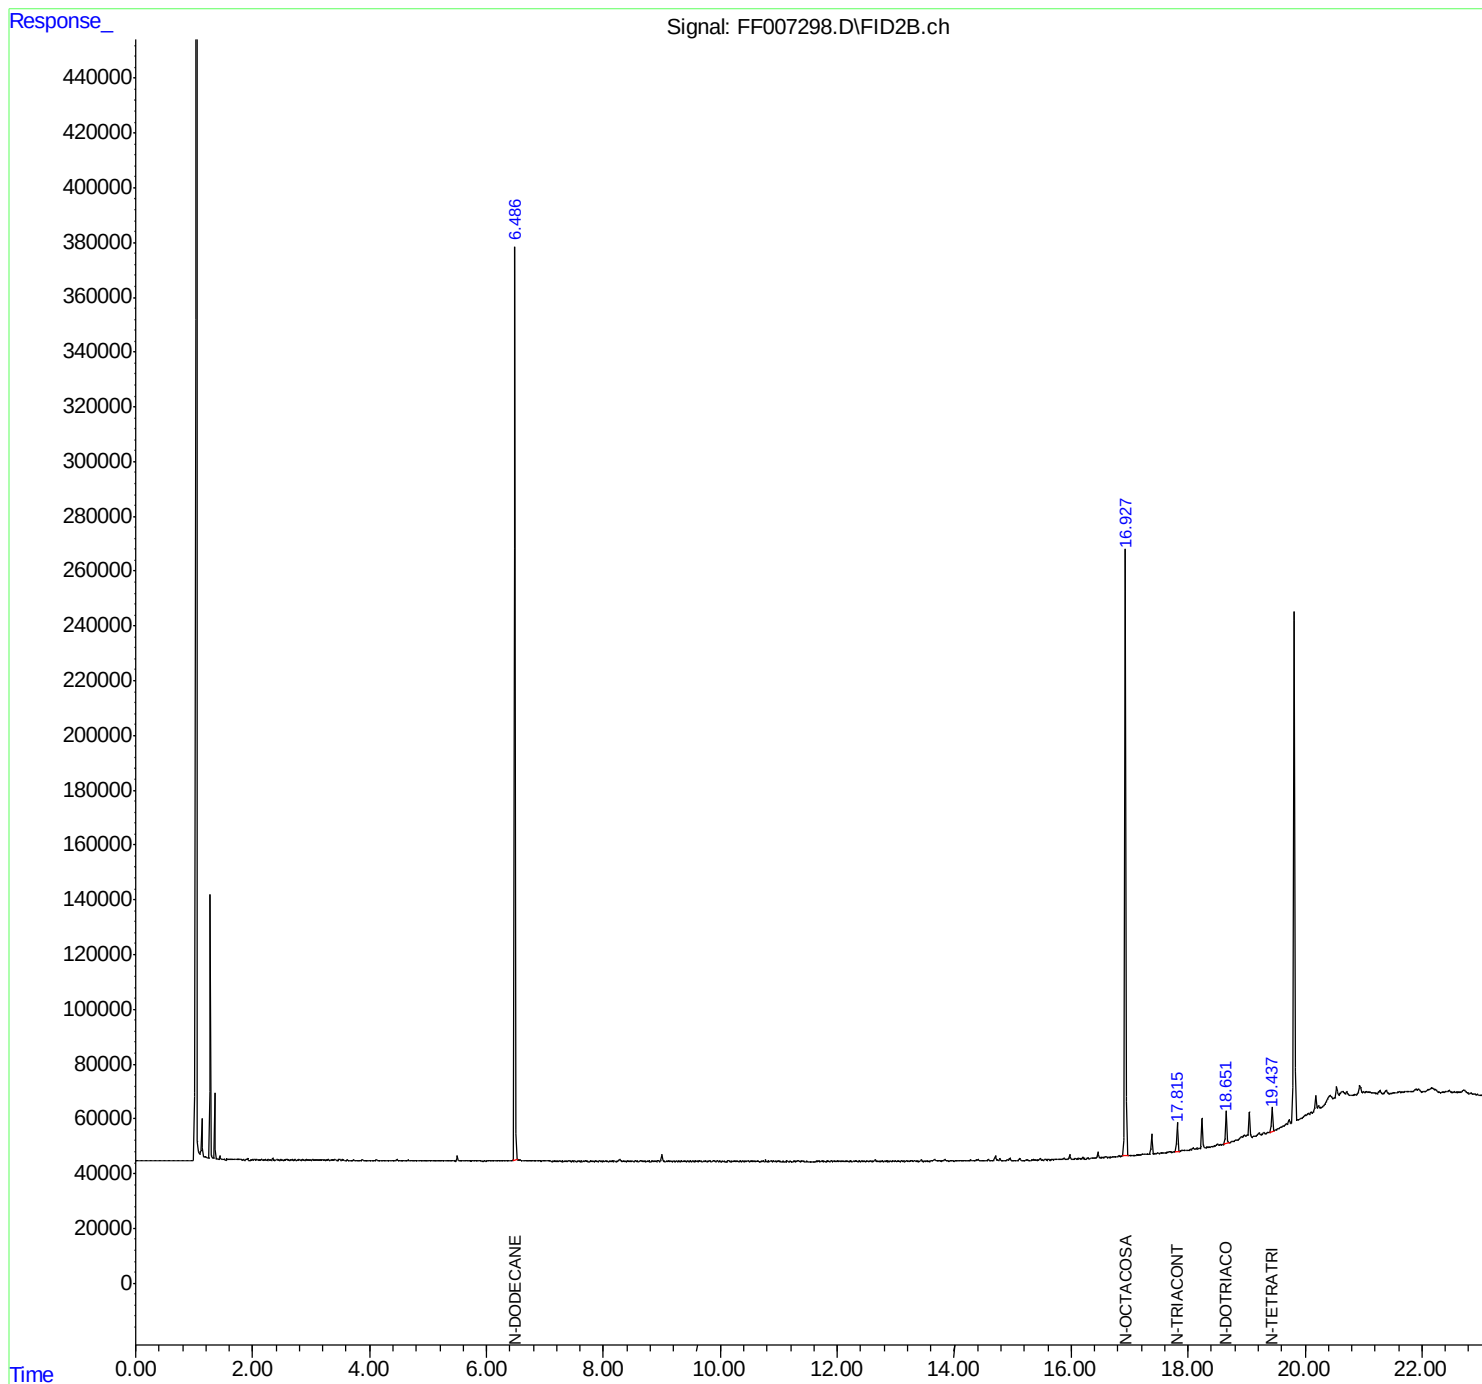


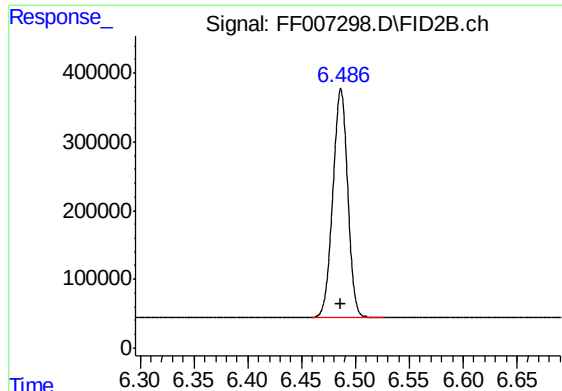

#3 N-DODECANE


R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 3177720
Conc: 22.34 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

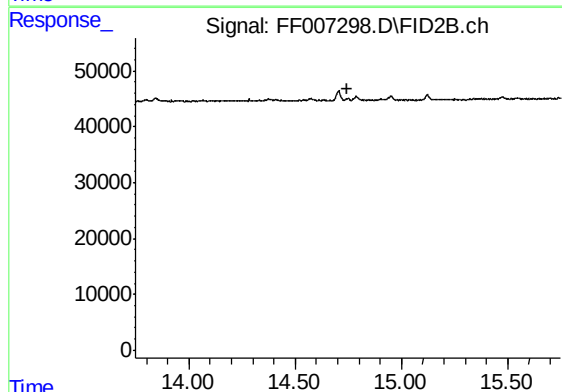


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.748 min
Response: 0
Conc: N.D.

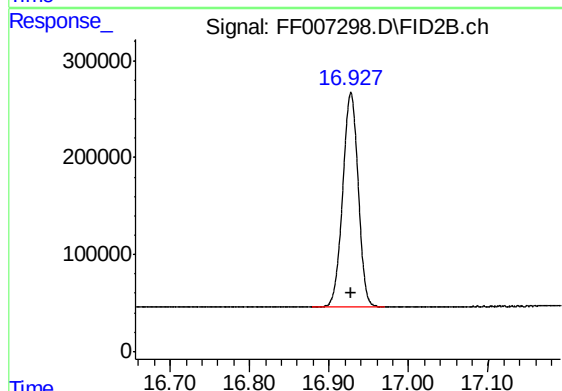


#12 N-OCTACOSANE

R.T.: 16.928 min
Delta R.T.: 0.000 min
Response: 2975241
Conc: 18.96 ug/ml

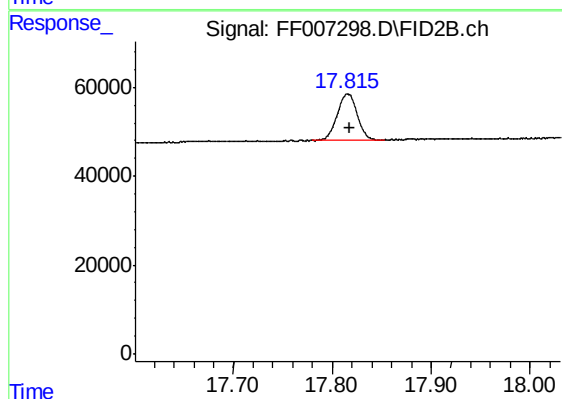

#13 N-TRIACONTANE


R.T.: 17.815 min
Delta R.T.: -0.003 min
Response: 147094
Conc: 0.94 ug/ml

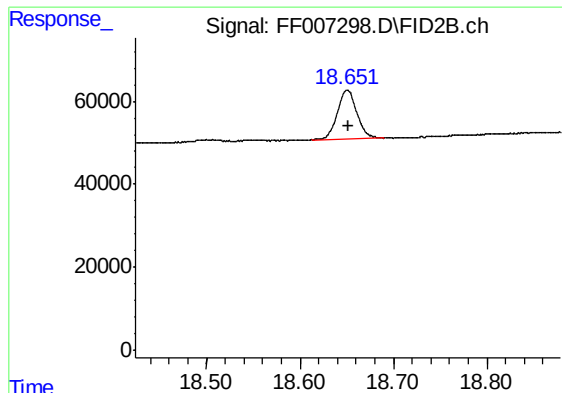

#14 N-DOTRIACONTANE

R.T.: 18.651 min
Delta R.T.: -0.001 min
Response: 170986
Conc: 1.15 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

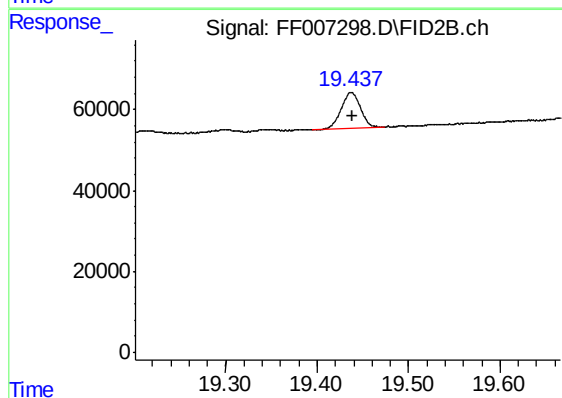

#15 N-TETRATRIACONTANE

R.T.: 19.438 min
Delta R.T.: -0.001 min
Response: 131293
Conc: 1.09 ug/ml