

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080720\
 Data File : FF007305.D
 Signal(s) : FID2B.ch
 Acq On : 07 Aug 2020 20:04
 Operator : DD\AJ
 Sample : L3508-01 20X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 TR-04-080620

Integration File: autoint1.e
 Quant Time: Aug 08 00:12:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
 Quant Title :
 QLast Update : Wed Jul 29 09:33:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.754	81422	0.596 ug/ml
Target Compounds			
8) N-DOCOSANE	13.896f	165141	1.058 ug/ml
10) N-TETRACOSANE	14.947	356325	2.256 ug/ml
13) N-TRIACONTANE	17.831	126132	0.804 ug/ml
14) N-DOTRIACONTANE	18.667	892033	6.021 ug/ml
15) N-TETRATRIACONTANE	19.454	847048	7.004 ug/ml
16) N-HEXATRIACONTANE	20.211	2601809	28.129 ug/ml
18) N-TETRACONTANE	21.868	104030	1.555 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080720\
Data File : FF007305.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2020 20:04
Operator : DD\AJ
Sample : L3508-01 20X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TR-04-080620

Integration File: autoint1.e
Quant Time: Aug 08 00:12:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072820.M
Quant Title :
QLast Update : Wed Jul 29 09:33:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

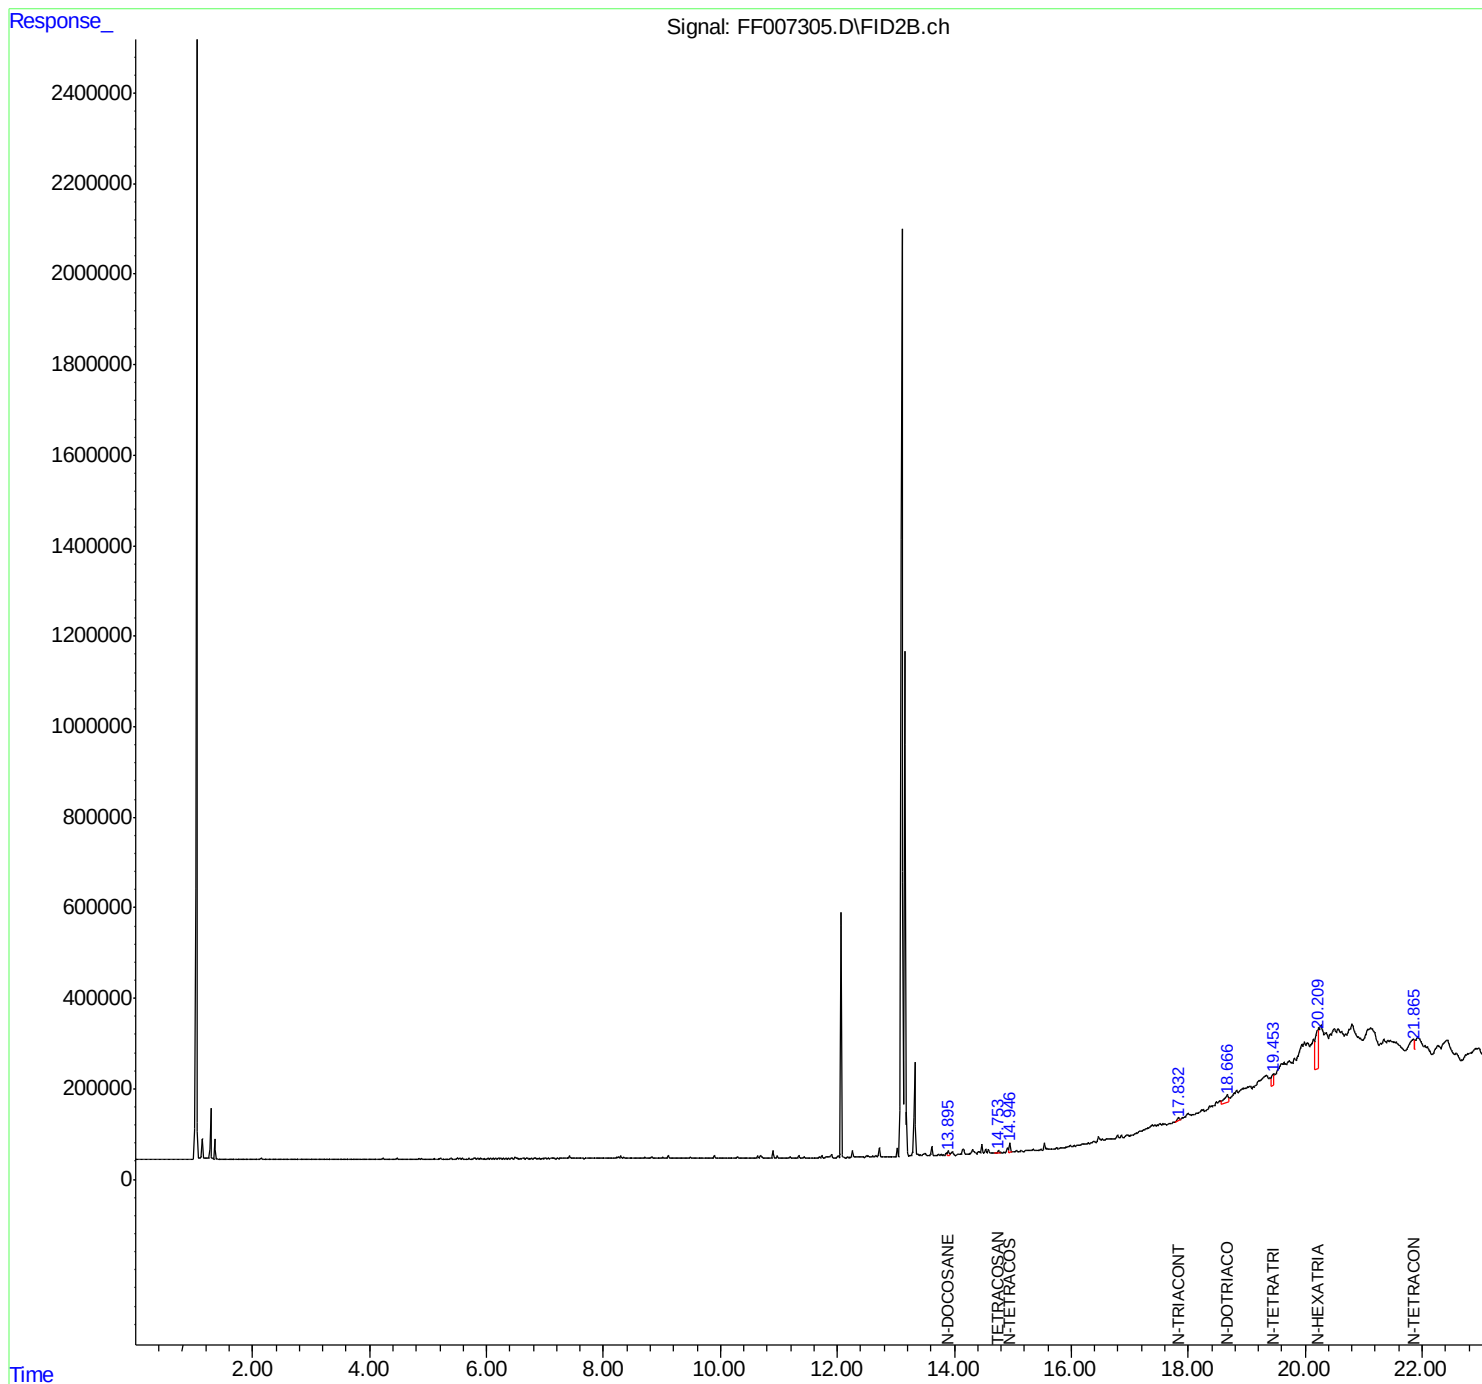


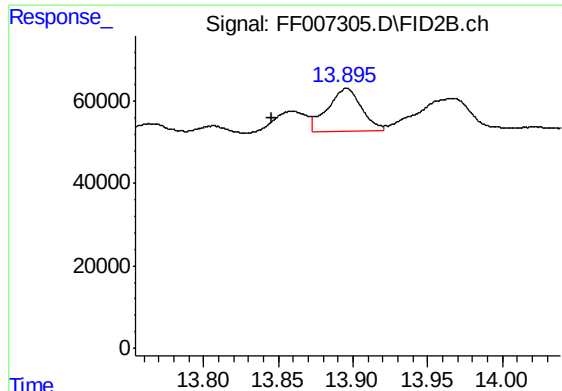

#8 N-DOCOSANE


R.T.: 13.896 min
Delta R.T.: 0.051 min
Response: 165141
Conc: 1.06 ug/ml

Instrument :
FID_F
ClientSampleId :
TR-04-080620

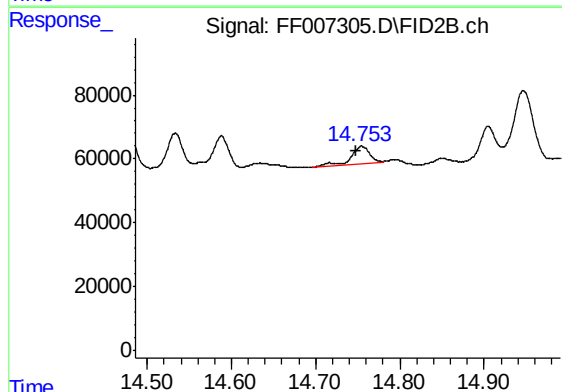


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.754 min
Delta R.T.: 0.006 min
Response: 81422
Conc: 0.60 ug/ml

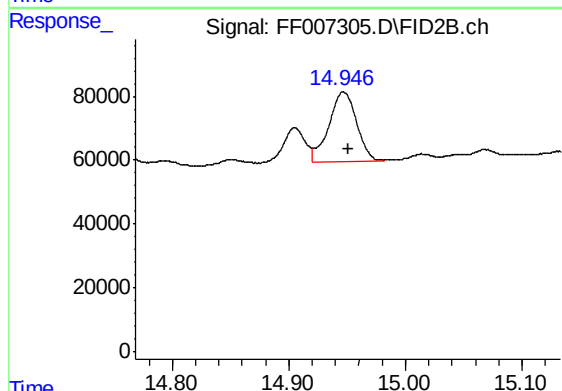


#10 N-TETRACOSANE

R.T.: 14.947 min
Delta R.T.: -0.005 min
Response: 356325
Conc: 2.26 ug/ml

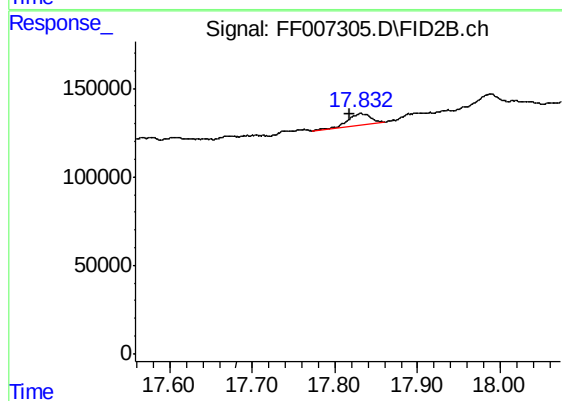

#13 N-TRIACONTANE


R.T.: 17.831 min
Delta R.T.: 0.013 min
Response: 126132
Conc: 0.80 ug/ml

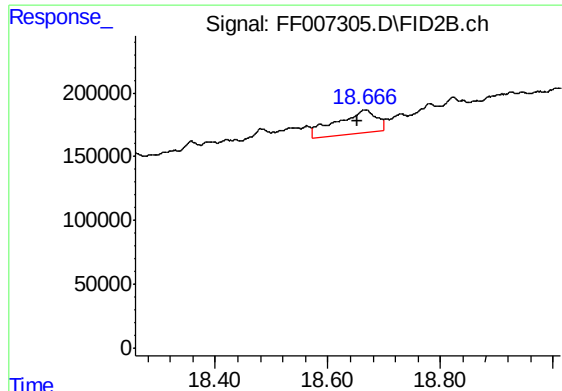

#14 N-DOTRIACONTANE


R.T.: 18.667 min
Delta R.T.: 0.014 min
Response: 892033
Conc: 6.02 ug/ml

Instrument :
FID_F
ClientSampleId :
TR-04-080620

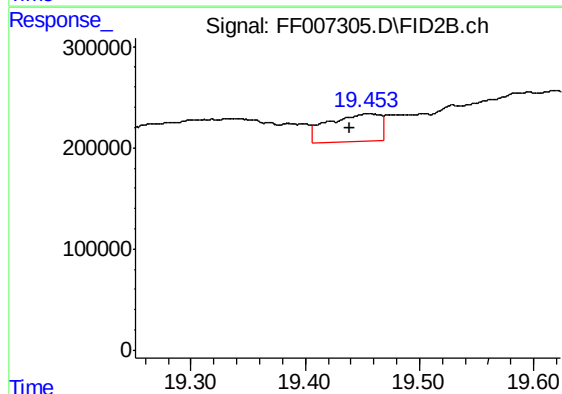


#15 N-TETRATRIACONTANE

R.T.: 19.454 min
Delta R.T.: 0.016 min
Response: 847048
Conc: 7.00 ug/ml

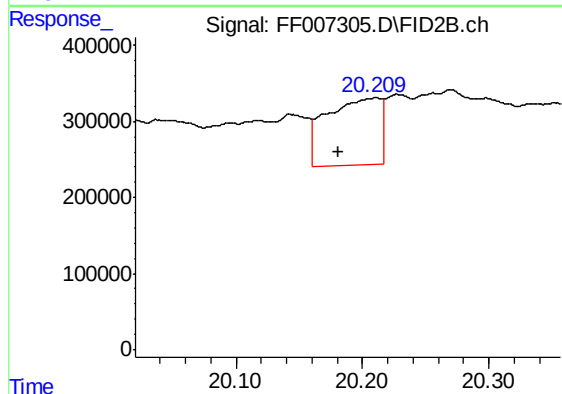

#16 N-HEXATRIACONTANE

R.T.: 20.211 min
Delta R.T.: 0.030 min
Response: 2601809
Conc: 28.13 ug/ml

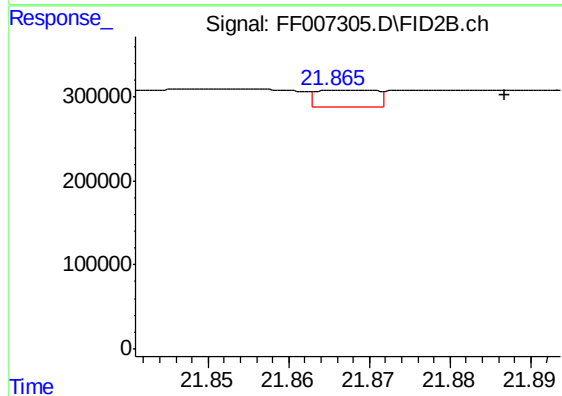

#18 N-TETRACONTANE

R.T.: 21.868 min
Delta R.T.: -0.019 min
Response: 104030
Conc: 1.56 ug/ml