

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
 Data File : FF013119.D
 Signal(s) : FID2B.ch
 Acq On : 07 Aug 2023 11:27
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 08 04:40:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
 Quant Title :
 QLast Update : Wed Aug 02 19:16:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.704	2300982	19.642 ug/ml
12) N-OCTACOSANE	17.159	2395188	19.382 ug/ml
14) N-DOTRIACONTANE	18.906	156183	1.386 ug/ml
16) N-HEXATRIACONTANE	20.454f	201932	2.259 ug/ml
18) N-TETRACONTANE	22.096f	255044	3.385 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
Data File : FF013119.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2023 11:27
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 04:40:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

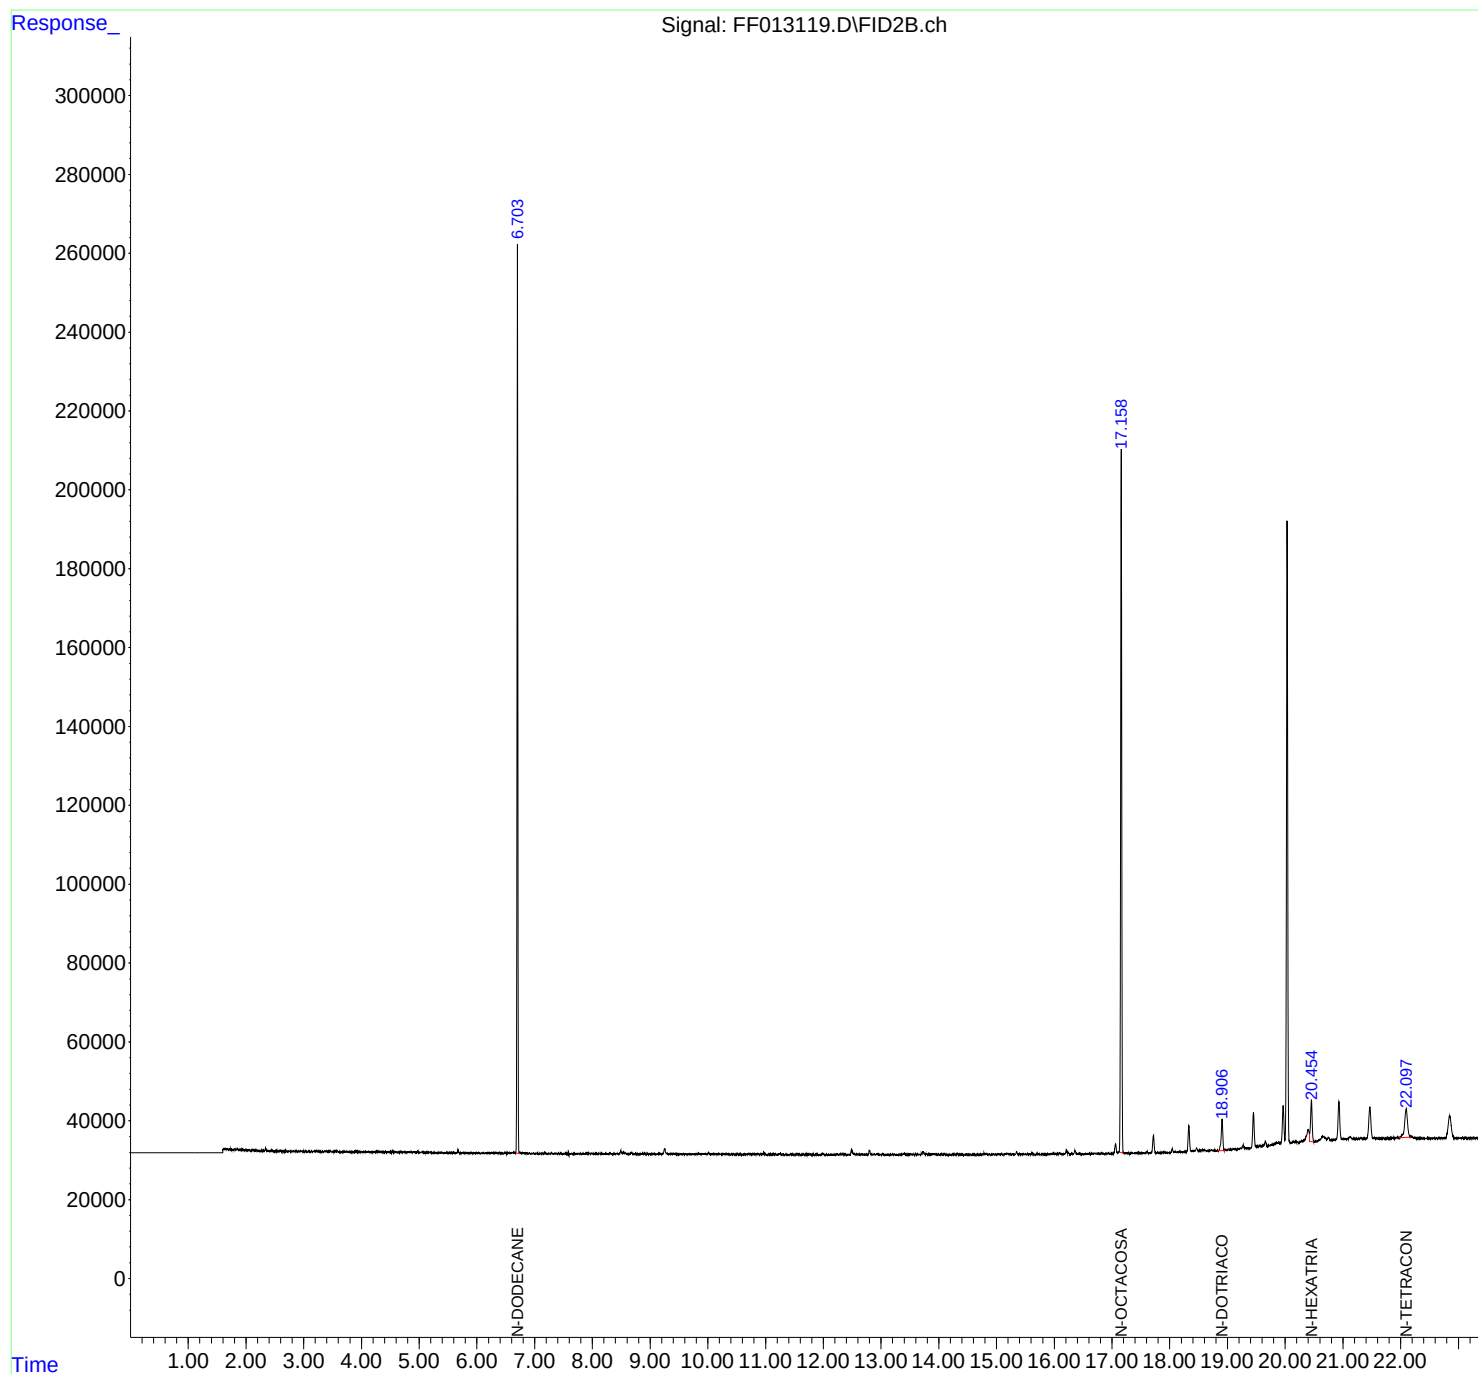


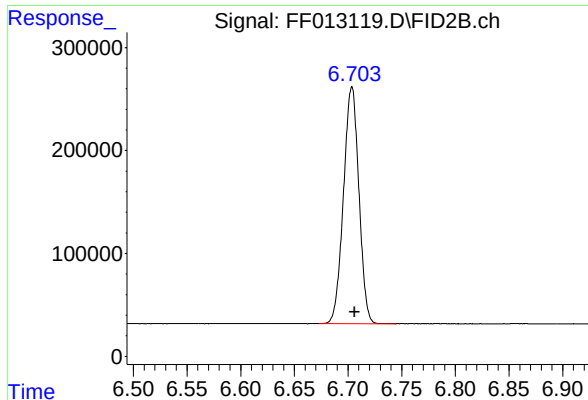

#3 N-DODECANE


R.T.: 6.704 min
Delta R.T.: -0.002 min
Response: 2300982
Conc: 19.64 ug/ml

Instrument :
FID_F
ClientSampleId :

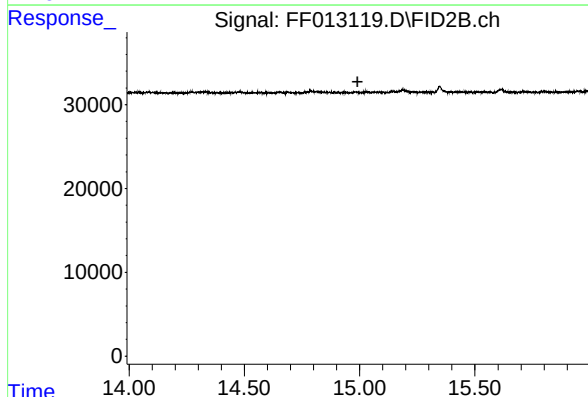


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.991 min
Response: 0
Conc: N.D.

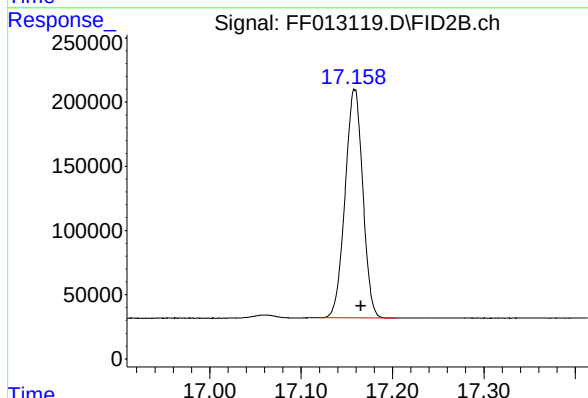


#12 N-OCTACOSANE

R.T.: 17.159 min
Delta R.T.: -0.007 min
Response: 2395188
Conc: 19.38 ug/ml

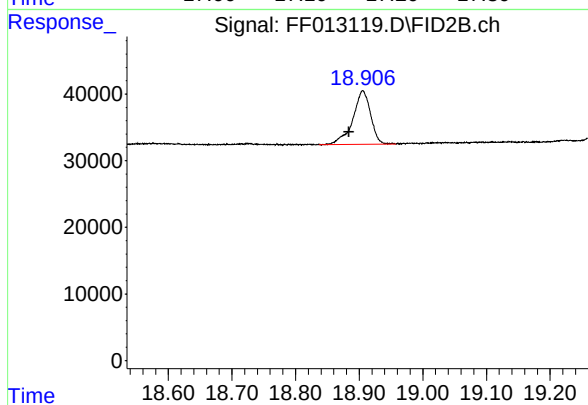

#14 N-DOTRIACONTANE


R.T.: 18.906 min
Delta R.T.: 0.022 min
Response: 156183
Conc: 1.39 ug/ml

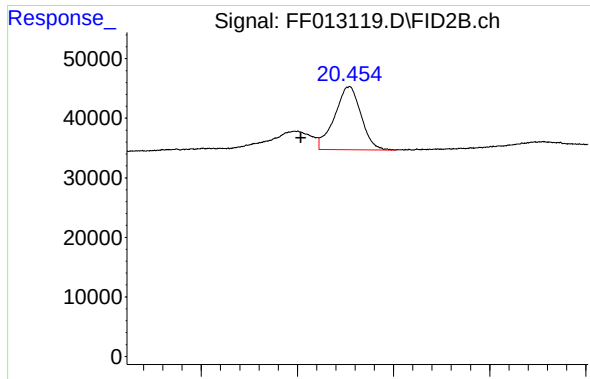

#16 N-HEXATRIACONTANE

R.T.: 20.454 min
Delta R.T.: 0.050 min
Response: 201932
Conc: 2.26 ug/ml

Instrument :
FID_F
ClientSampleId :

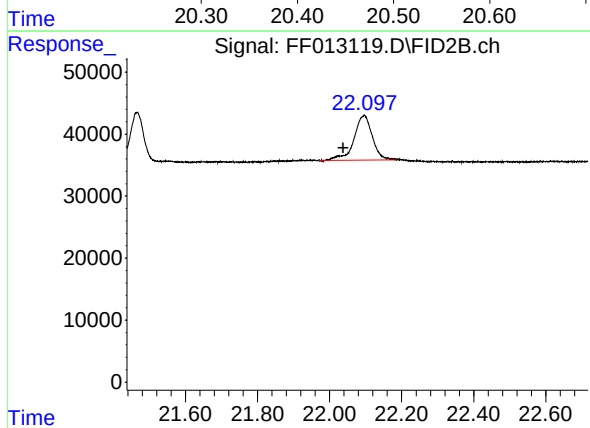

#18 N-TETRACONTANE

R.T.: 22.096 min
Delta R.T.: 0.058 min
Response: 255044
Conc: 3.38 ug/ml