

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
Data File : FF013123.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2023 15:25
Operator : YP\AJ
Sample : PB154659BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 04:41:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.987	2127420	19.738 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.456f	78916	0.883 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
Data File : FF013123.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2023 15:25
Operator : YP\AJ
Sample : PB154659BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 04:41:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

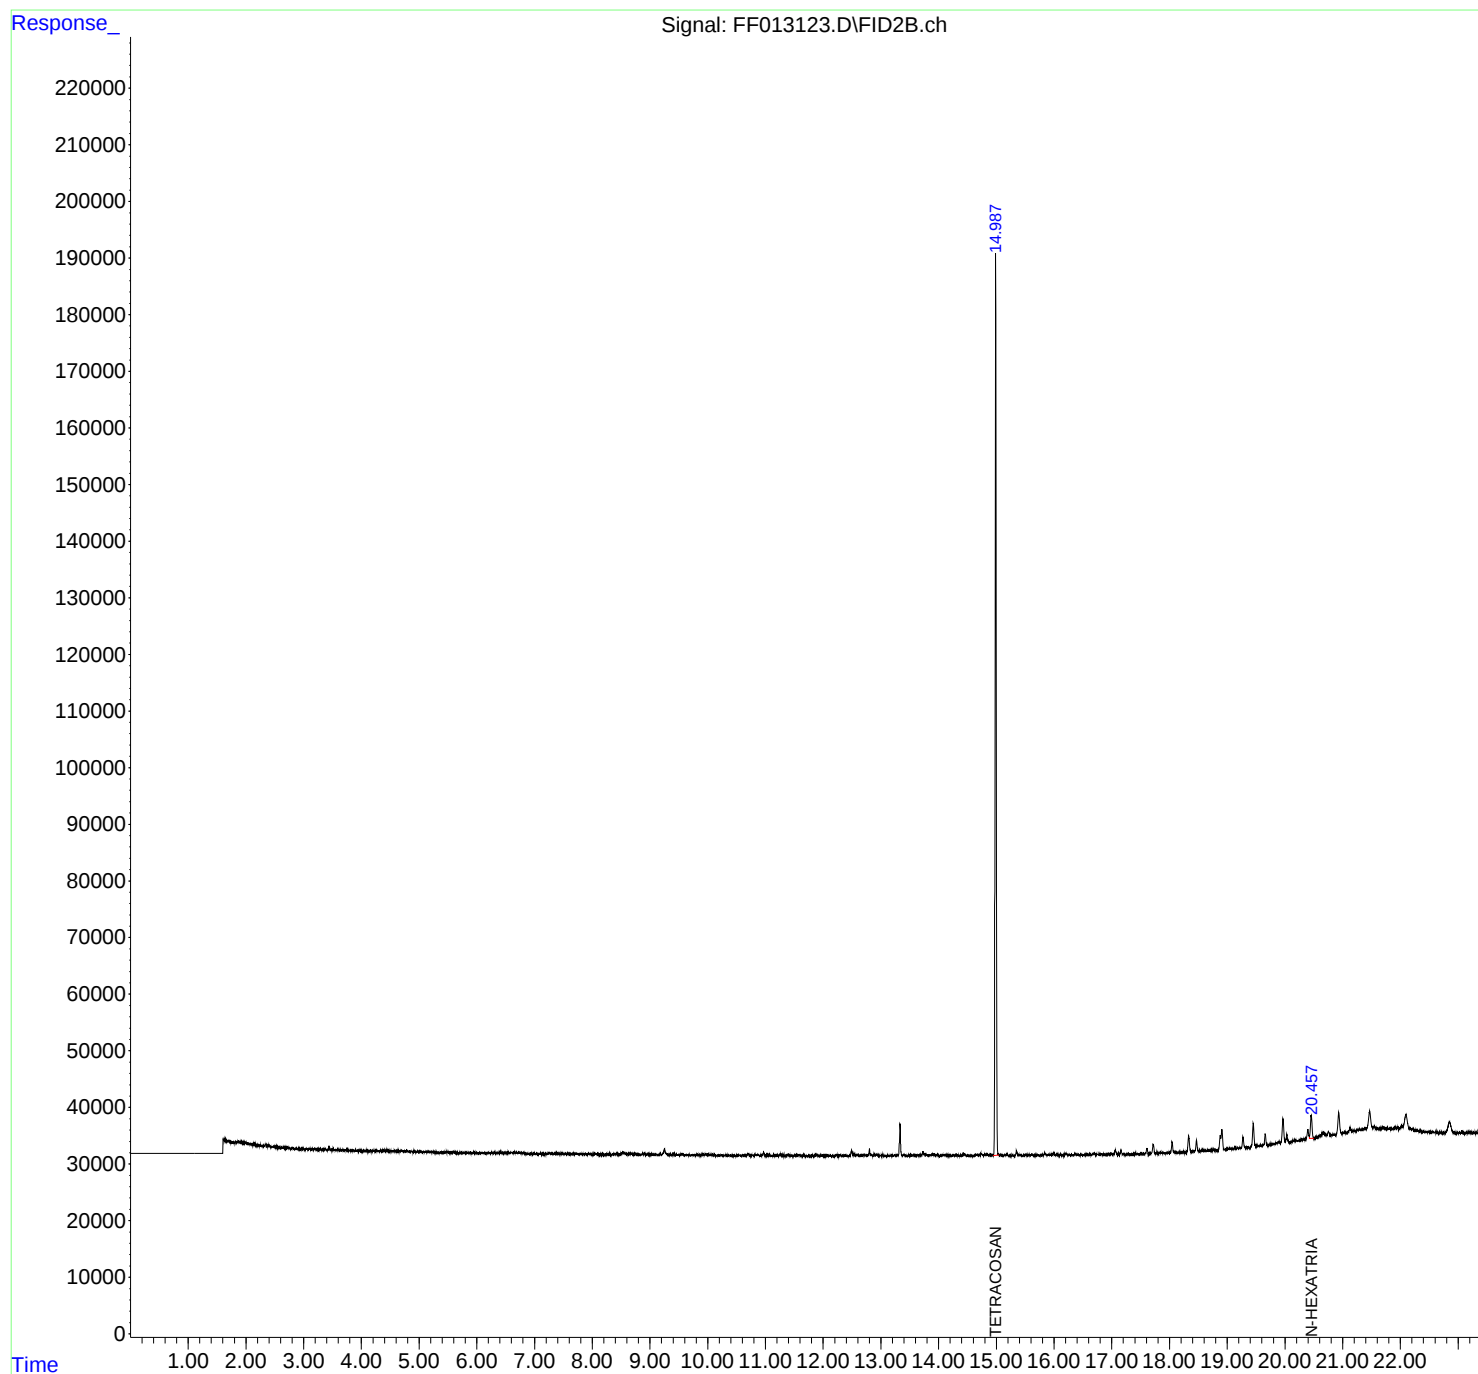


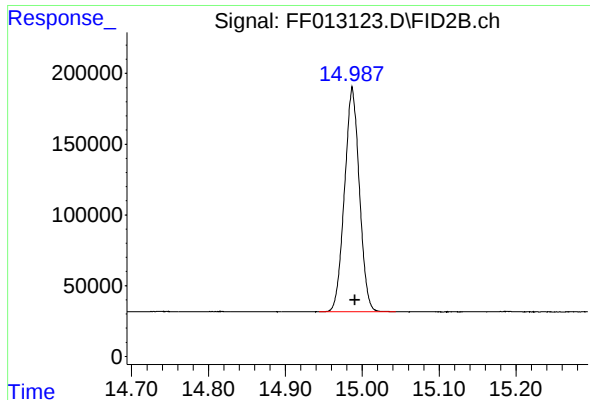

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.987 min
Delta R.T.: -0.004 min
Response: 2127420
Conc: 19.74 ug/ml

Instrument :
FID_F
ClientSampleId :

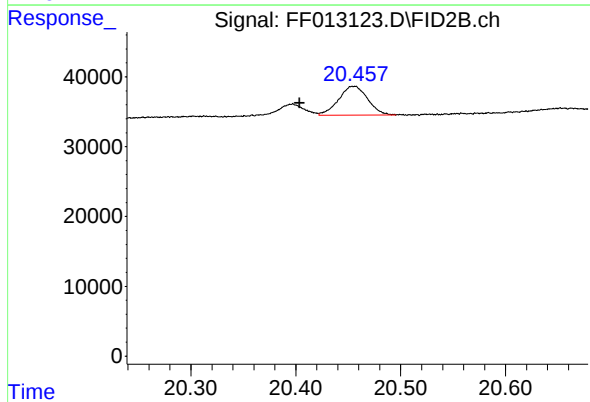

#16 N-HEXATRIACONTANE

R.T.: 20.456 min
Delta R.T.: 0.052 min
Response: 78916
Conc: 0.88 ug/ml