

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
Data File : FF013130.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2023 18:53
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 04:42:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.988	2151259	19.959 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.877	36812	0.327 ug/ml
16) N-HEXATRIACONTANE	20.399	78667	0.880 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
Data File : FF013130.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2023 18:53
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 04:42:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

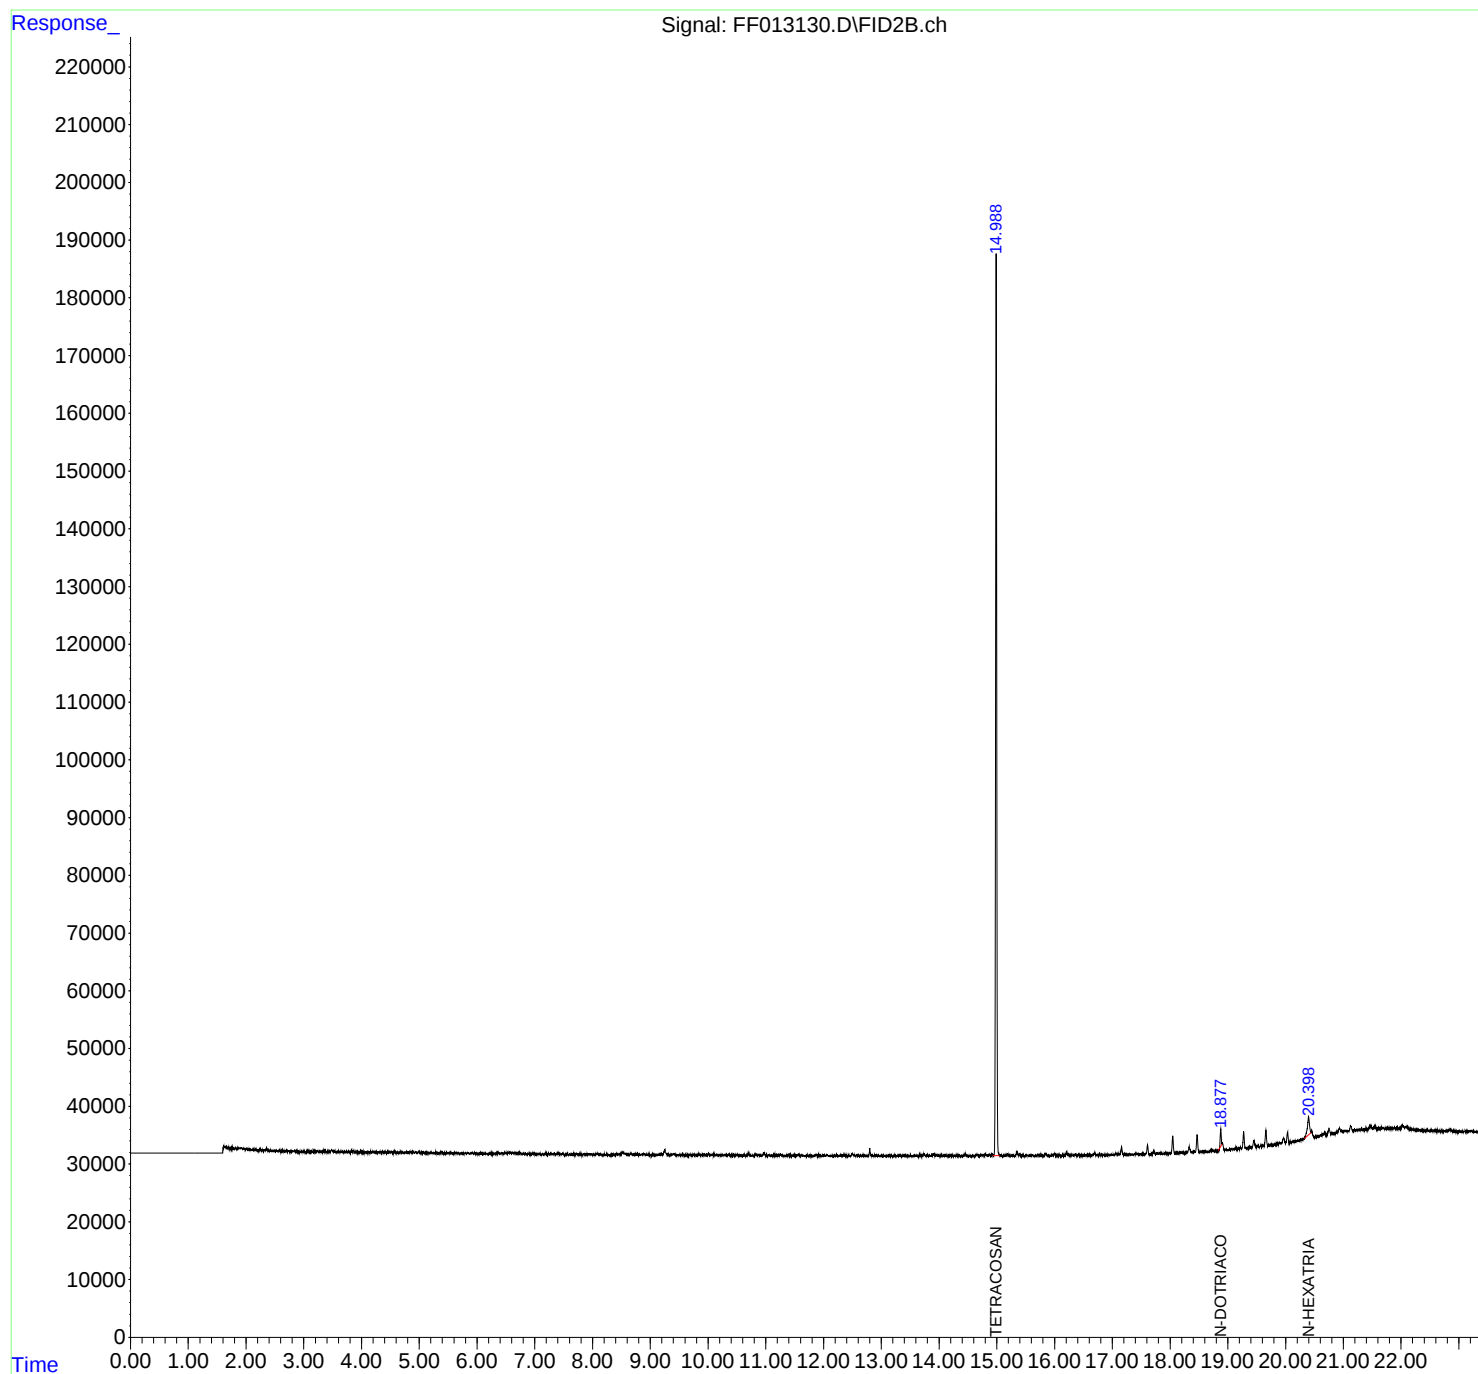


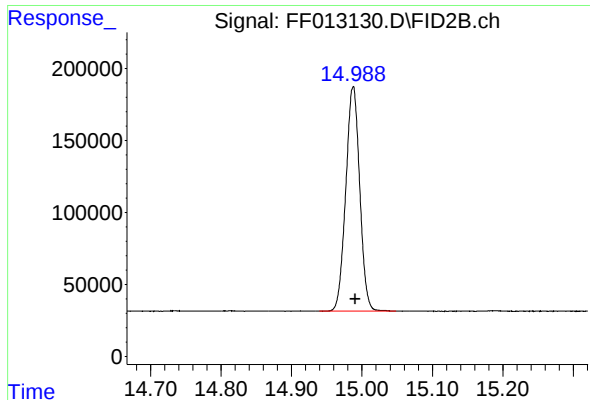

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.988 min
Delta R.T.: -0.003 min
Response: 2151259
Conc: 19.96 ug/ml

Instrument :
FID_F
ClientSampleId :

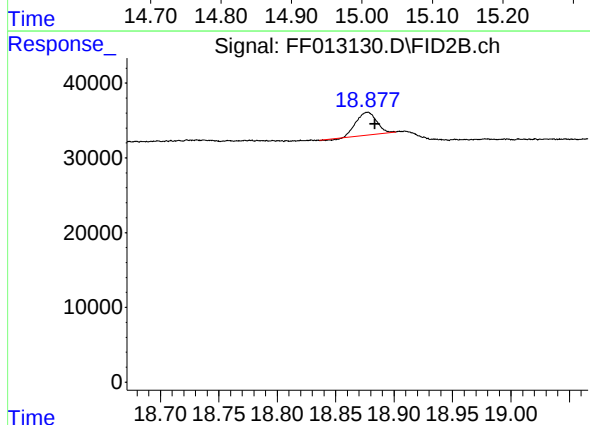

#14 N-DOTRIACONTANE

R.T.: 18.877 min
Delta R.T.: -0.006 min
Response: 36812
Conc: 0.33 ug/ml

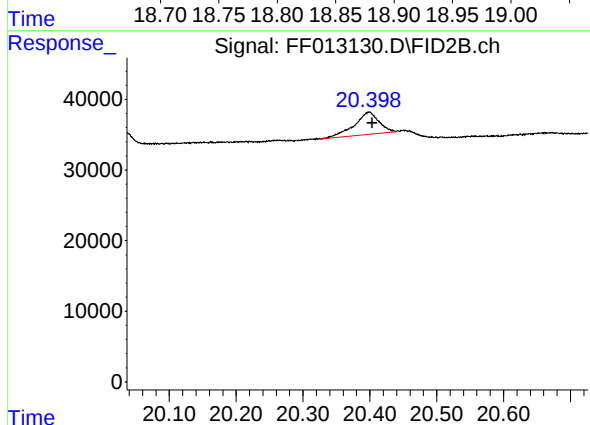

#16 N-HEXATRIACONTANE

R.T.: 20.399 min
Delta R.T.: -0.005 min
Response: 78667
Conc: 0.88 ug/ml