

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
 Data File : FF013134.D
 Signal(s) : FID2B.ch
 Acq On : 07 Aug 2023 20:53
 Operator : YP\AJ
 Sample : 03572-06
 Misc : TPH GC MDL 1 PPM
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 08 04:42:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
 Quant Title :
 QLast Update : Wed Aug 02 19:16:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.987	2116749	19.639 ug/ml
Target Compounds			
1) N-OCTANE	2.013	101563	0.899 ug/ml
2) N-DECANE	4.539	119384	1.026 ug/ml
3) N-DODECANE	6.704	119773	1.022 ug/ml
4) N-TETRADECANE	8.528	124365	1.055 ug/ml
5) N-HEXADECANE	10.136	122961	1.031 ug/ml
6) N-OCTADECANE	11.579	127889	1.053 ug/ml
7) N-EICOSANE	12.889	125935	1.042 ug/ml
8) N-DOCOSANE	14.086	126230	1.046 ug/ml
10) N-TETRACOSANE	15.189	129177	1.055 ug/ml
11) N-HEXACOSANE	16.209	129719	1.041 ug/ml
12) N-OCTACOSANE	17.157	138460	1.120 ug/ml
13) N-TRIACONTANE	18.044	164052	1.351 ug/ml
14) N-DOTRIACONTANE	18.875	204391	1.814 ug/ml
15) N-TETRATRIACONTANE	19.658	152277	1.529 ug/ml
16) N-HEXATRIACONTANE	20.396	117236	1.312 ug/ml
17) N-OCTATRIACONTANE	21.126	98500	1.255 ug/ml
18) N-TETRACONTANE	22.025	73700	0.978 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
Data File : FF013134.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2023 20:53
Operator : YP\AJ
Sample : 03572-06
Misc : TPH GC MDL 1 PPM
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 04:42:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

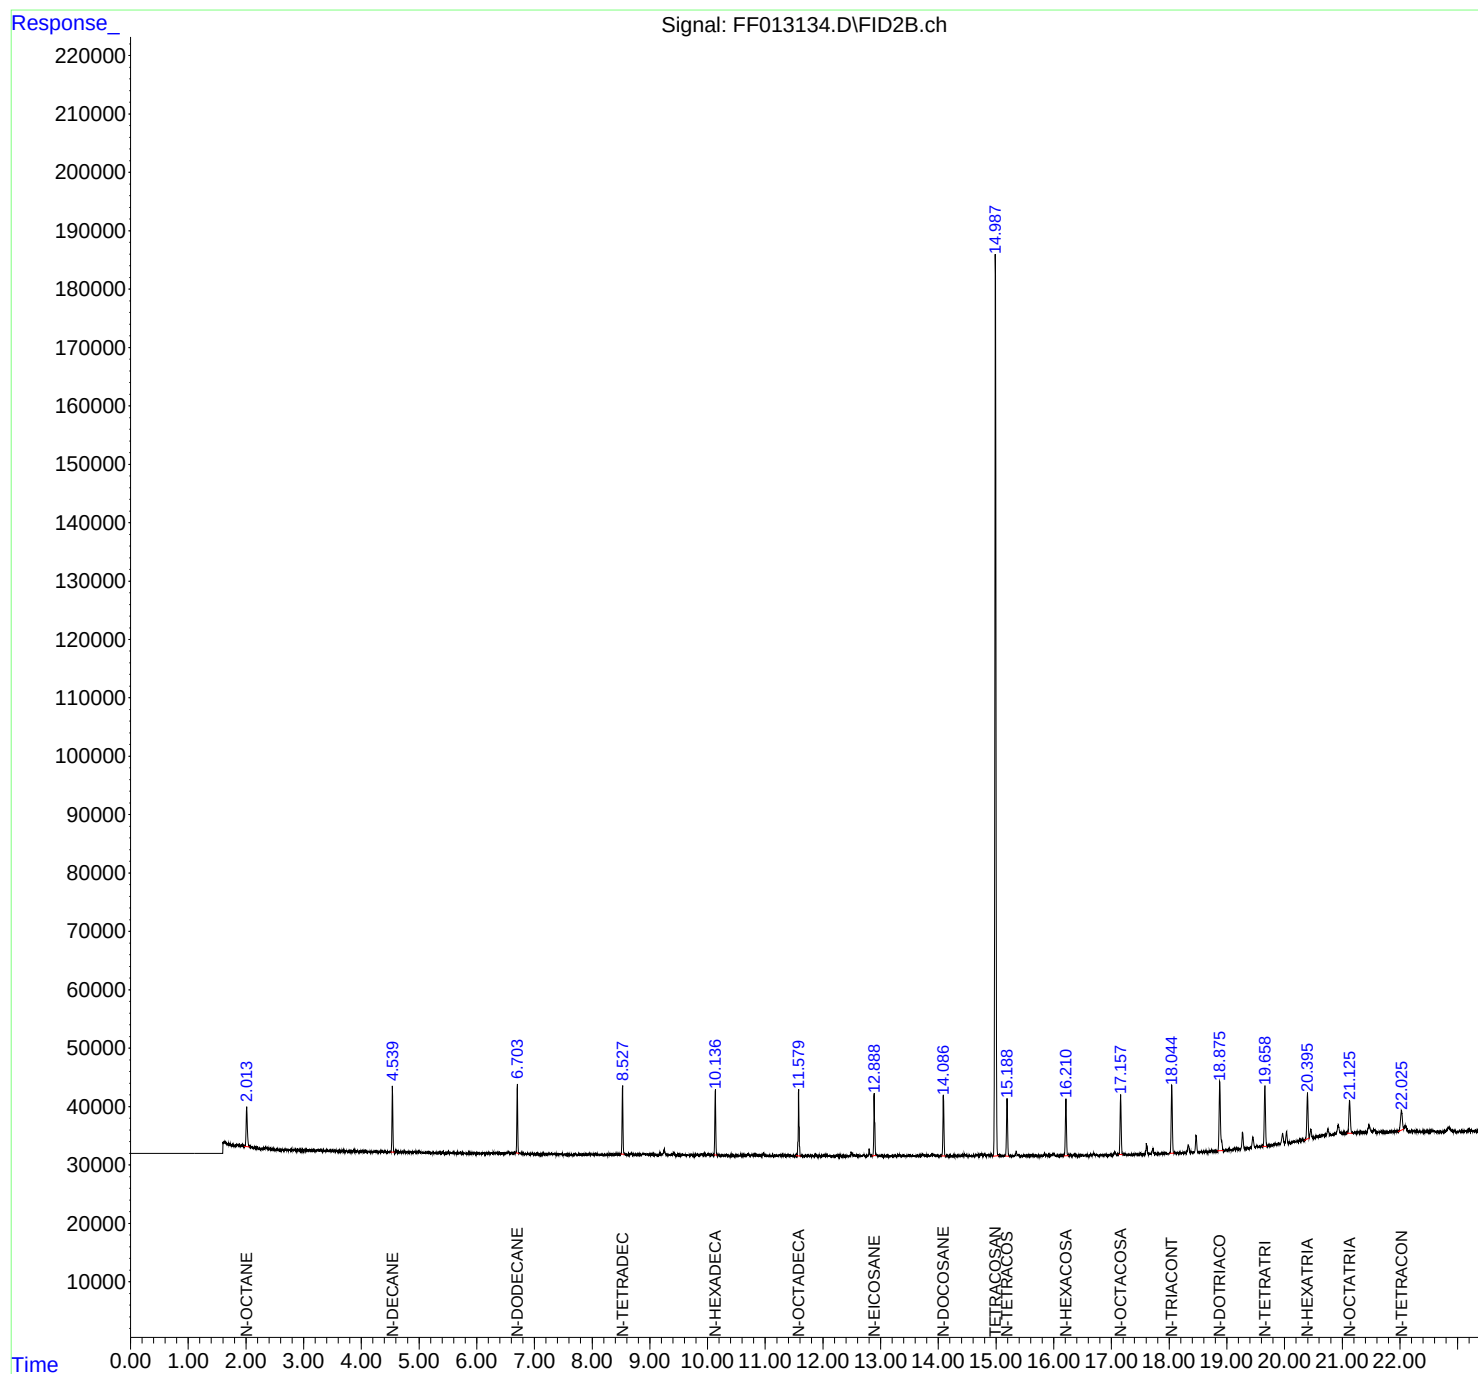


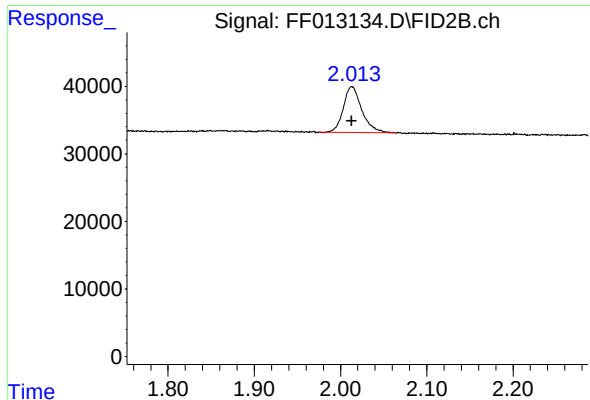

#1 N-OCTANE


R.T.: 2.013 min
Delta R.T.: 0.000 min
Response: 101563
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :

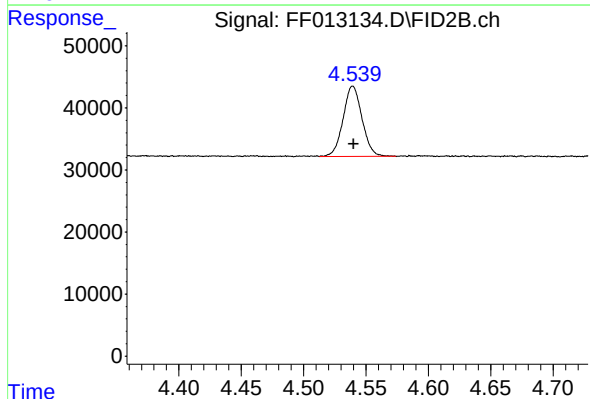


#2 N-DECANE

R.T.: 4.539 min
Delta R.T.: 0.000 min
Response: 119384
Conc: 1.03 ug/ml

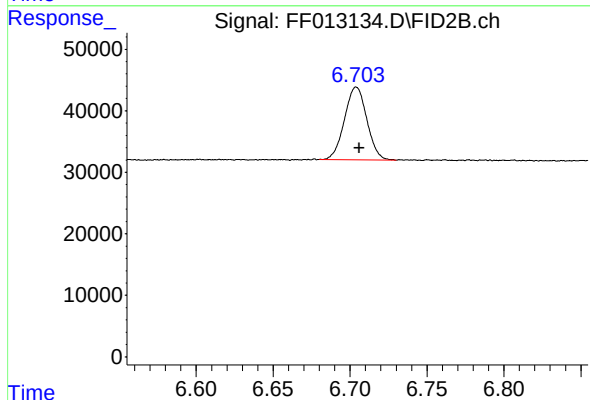


#3 N-DODECANE

R.T.: 6.704 min
Delta R.T.: -0.002 min
Response: 119773
Conc: 1.02 ug/ml

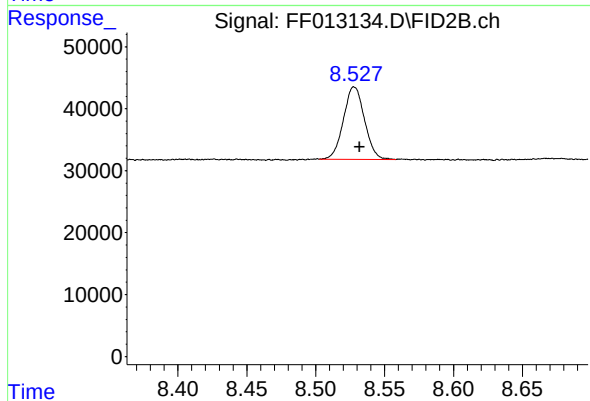

#4 N-TETRADECANE


R.T.: 8.528 min
Delta R.T.: -0.004 min
Response: 124365
Conc: 1.06 ug/ml

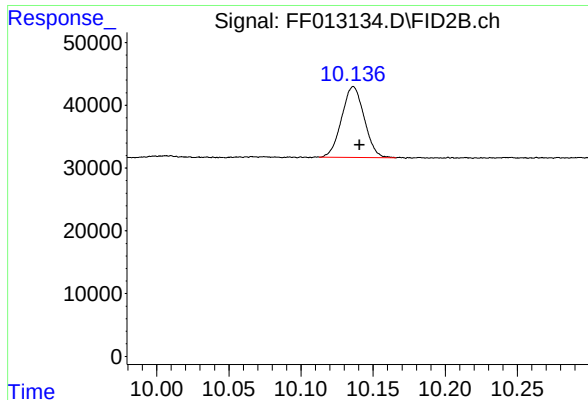

#5 N-HEXADECANE


R.T.: 10.136 min
Delta R.T.: -0.004 min
Response: 122961
Conc: 1.03 ug/ml

Instrument :
FID_F
ClientSampleId :

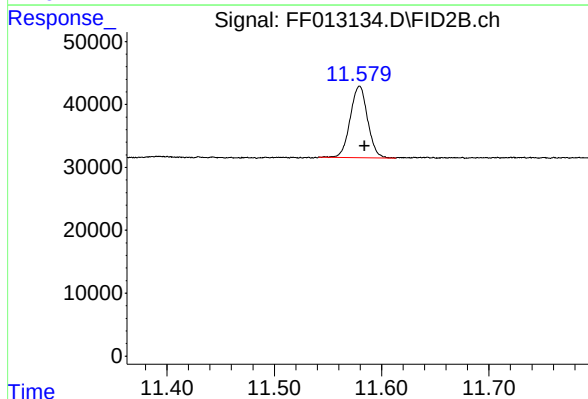


#6 N-OCTADECANE

R.T.: 11.579 min
Delta R.T.: -0.005 min
Response: 127889
Conc: 1.05 ug/ml

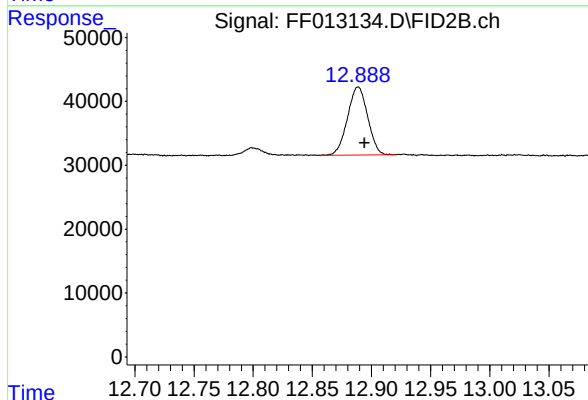


#7 N-EICOSANE

R.T.: 12.889 min
Delta R.T.: -0.005 min
Response: 125935
Conc: 1.04 ug/ml

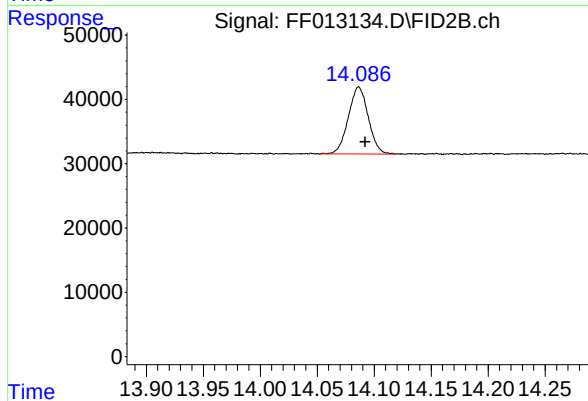

#8 N-DOCOSANE


R.T.: 14.086 min
Delta R.T.: -0.006 min
Response: 126230
Conc: 1.05 ug/ml

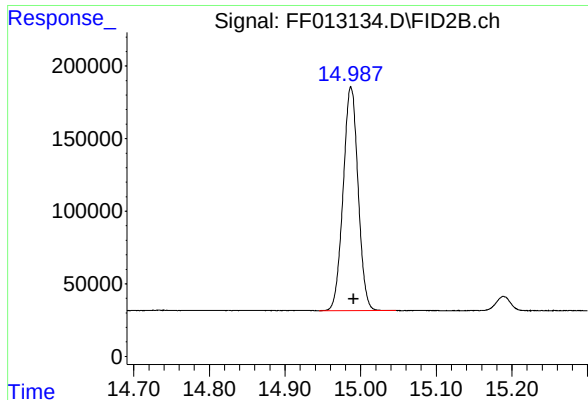

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.987 min
Delta R.T.: -0.003 min
Response: 2116749
Conc: 19.64 ug/ml

Instrument :
FID_F
ClientSampleId :

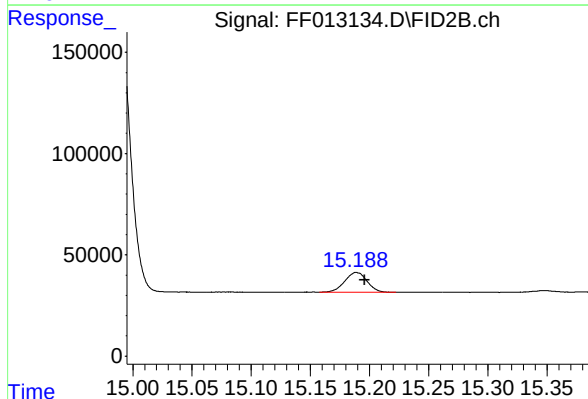


#10 N-TETRACOSANE

R.T.: 15.189 min
Delta R.T.: -0.007 min
Response: 129177
Conc: 1.06 ug/ml

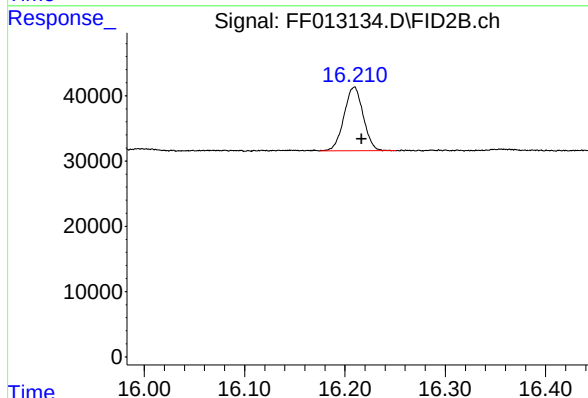


#11 N-HEXACOSANE

R.T.: 16.209 min
Delta R.T.: -0.007 min
Response: 129719
Conc: 1.04 ug/ml

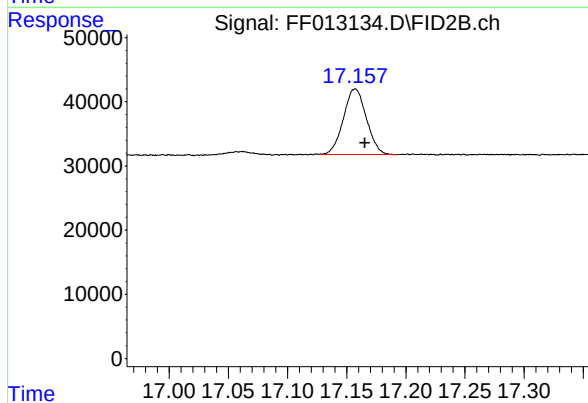

#12 N-OCTACOSANE

R.T.: 17.157 min
Delta R.T.: -0.008 min
Response: 138460
Conc: 1.12 ug/ml

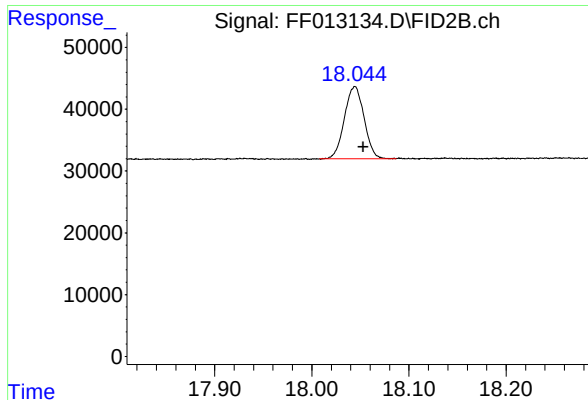


#13 N-TRIACONTANE

R.T.: 18.044 min
Delta R.T.: -0.008 min
Response: 164052
Conc: 1.35 ug/ml

Instrument :


FID_F

ClientSampleId :

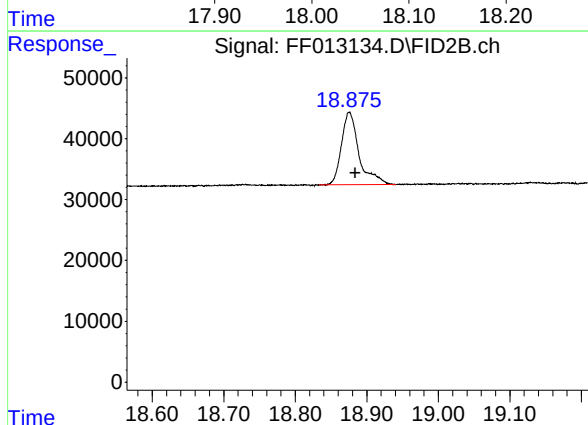


#14 N-DOTRIACONTANE

R.T.: 18.875 min
Delta R.T.: -0.008 min
Response: 204391
Conc: 1.81 ug/ml

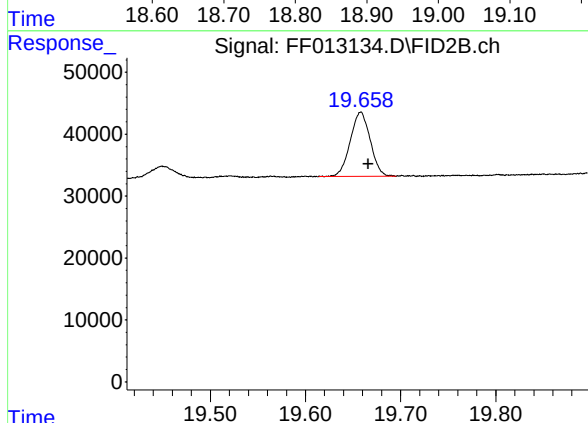


#15 N-TETRATRIACONTANE

R.T.: 19.658 min
Delta R.T.: -0.008 min
Response: 152277
Conc: 1.53 ug/ml

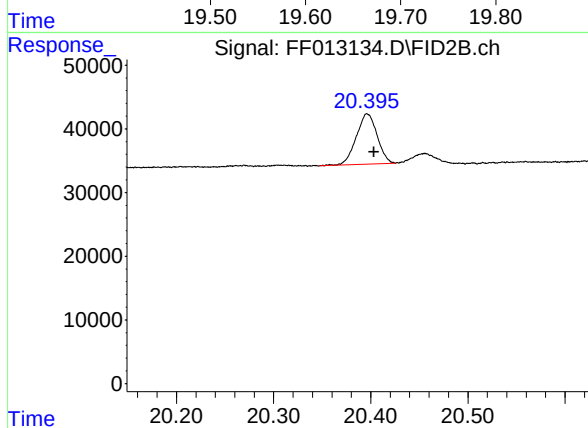

#16 N-HEXATRIACONTANE


R.T.: 20.396 min
Delta R.T.: -0.007 min
Response: 117236
Conc: 1.31 ug/ml

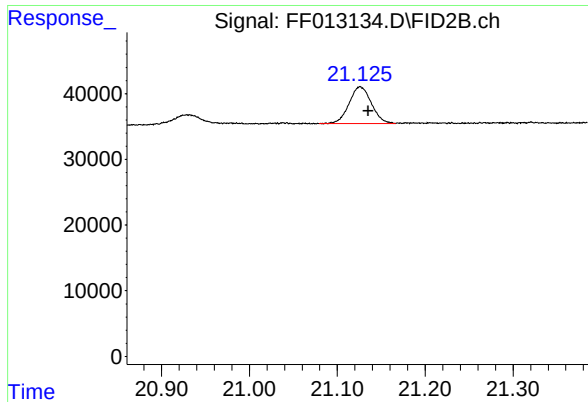

#17 N-OCTATRIACONTANE

R.T.: 21.126 min
Delta R.T.: -0.009 min
Response: 98500
Conc: 1.26 ug/ml

Instrument :
FID_F
ClientSampleId :

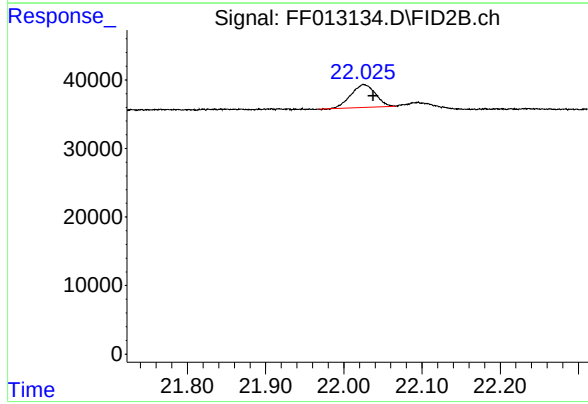

#18 N-TETRACONTANE

R.T.: 22.025 min
Delta R.T.: -0.013 min
Response: 73700
Conc: 0.98 ug/ml