

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF080723\  
Data File : FF013137.D  
Signal(s) : FID2B.ch  
Acq On : 07 Aug 2023 22:22  
Operator : YP\AJ  
Sample : I.BLK  
Misc : TPH GC MDL 1 PPM  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 08 04:43:14 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF080223.M  
Quant Title :  
QLast Update : Wed Aug 02 19:16:13 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.988 | 2069854  | 19.204 ug/ml |
| Target Compounds              |        |          |              |
| 14) N-DOTRIACONTANE           | 18.877 | 35534    | 0.315 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF080723\  
Data File : FF013137.D  
Signal(s) : FID2B.ch  
Acq On : 07 Aug 2023 22:22  
Operator : YP\AJ  
Sample : I.BLK  
Misc : TPH GC MDL 1 PPM  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 08 04:43:14 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF080223.M  
Quant Title :  
QLast Update : Wed Aug 02 19:16:13 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

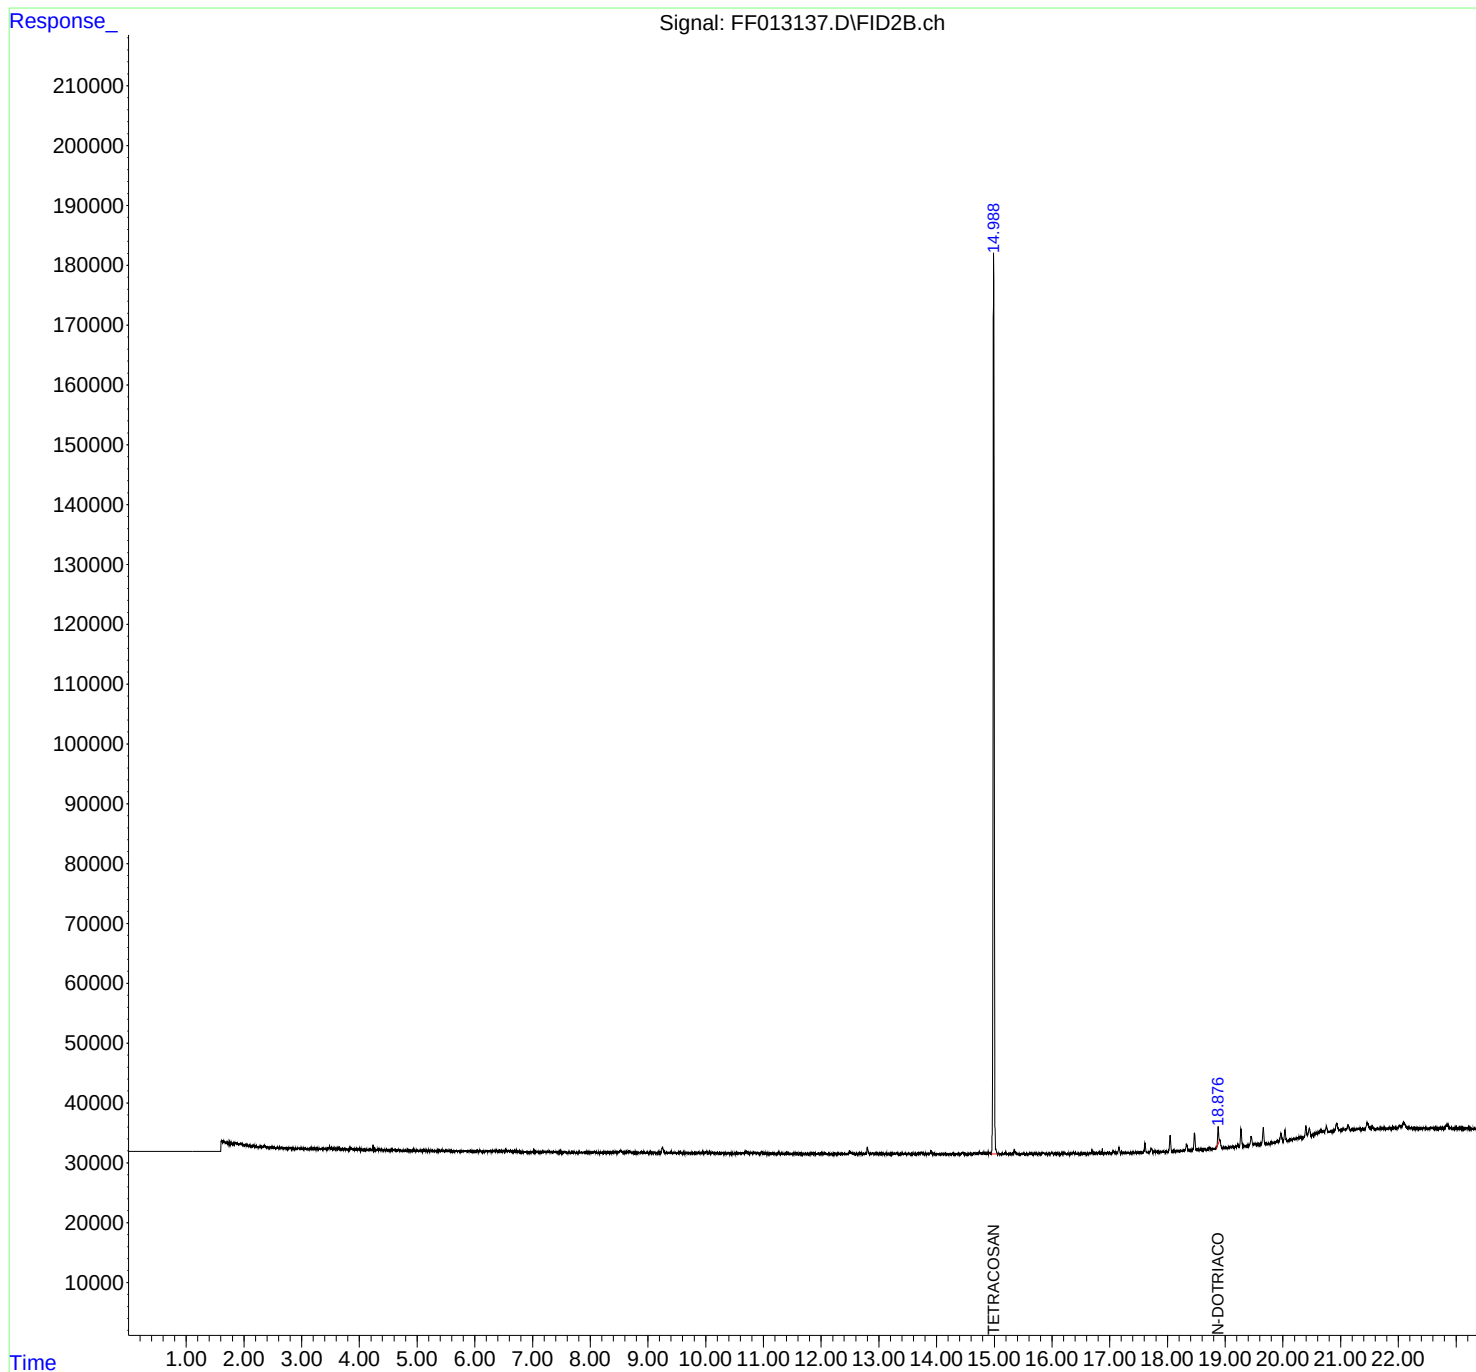


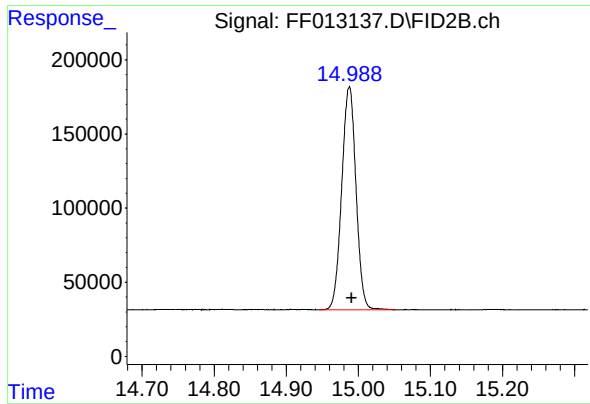

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.988 min  
Delta R.T.: -0.003 min  
Response: 2069854  
Conc: 19.20 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

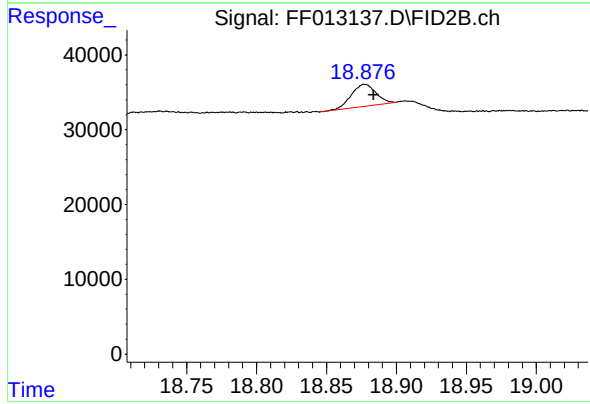

#14 N-DOTRIACONTANE

R.T.: 18.877 min  
Delta R.T.: -0.006 min  
Response: 35534  
Conc: 0.32 ug/ml