

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
 Data File : FF013129.D
 Signal(s) : FID2B.ch
 Acq On : 07 Aug 2023 18:23
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Aug 08 04:42:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
 Quant Title :
 QLast Update : Wed Aug 02 19:16:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.988	4754579	44.112 ug/ml
Target Compounds			
2) N-DECANE	4.540	5195592	44.648 ug/ml
3) N-DODECANE	6.706	5241434	44.742 ug/ml
4) N-TETRADECANE	8.531	5262135	44.656 ug/ml
5) N-HEXADECANE	10.139	5316225	44.561 ug/ml
6) N-OCTADECANE	11.582	5404030	44.489 ug/ml
7) N-EICOSANE	12.893	5370936	44.442 ug/ml
8) N-DOCOSANE	14.090	5342194	44.277 ug/ml
10) N-TETRACOSANE	15.193	5401734	44.132 ug/ml
11) N-HEXACOSANE	16.212	5399761	43.352 ug/ml
12) N-OCTACOSANE	17.162	5371430	43.465 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
Data File : FF013129.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2023 18:23
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Aug 08 04:42:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

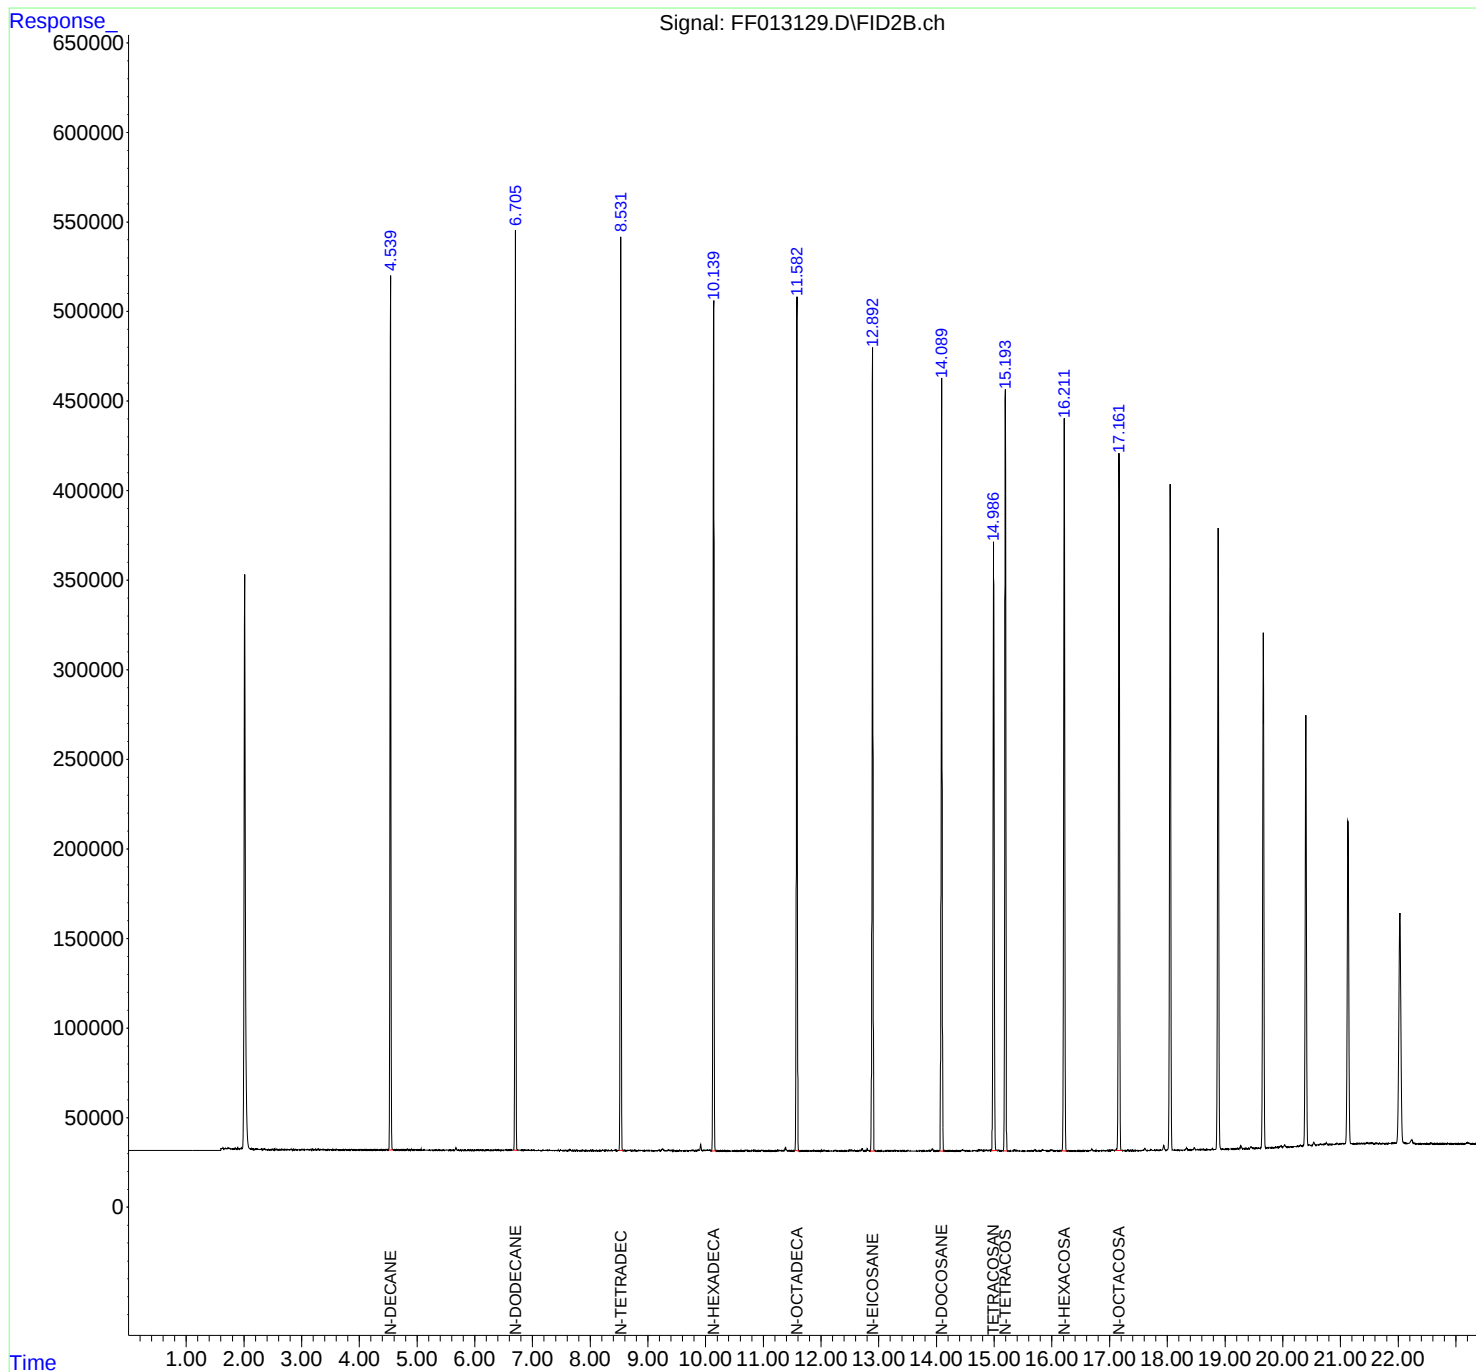


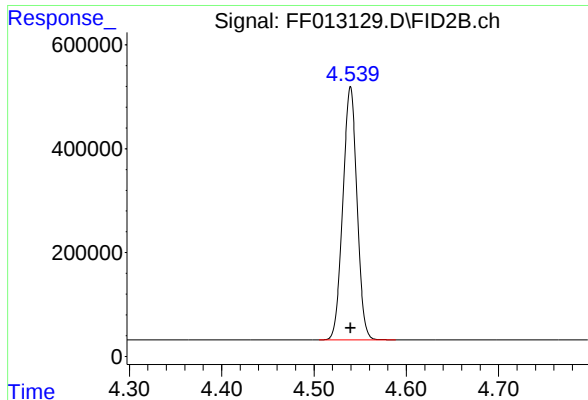

#2 N-DECANE


R.T.: 4.540 min
Delta R.T.: 0.000 min
Response: 5195592
Conc: 44.65 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

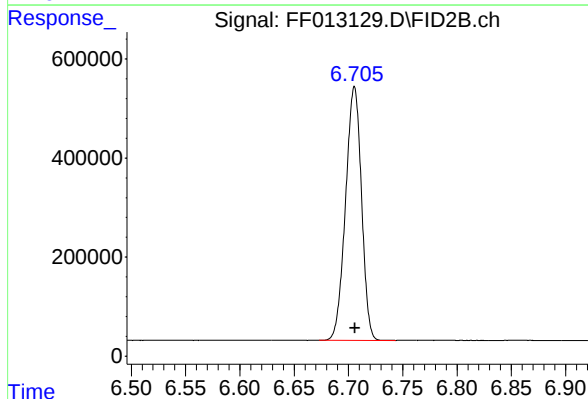


#3 N-DODECANE

R.T.: 6.706 min
Delta R.T.: 0.000 min
Response: 5241434
Conc: 44.74 ug/ml

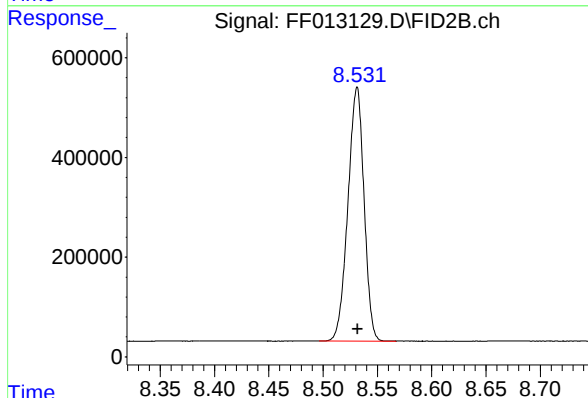


#4 N-TETRADECANE

R.T.: 8.531 min
Delta R.T.: 0.000 min
Response: 5262135
Conc: 44.66 ug/ml

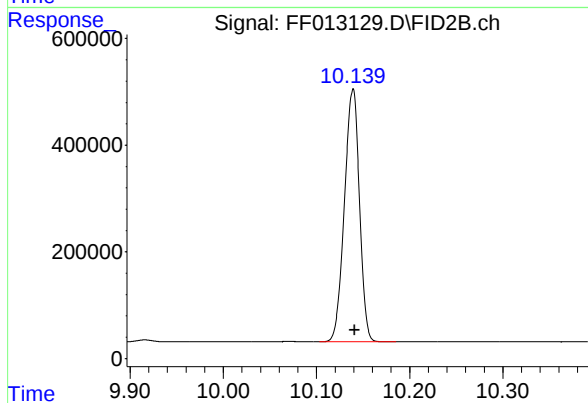

#5 N-HEXADECANE


R.T.: 10.139 min
Delta R.T.: -0.001 min
Response: 5316225
Conc: 44.56 ug/ml

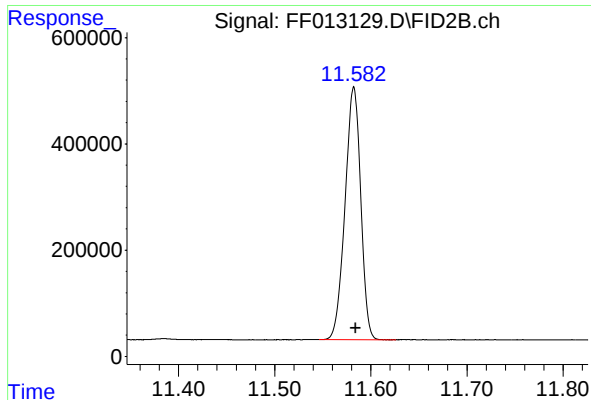

#6 N-OCTADECANE


R.T.: 11.582 min
Delta R.T.: -0.002 min
Response: 5404030
Conc: 44.49 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

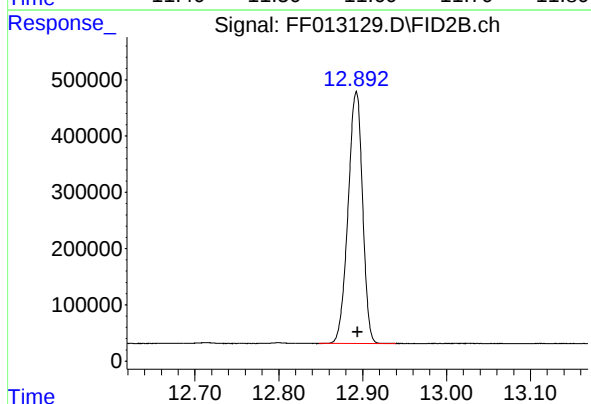


#7 N-EICOSANE

R.T.: 12.893 min
Delta R.T.: -0.002 min
Response: 5370936
Conc: 44.44 ug/ml

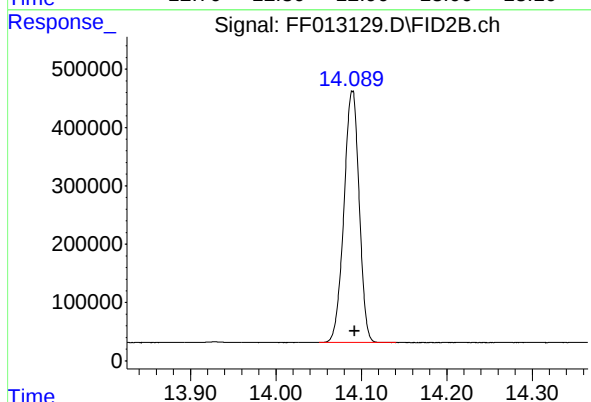


#8 N-DOCOSANE

R.T.: 14.090 min
Delta R.T.: -0.003 min
Response: 5342194
Conc: 44.28 ug/ml

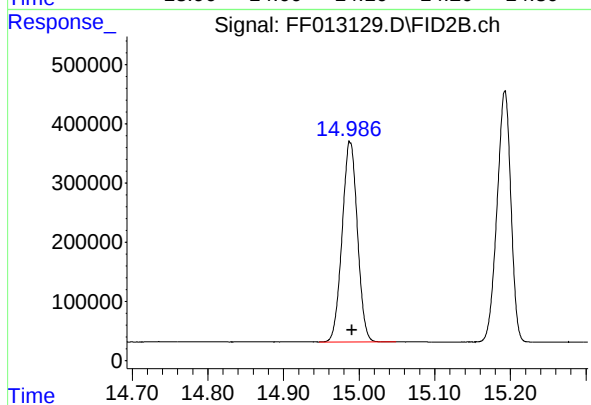

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.988 min
Delta R.T.: -0.003 min
Response: 4754579
Conc: 44.11 ug/ml

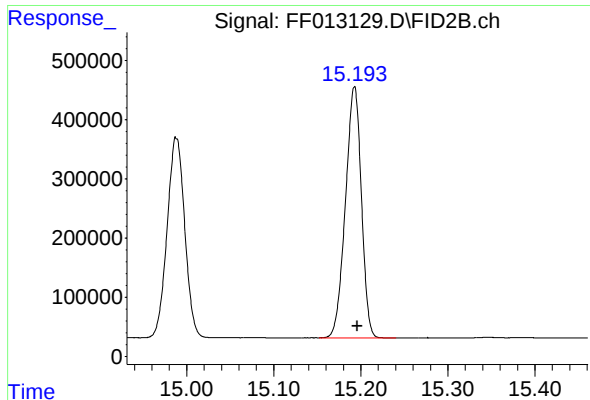

#10 N-TETRACOSANE


R.T.: 15.193 min
Delta R.T.: -0.003 min
Response: 5401734
Conc: 44.13 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

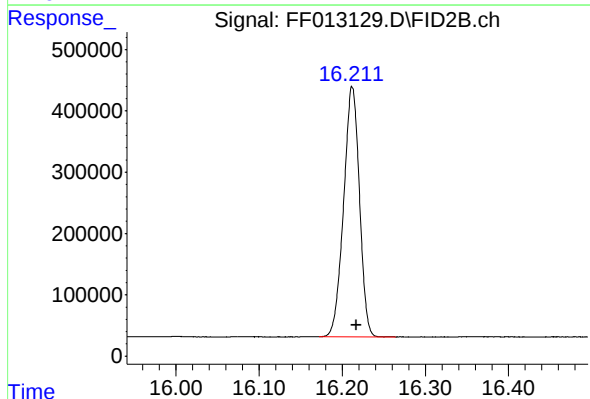

#11 N-HEXACOSANE

R.T.: 16.212 min
Delta R.T.: -0.005 min
Response: 5399761
Conc: 43.35 ug/ml

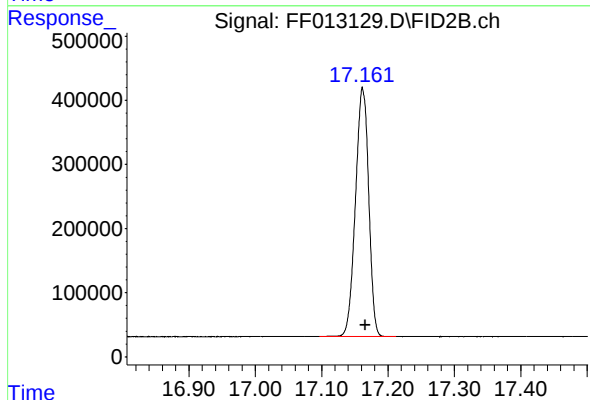

#12 N-OCTACOSANE

R.T.: 17.162 min
Delta R.T.: -0.004 min
Response: 5371430
Conc: 43.47 ug/ml