

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
Data File : FF013137.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2023 22:22
Operator : YP\AJ
Sample : I.BLK
Misc : TPH GC MDL 1 PPM
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 08 04:43:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.988	2069854	19.204 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080723\
Data File : FF013137.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2023 22:22
Operator : YP\AJ
Sample : I.BLK
Misc : TPH GC MDL 1 PPM
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 08 04:43:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

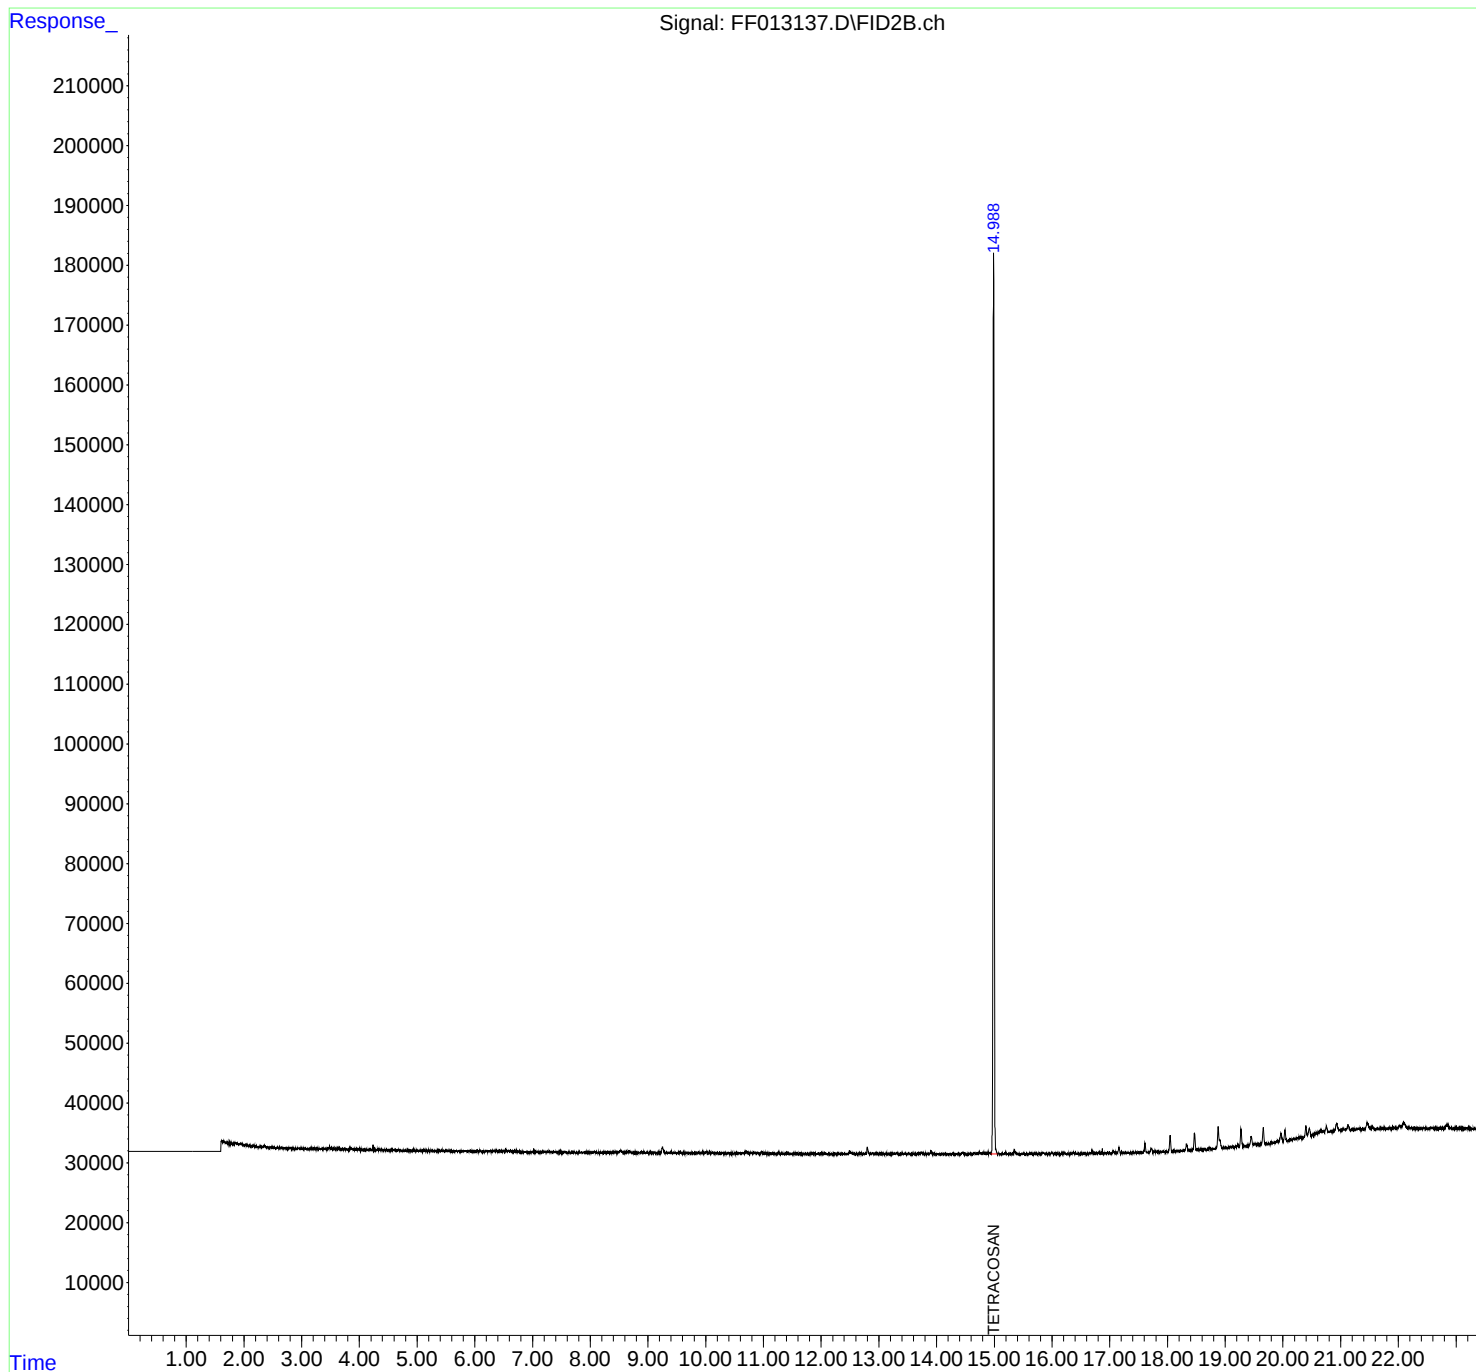

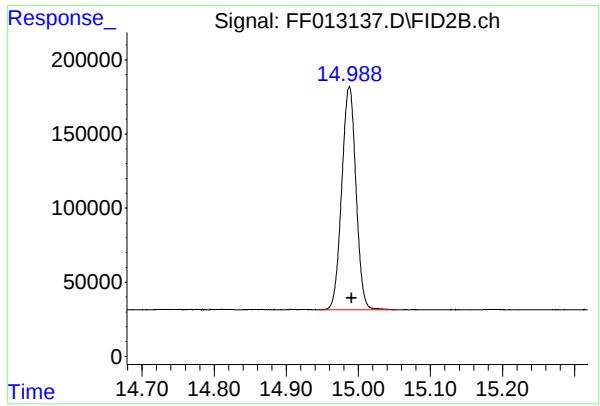

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.988 min
Delta R.T.: -0.003 min
Response: 2069854
Conc: 19.20 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK