

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080823\
Data File : FF013147.D
Signal(s) : FID2B.ch
Acq On : 08 Aug 2023 11:18
Operator : YP\AJ
Sample : PB154660BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB154660BL

Integration File: autoint1.e
Quant Time: Aug 09 02:11:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.988	3221989	29.893 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080823\
Data File : FF013147.D
Signal(s) : FID2B.ch
Acq On : 08 Aug 2023 11:18
Operator : YP\AJ
Sample : PB154660BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB154660BL

Integration File: autoint1.e
Quant Time: Aug 09 02:11:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080223.M
Quant Title :
QLast Update : Wed Aug 02 19:16:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

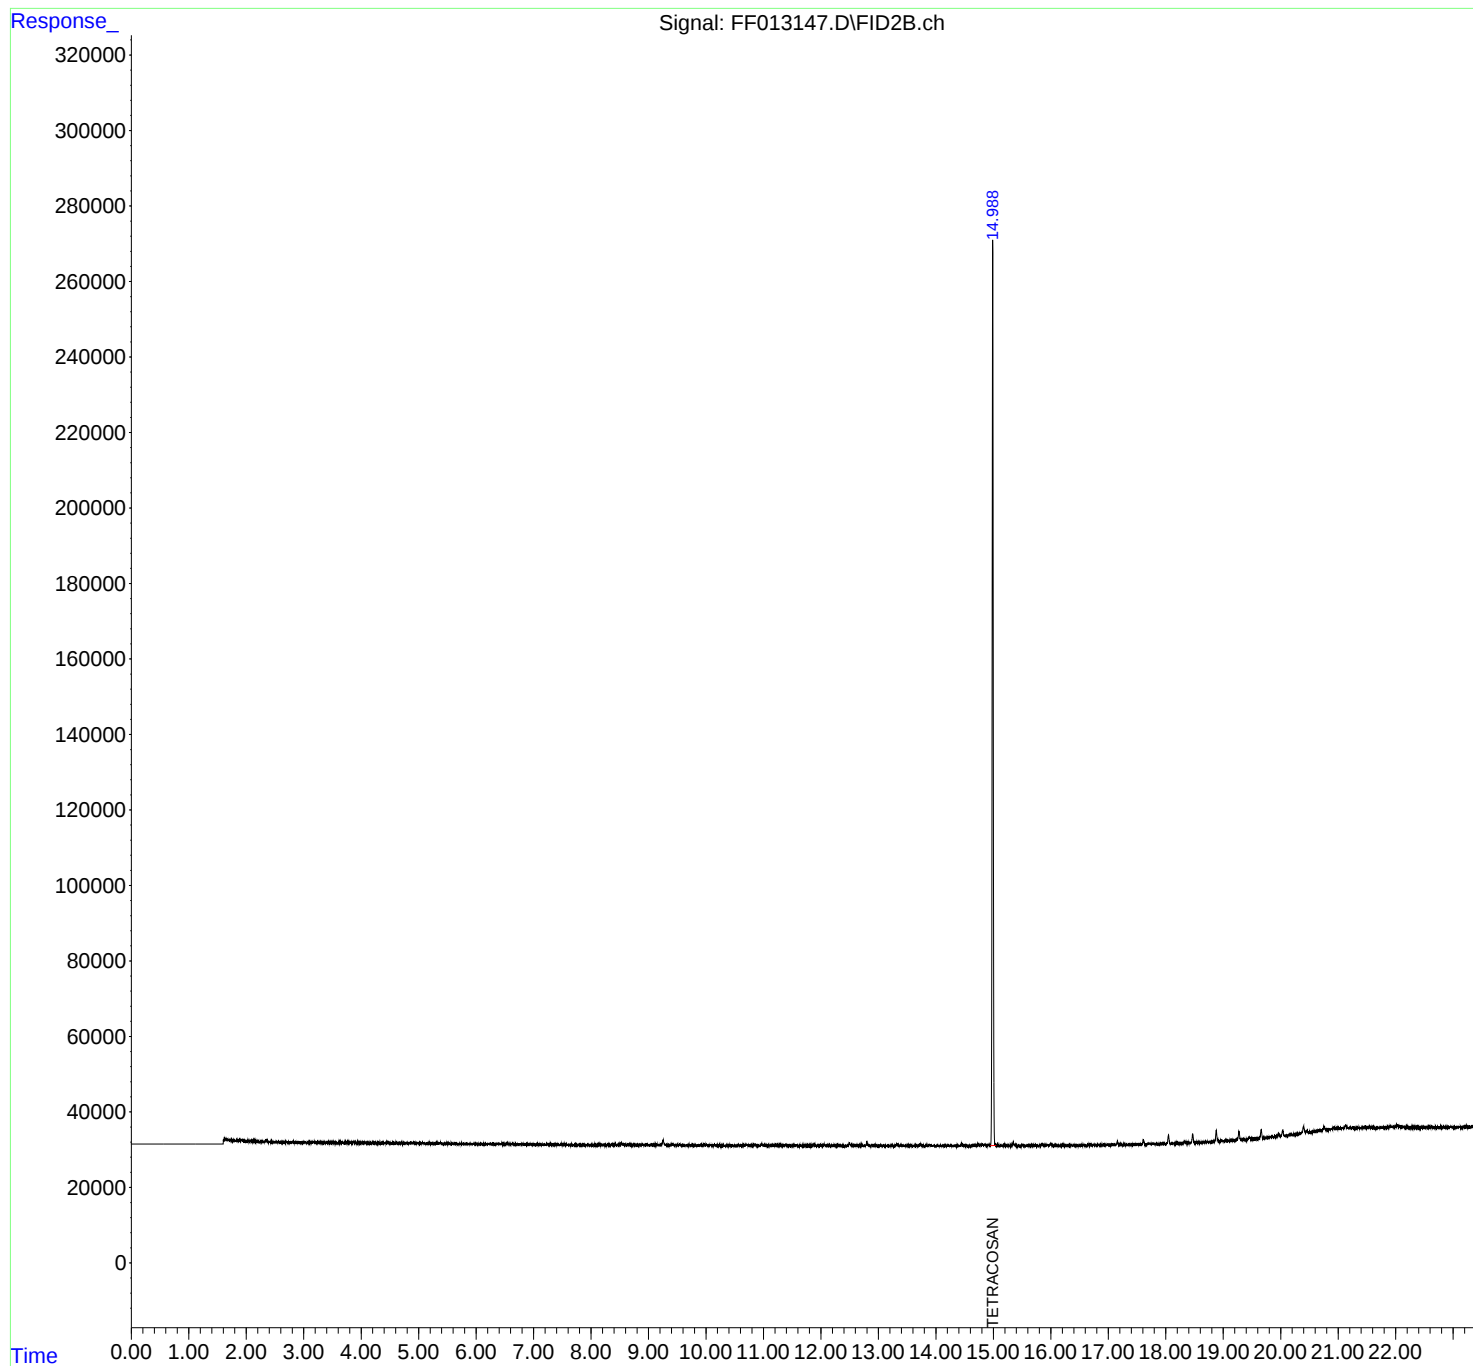

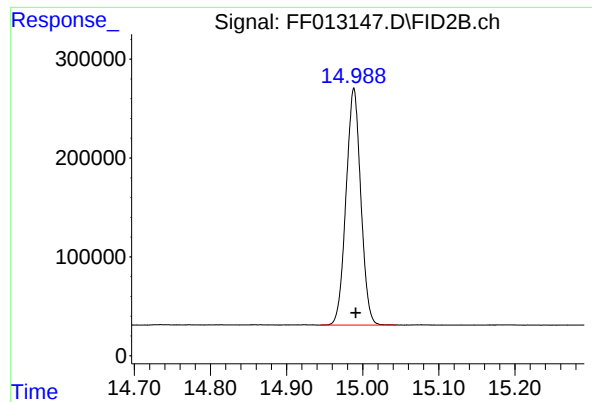

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.988 min
Delta R.T.: -0.002 min
Response: 3221989
Conc: 29.89 ug/ml

Instrument :
FID_F
ClientSampleId :
PB154660BL