

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080918\
 Data File : FF001764.D
 Signal(s) : FID2B.ch
 Acq On : 09 Aug 2018 19:22
 Operator : AJ\SJ
 Sample : J4275-01MSD
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 10 01:15:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.320	2234649	17.693 ug/mlm
Target Compounds			
2) N-DECANE	4.105	2071464	14.204 ug/ml
3) N-DODECANE	6.112	2272080	15.242 ug/ml
4) N-TETRADECANE	7.896	2449878	16.255 ug/ml
5) N-HEXADECANE	9.489	2476959	16.546 ug/ml
6) N-OCTADECANE	10.924	2543596	16.876 ug/ml
7) N-EICOSANE	12.229	2480623	16.643 ug/ml
8) N-DOCOSANE	13.423	2474846	16.943 ug/ml
10) N-TETRACOSANE	14.522	2631888	18.450 ug/ml
11) N-HEXACOSANE	15.540	2399336	17.033 ug/ml
12) N-OCTACOSANE	16.489	2286243	16.305 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080918\
Data File : FF001764.D
Signal(s) : FID2B.ch
Acq On : 09 Aug 2018 19:22
Operator : AJ\SJ
Sample : J4275-01MSD
Misc :
ALS Vial : 68 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 10 01:15:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

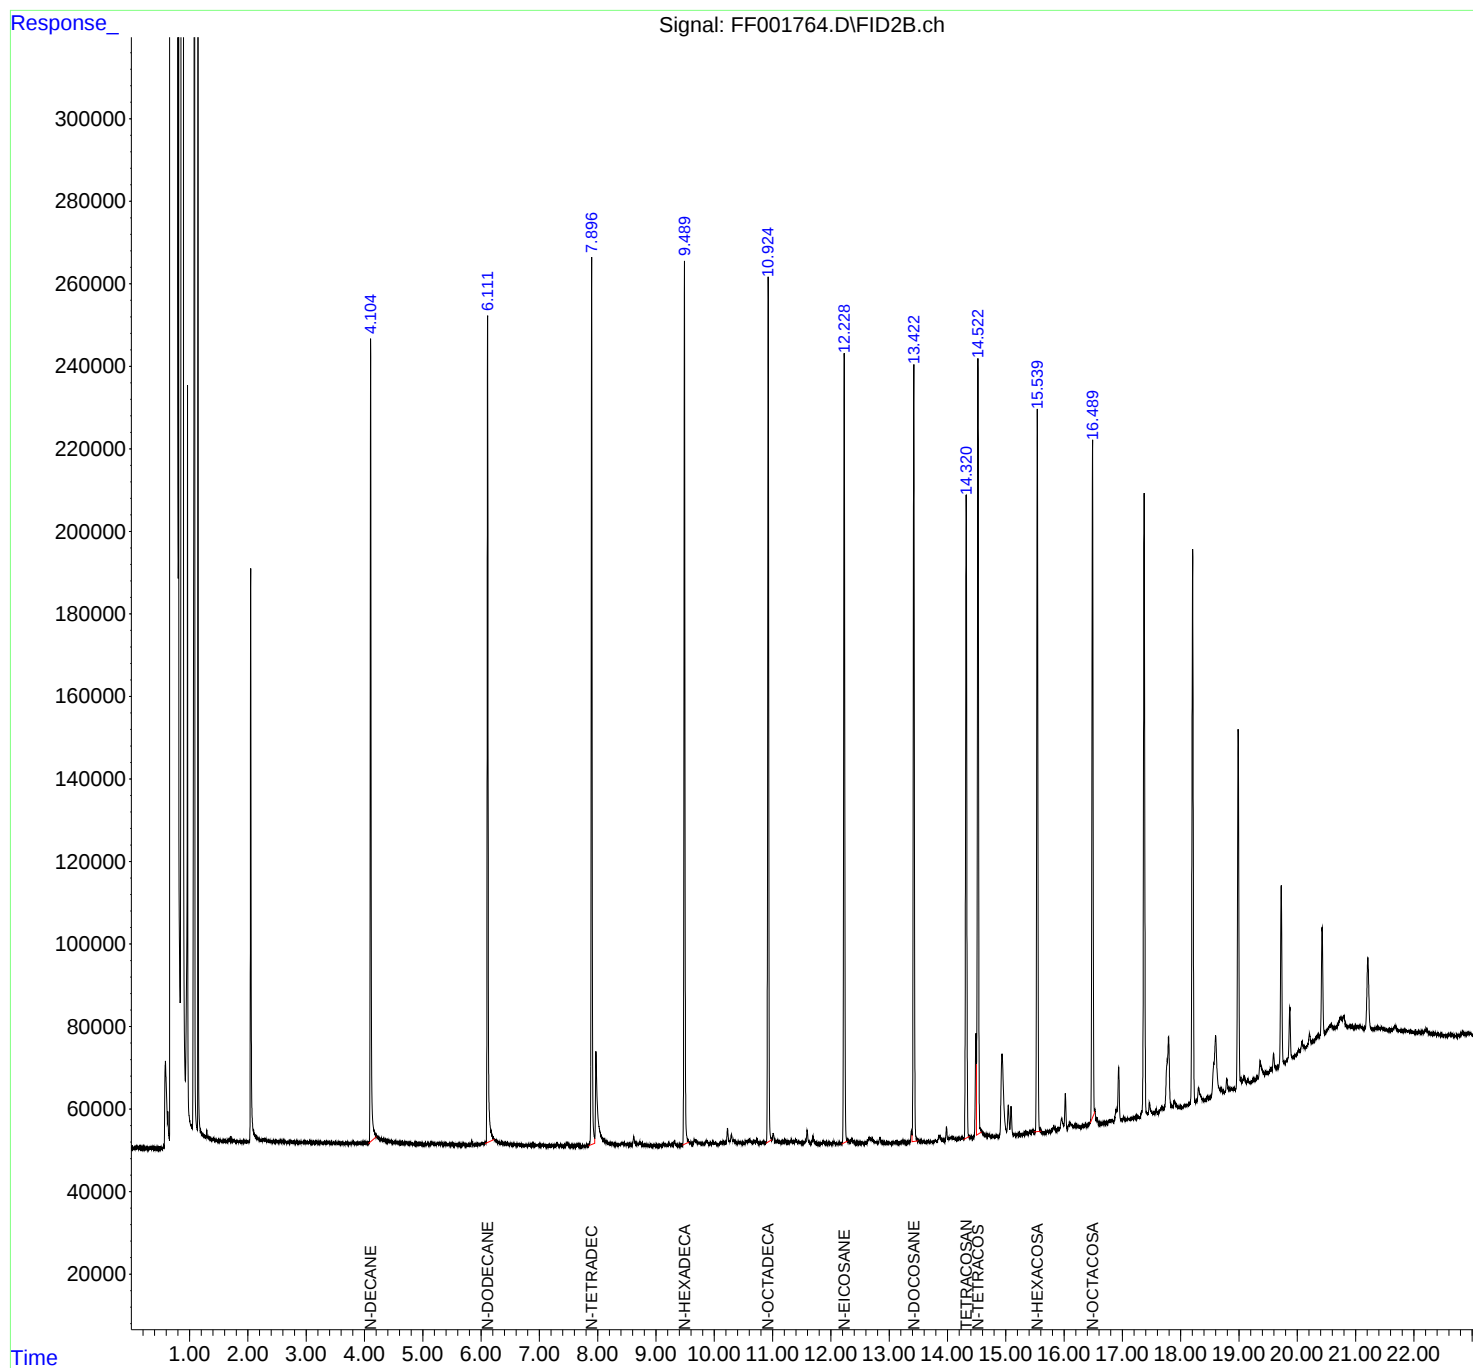

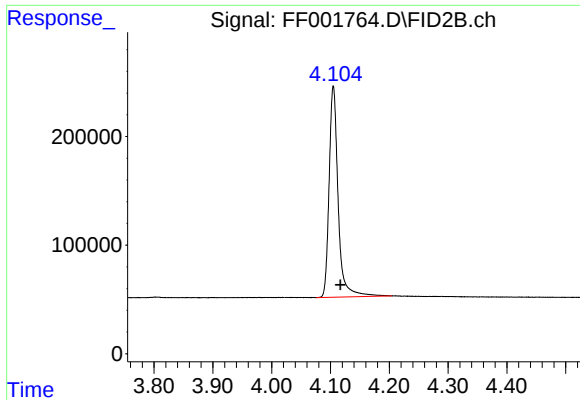


#2 N-DECANE

R.T.: 4.105 min
Delta R.T.: -0.012 min
Response: 2071464
Conc: 14.20 ug/ml

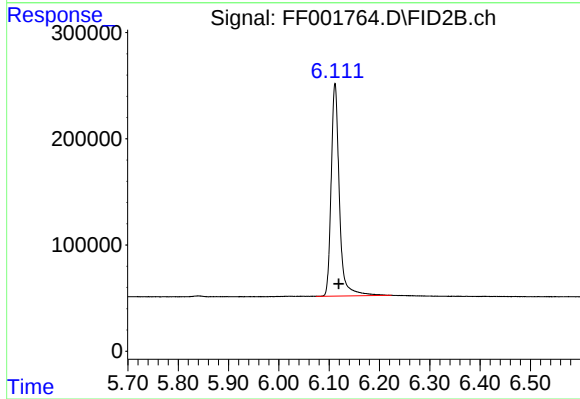


#3 N-DODECANE

R.T.: 6.112 min
Delta R.T.: -0.007 min
Response: 2272080
Conc: 15.24 ug/ml

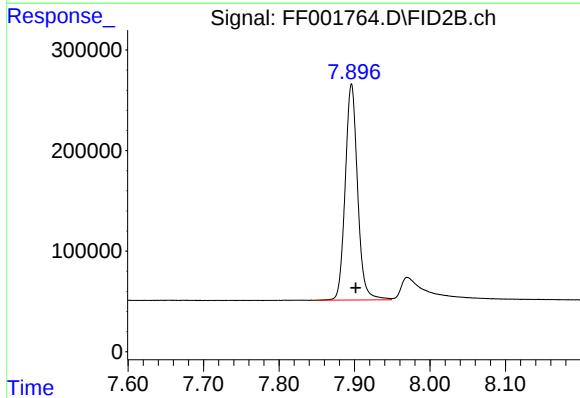


#4 N-TETRADECANE

R.T.: 7.896 min
Delta R.T.: -0.006 min
Response: 2449878
Conc: 16.25 ug/ml

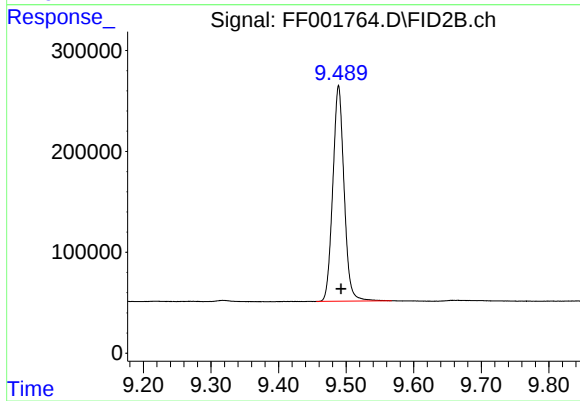


#5 N-HEXADECANE

R.T.: 9.489 min
Delta R.T.: -0.004 min
Response: 2476959
Conc: 16.55 ug/ml

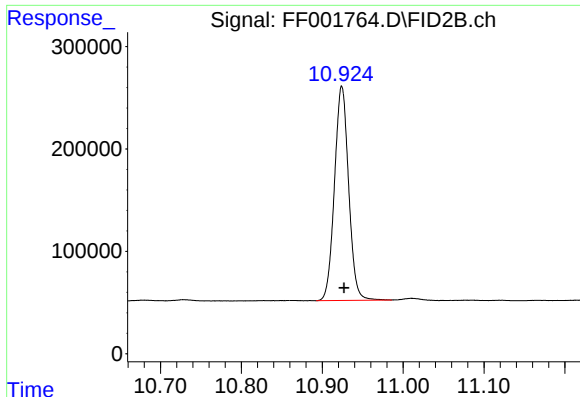


#6 N-OCTADECANE

R.T.: 10.924 min
Delta R.T.: -0.003 min
Response: 2543596
Conc: 16.88 ug/ml

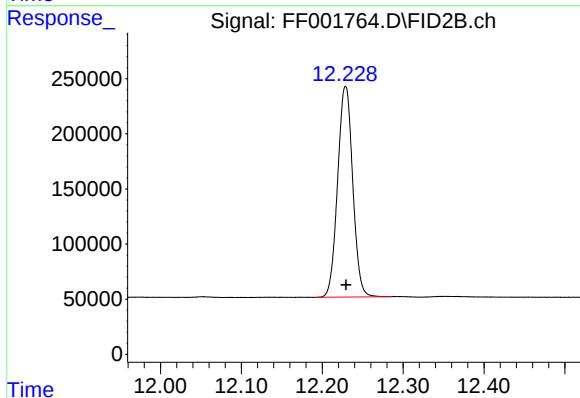


#7 N-EICOSANE

R.T.: 12.229 min
Delta R.T.: 0.000 min
Response: 2480623
Conc: 16.64 ug/ml

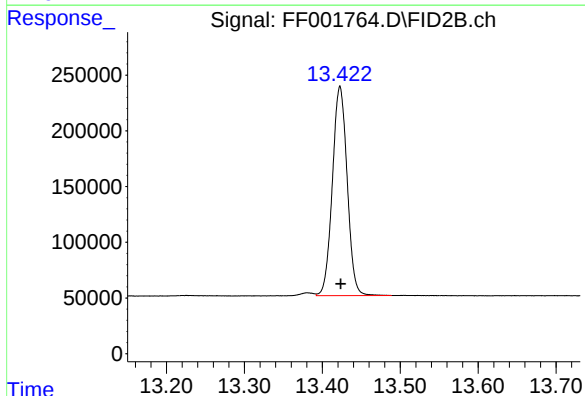


#8 N-DOCOSANE

R.T.: 13.423 min
Delta R.T.: 0.000 min
Response: 2474846
Conc: 16.94 ug/ml

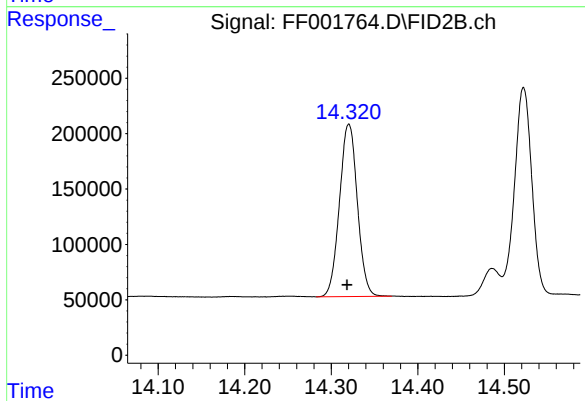


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.320 min
Delta R.T.: 0.002 min
Response: 2234649
Conc: 17.69 ug/ml m

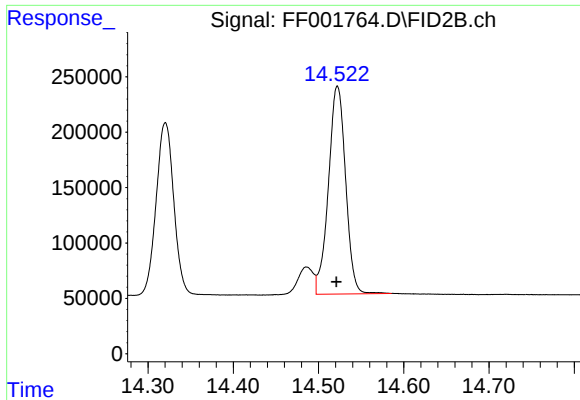


#10 N-TETRACOSANE

R.T.: 14.522 min
Delta R.T.: 0.001 min
Response: 2631888
Conc: 18.45 ug/ml

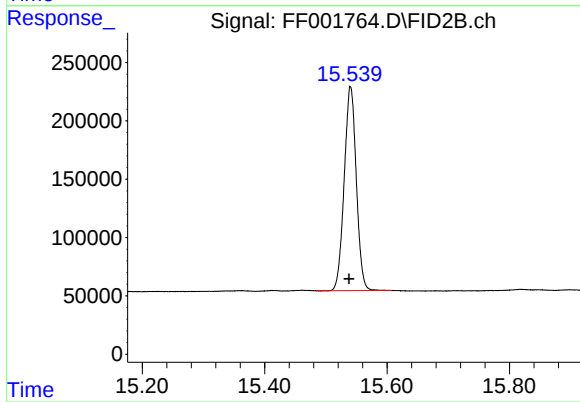

#11 N-HEXACOSANE

R.T.: 15.540 min
Delta R.T.: 0.003 min
Response: 2399336
Conc: 17.03 ug/ml

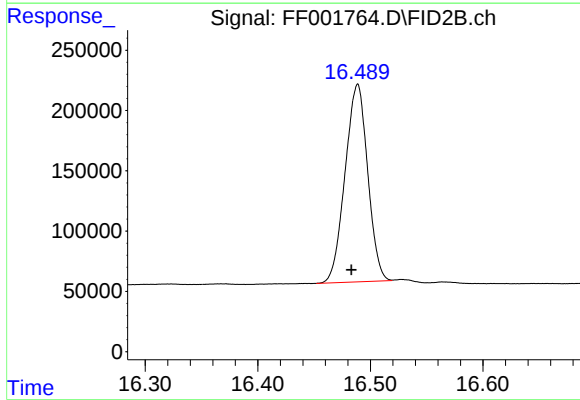

#12 N-OCTACOSANE

R.T.: 16.489 min
Delta R.T.: 0.005 min
Response: 2286243
Conc: 16.30 ug/ml m