

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080918\
 Data File : FF001776.D
 Signal(s) : FID2B.ch
 Acq On : 10 Aug 2018 01:33
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 10 08:51:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
 Quant Title :
 QLast Update : Fri Aug 03 12:00:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.325	5370640	42.522 ug/mlm
Target Compounds			
2) N-DECANE	4.106	6692057	45.888 ug/ml
3) N-DODECANE	6.115	6815181	45.720 ug/ml
4) N-TETRADECANE	7.900	6814199	45.211 ug/ml
5) N-HEXADECANE	9.493	6741027	45.029 ug/ml
6) N-OCTADECANE	10.928	6632844	44.006 ug/ml
7) N-EICOSANE	12.234	6410384	43.010 ug/ml
8) N-DOCOSANE	13.428	6186830	42.356 ug/ml
10) N-TETRACOSANE	14.529	6057504	42.463 ug/ml
11) N-HEXACOSANE	15.547	5803389	41.199 ug/ml
12) N-OCTACOSANE	16.495	5703087	40.673 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080918\
Data File : FF001776.D
Signal(s) : FID2B.ch
Acq On : 10 Aug 2018 01:33
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 10 08:51:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF073018.M
Quant Title :
QLast Update : Fri Aug 03 12:00:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

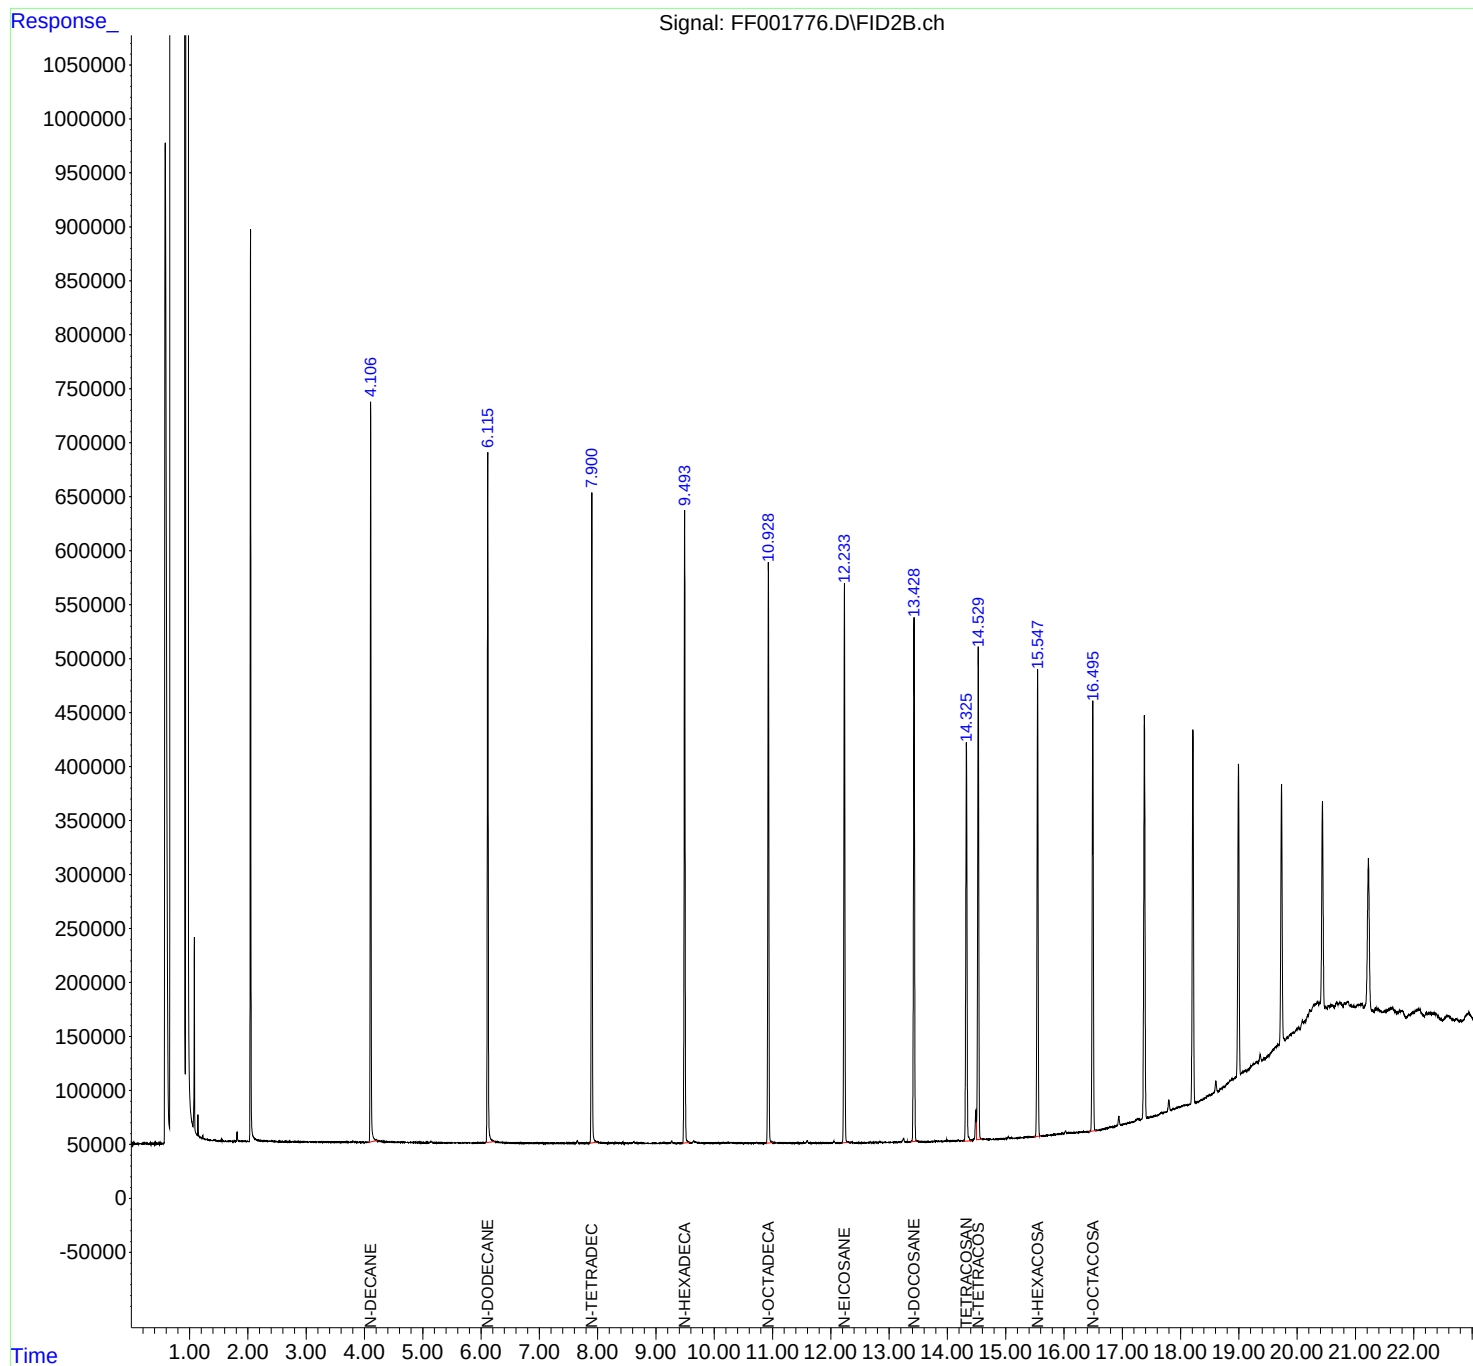

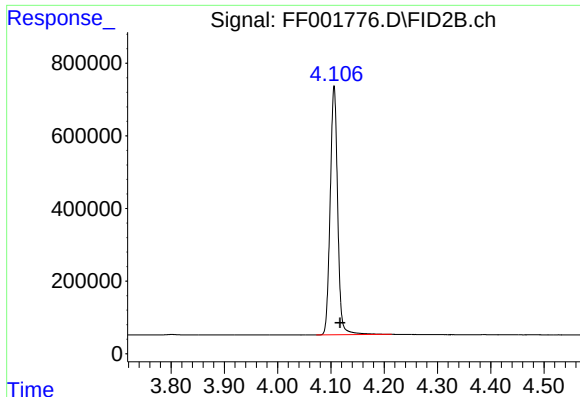


#2 N-DECANE

R.T.: 4.106 min
Delta R.T.: -0.011 min
Response: 6692057
Conc: 45.89 ug/ml

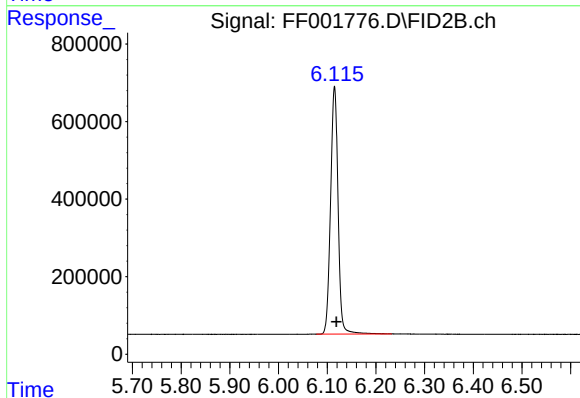


#3 N-DODECANE

R.T.: 6.115 min
Delta R.T.: -0.004 min
Response: 6815181
Conc: 45.72 ug/ml

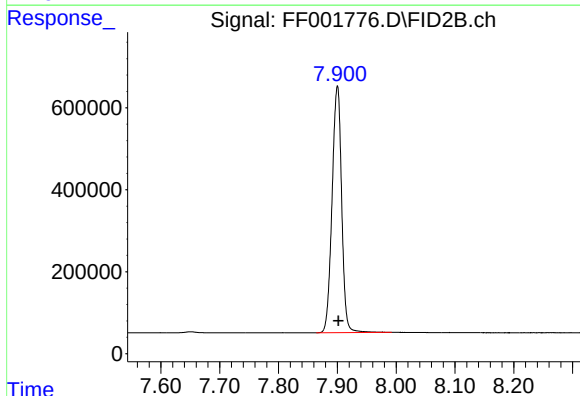


#4 N-TETRADECANE

R.T.: 7.900 min
Delta R.T.: -0.002 min
Response: 6814199
Conc: 45.21 ug/ml

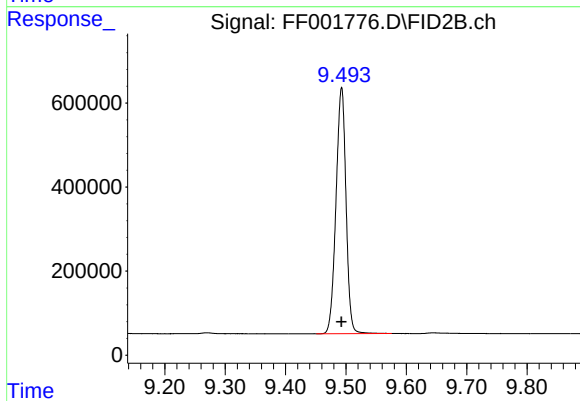


#5 N-HEXADECANE

R.T.: 9.493 min
Delta R.T.: 0.000 min
Response: 6741027
Conc: 45.03 ug/ml

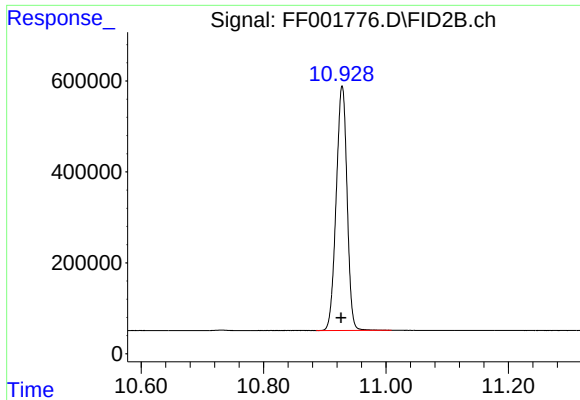


#6 N-OCTADECANE

R.T.: 10.928 min
Delta R.T.: 0.002 min
Response: 6632844
Conc: 44.01 ug/ml

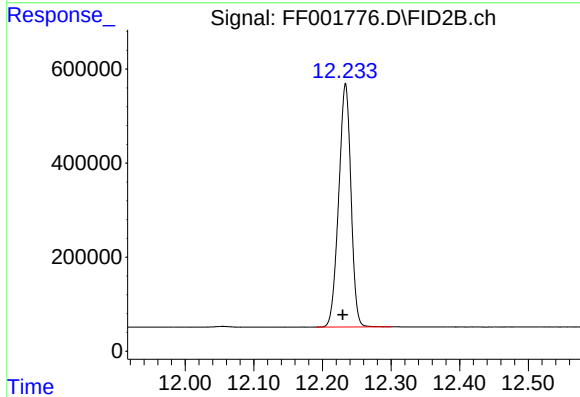


#7 N-EICOSANE

R.T.: 12.234 min
Delta R.T.: 0.004 min
Response: 6410384
Conc: 43.01 ug/ml

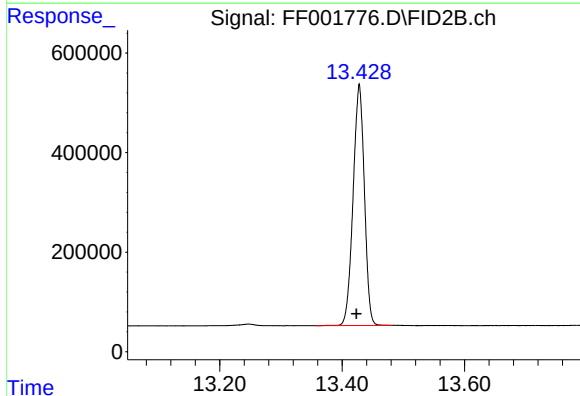


#8 N-DOCOSANE

R.T.: 13.428 min
Delta R.T.: 0.005 min
Response: 6186830
Conc: 42.36 ug/ml

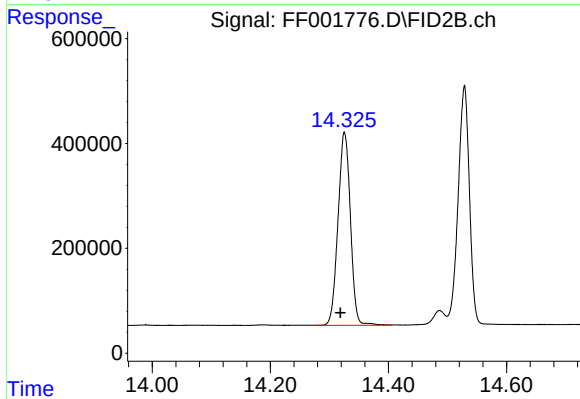


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.325 min
Delta R.T.: 0.007 min
Response: 5370640
Conc: 42.52 ug/ml m

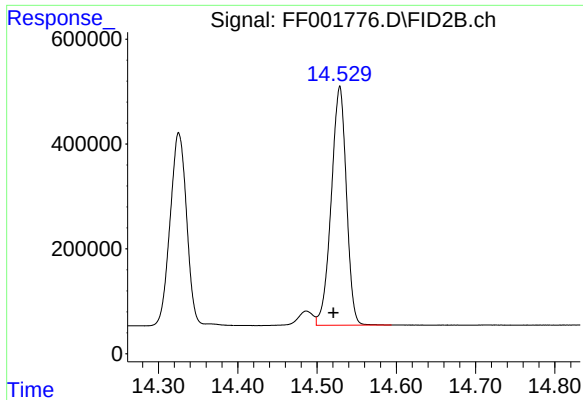


#10 N-TETRACOSANE

R.T.: 14.529 min
Delta R.T.: 0.008 min
Response: 6057504
Conc: 42.46 ug/ml

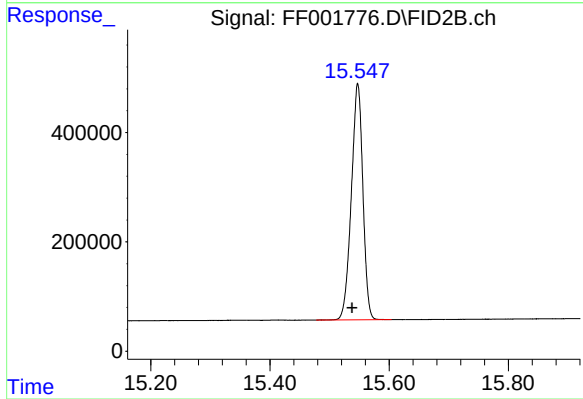

#11 N-HEXACOSANE

R.T.: 15.547 min
Delta R.T.: 0.010 min
Response: 5803389
Conc: 41.20 ug/ml

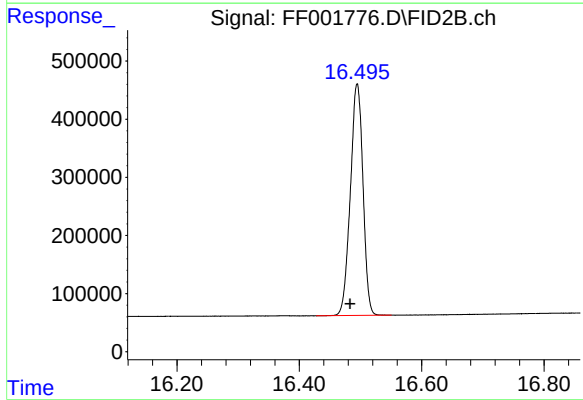

#12 N-OCTACOSANE

R.T.: 16.495 min
Delta R.T.: 0.011 min
Response: 5703087
Conc: 40.67 ug/ml