

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080922\
Data File : FF011200.D
Signal(s) : FID2B.ch
Acq On : 09 Aug 2022 10:16
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 10 01:15:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.522	2249635	17.871 ug/ml
12)	N-OCTACOSANE	16.969	2183259	18.086 ug/ml
14)	N-DOTRIACONTANE	18.684	61115	0.517 ug/ml
15)	N-TETRATRIACONTANE	19.464	51181	0.459 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080922\
Data File : FF011200.D
Signal(s) : FID2B.ch
Acq On : 09 Aug 2022 10:16
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 10 01:15:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF072822.M
Quant Title :
QLast Update : Thu Jul 28 14:46:22 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

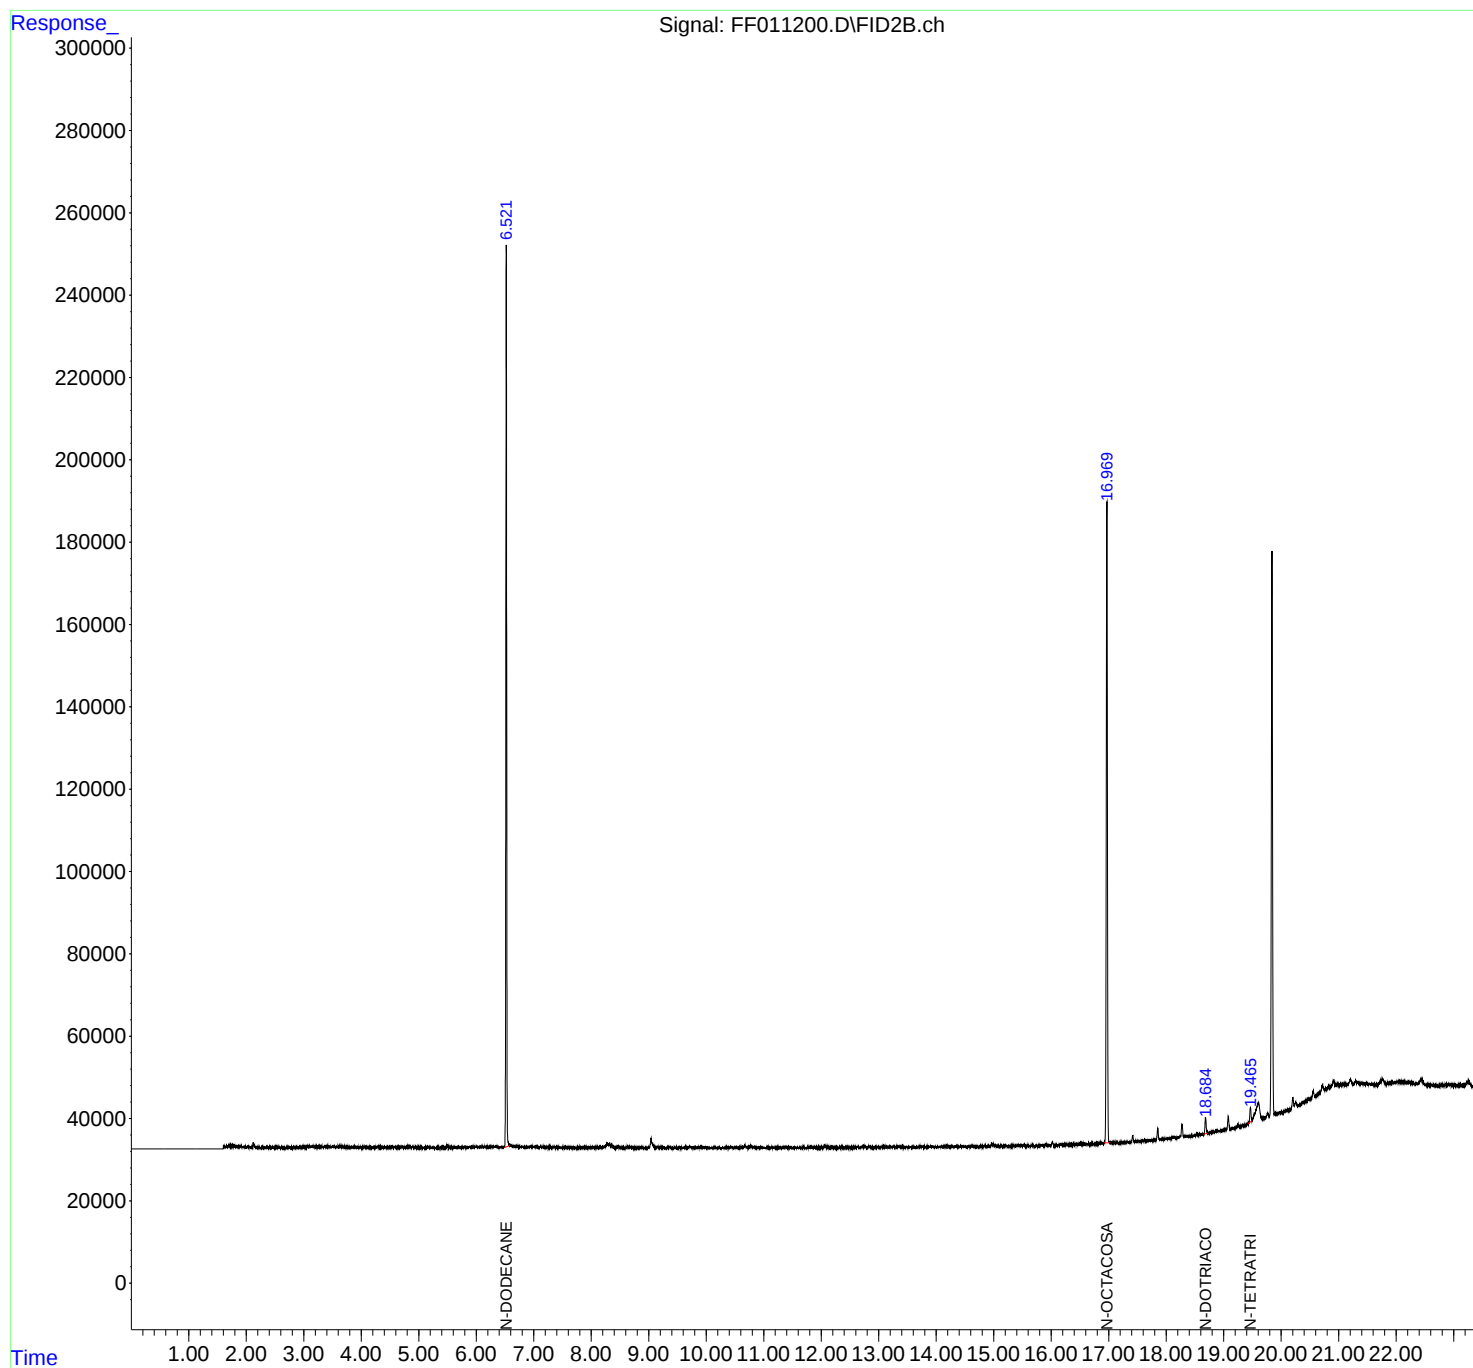

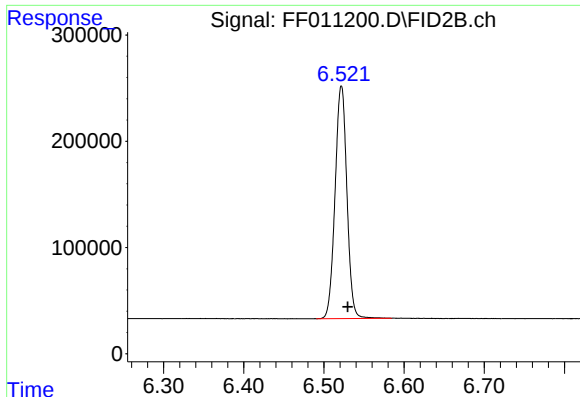


#3 N-DODECANE

R.T.: 6.522 min
Delta R.T.: -0.008 min
Response: 2249635
Conc: 17.87 ug/ml

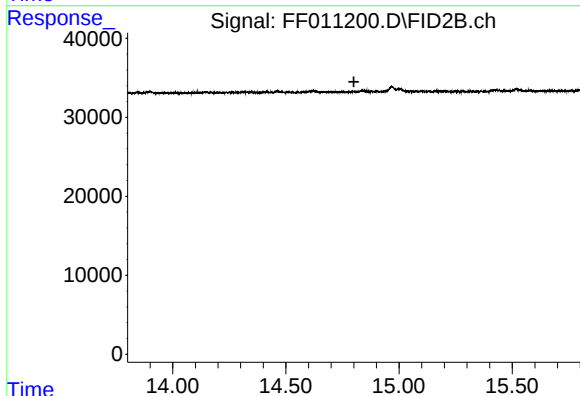


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.801 min
Response: 0
Conc: N.D.

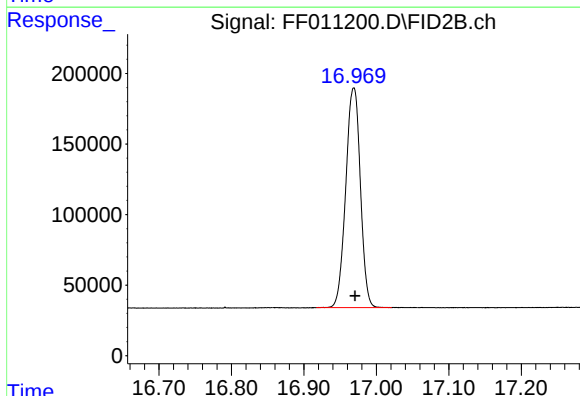


#12 N-OCTACOSANE

R.T.: 16.969 min
Delta R.T.: -0.002 min
Response: 2183259
Conc: 18.09 ug/ml

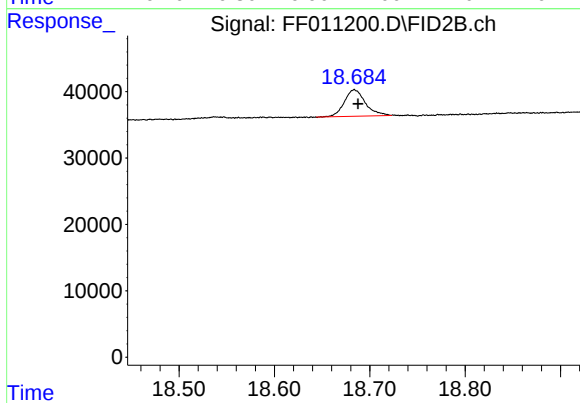

#14 N-DOTRIACONTANE

R.T.: 18.684 min
Delta R.T.: -0.004 min
Response: 61115
Conc: 0.52 ug/ml

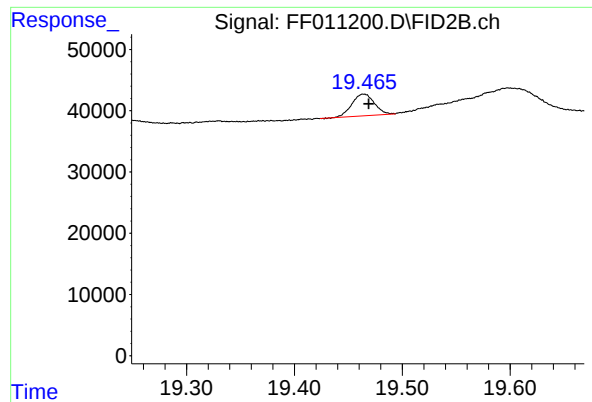

#15 N-TETRATRIACONTANE

R.T.: 19.464 min
Delta R.T.: -0.005 min
Response: 51181
Conc: 0.46 ug/ml